


Methyl Iodide

Response Ratio

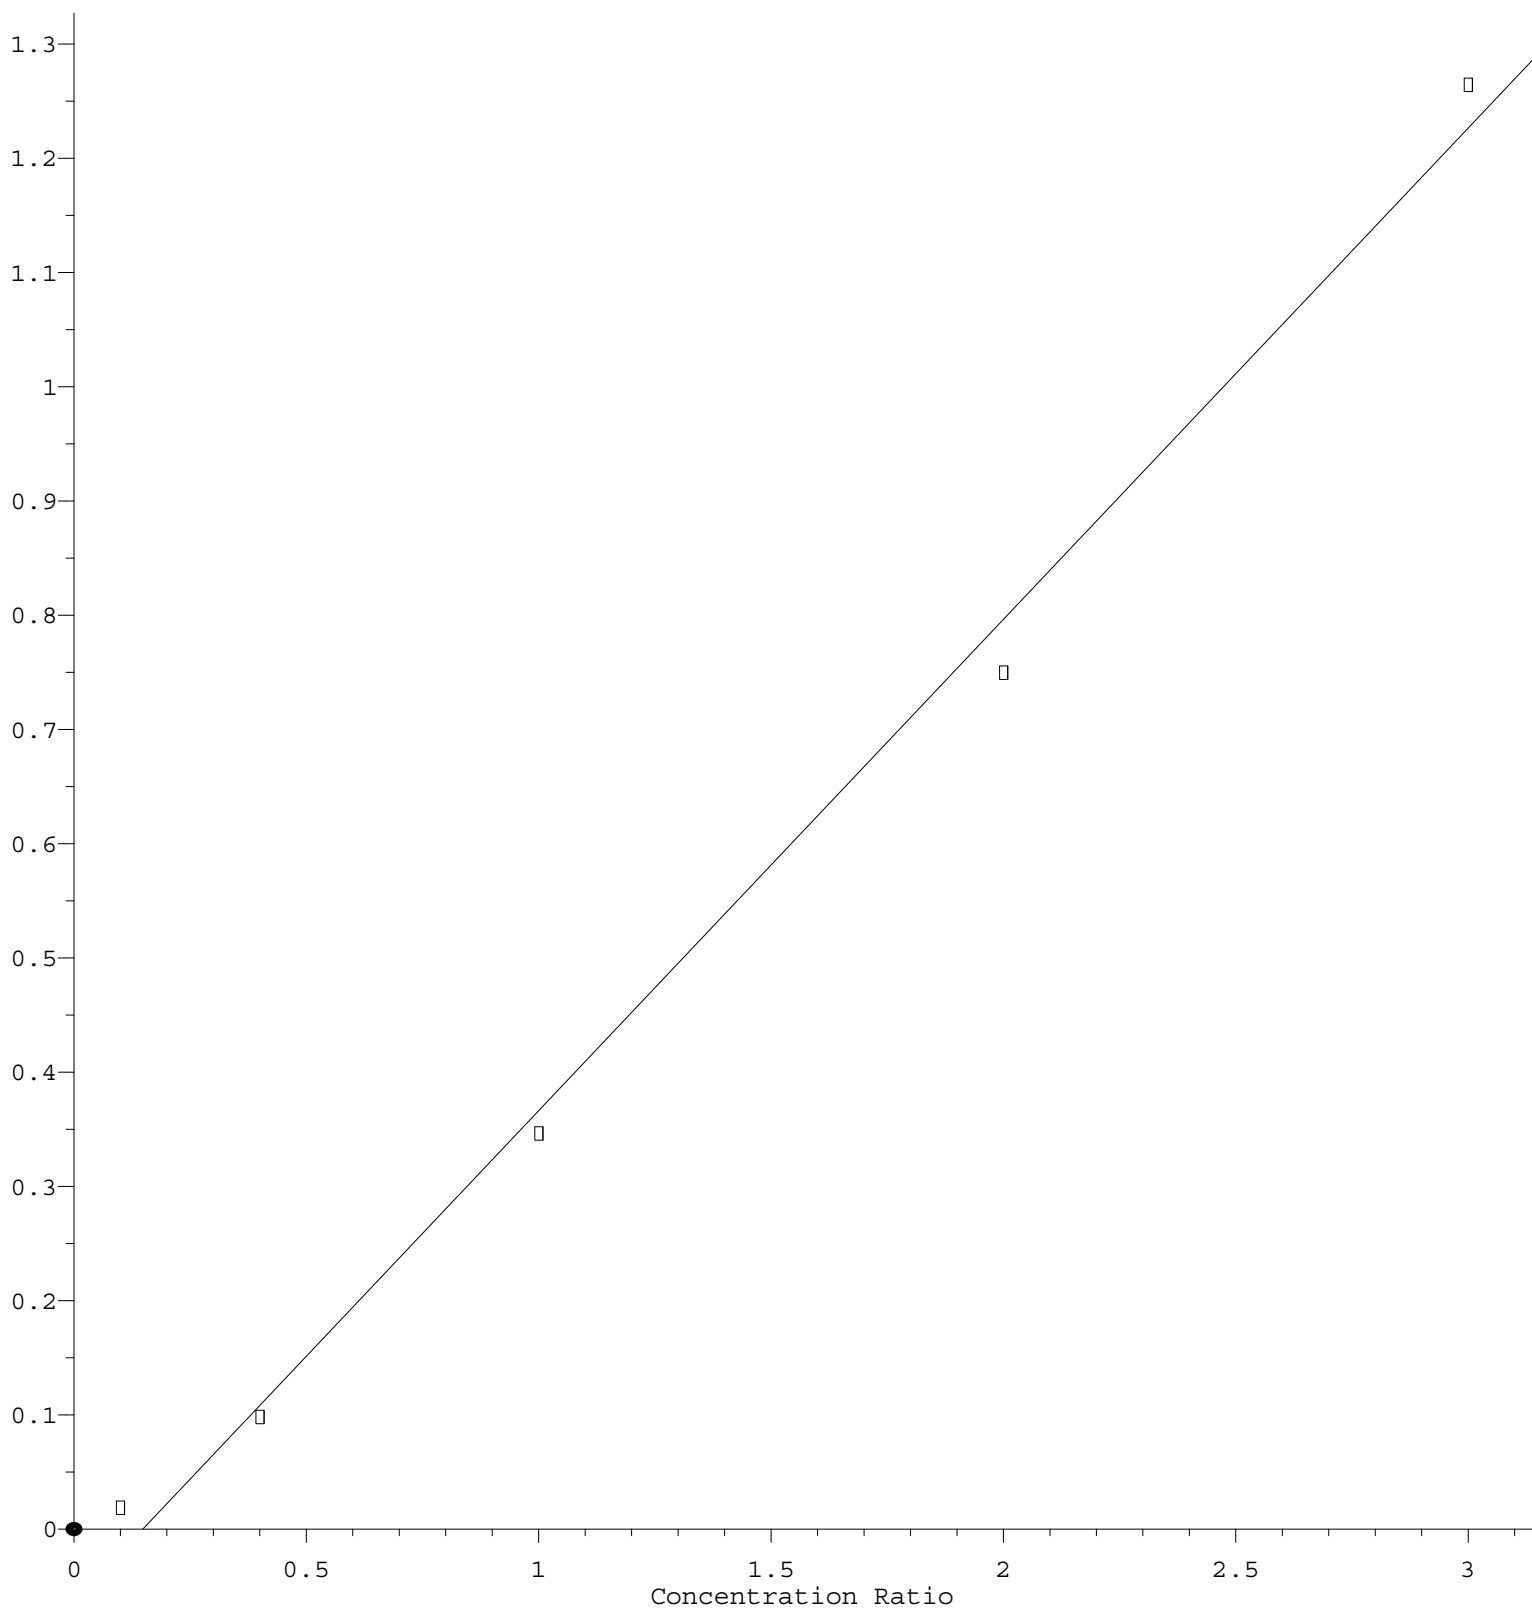

$$\text{Response} = 4.299\text{e-}001 * \text{Amt} - 6.348\text{e-}002$$


Coef of Det (r^2) = 0.994667 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U033022W.M

Calibration Table Last Updated: Thu Mar 31 11:49:29 2022

Methylene Chloride

Response Ratio

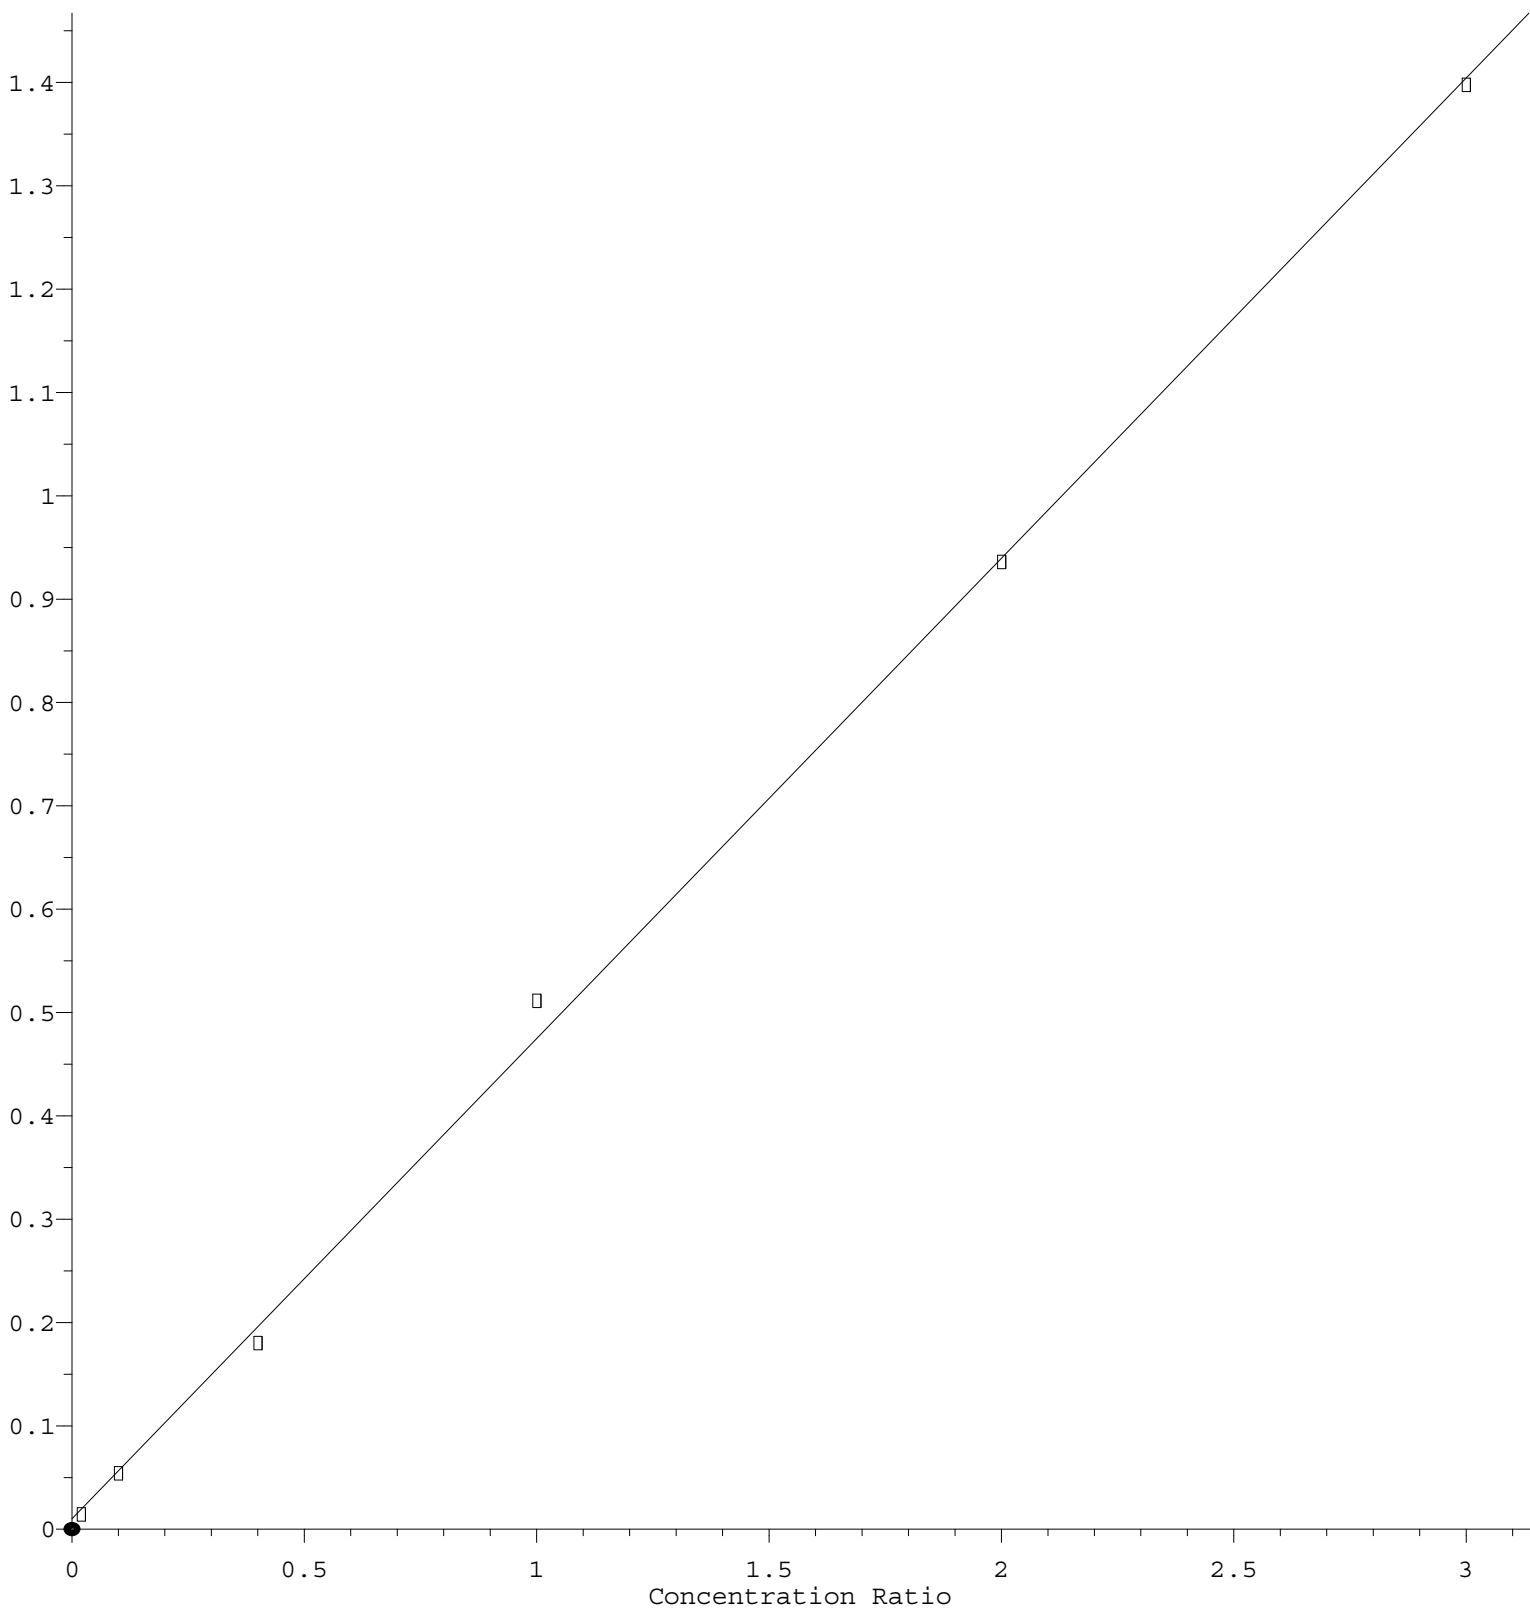

$$\text{Response} = 4.647\text{e-}001 * \text{Amt} + 1.049\text{e-}002$$


Coef of Det (r^2) = 0.998913 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U033022W.M

Calibration Table Last Updated: Thu Mar 31 11:49:29 2022

Naphthalene

Response Ratio

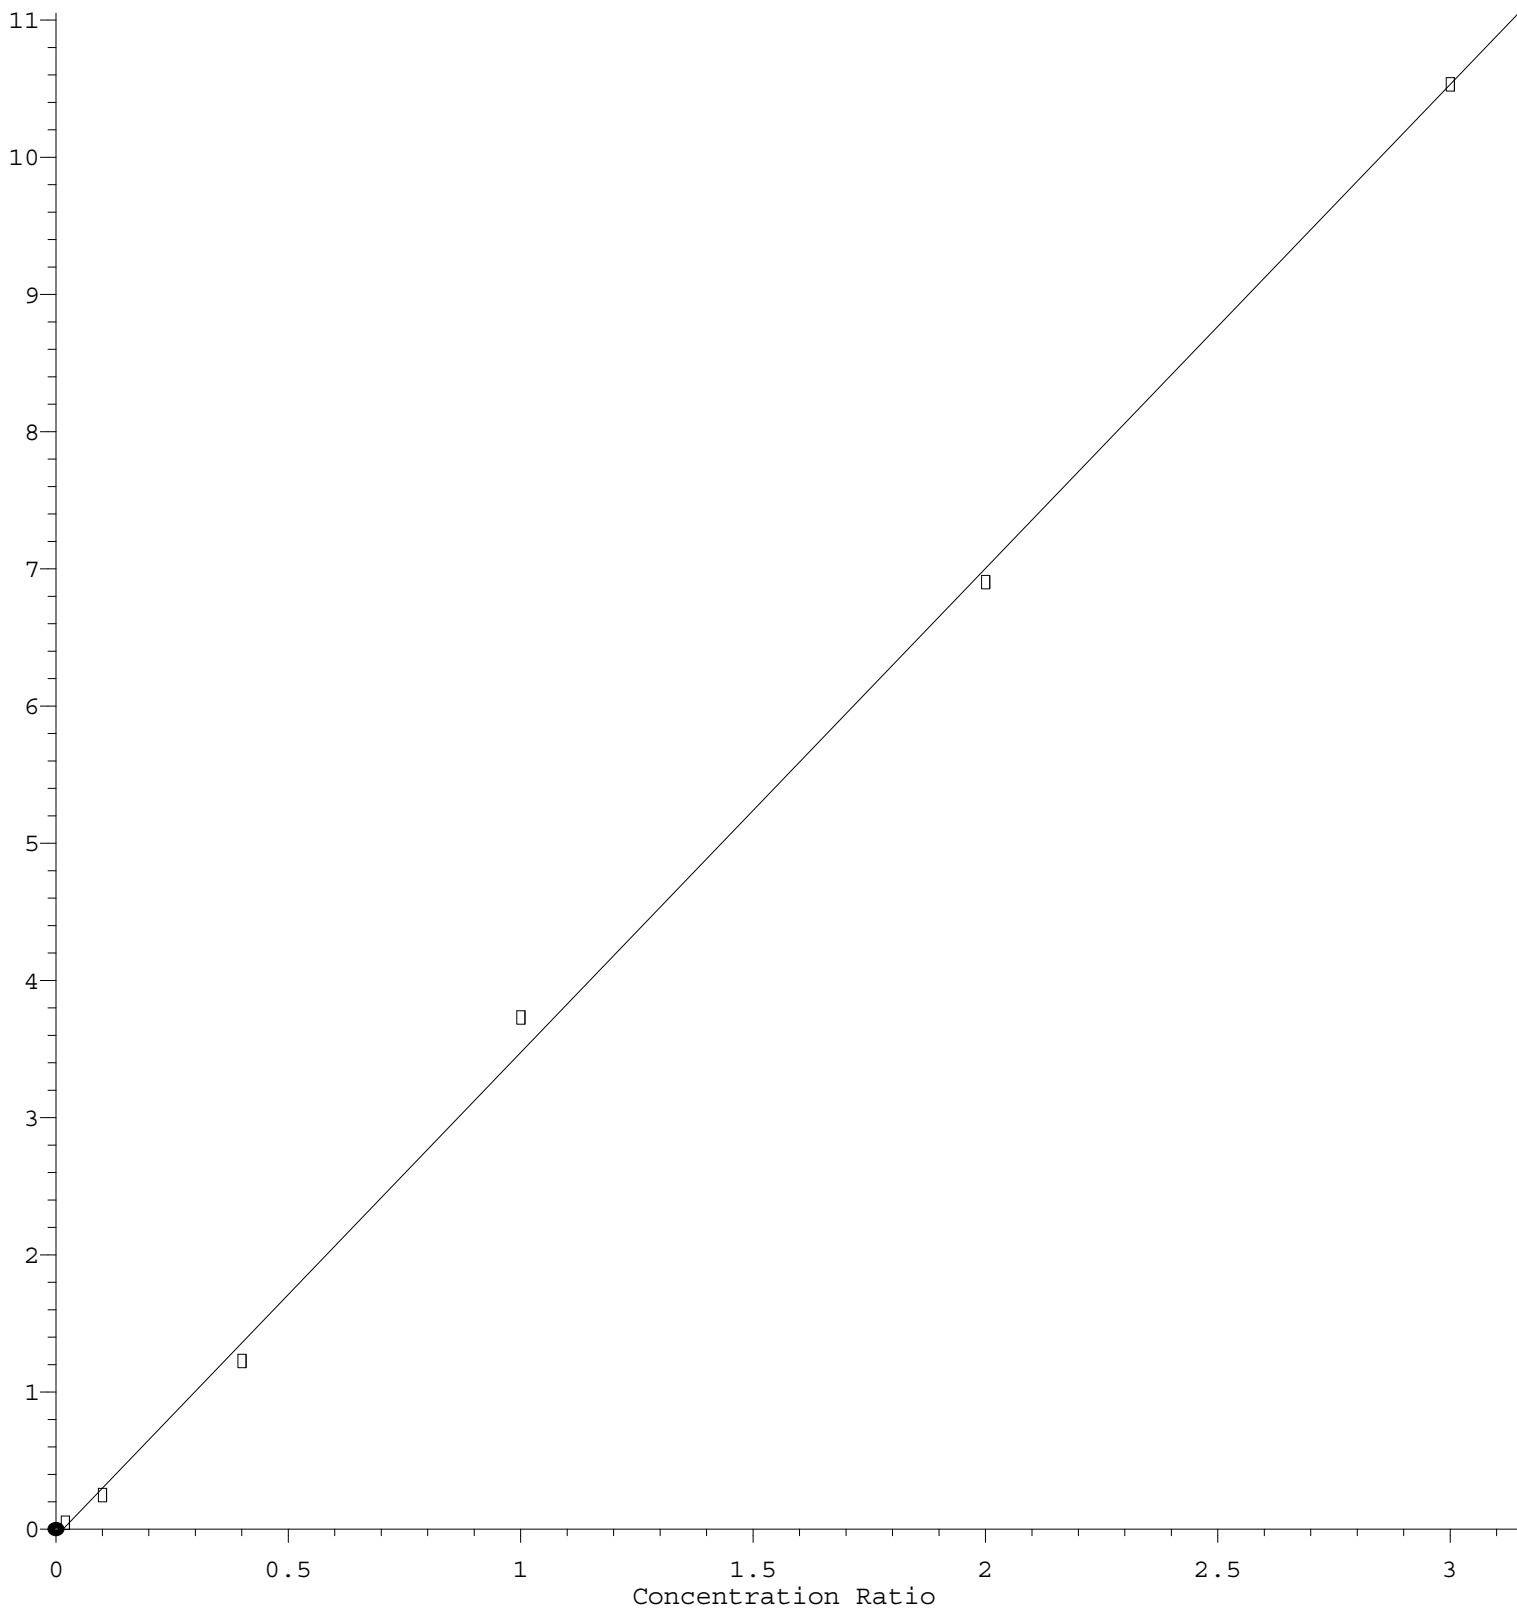


$$\text{Response} = 3.528\text{e}+000 * \text{Amt} - 5.252\text{e}-002$$

Coef of Det (r^2) = 0.998912 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U033022W.M

Calibration Table Last Updated: Thu Mar 31 11:49:29 2022


2-Chloroethyl Vinyl ether

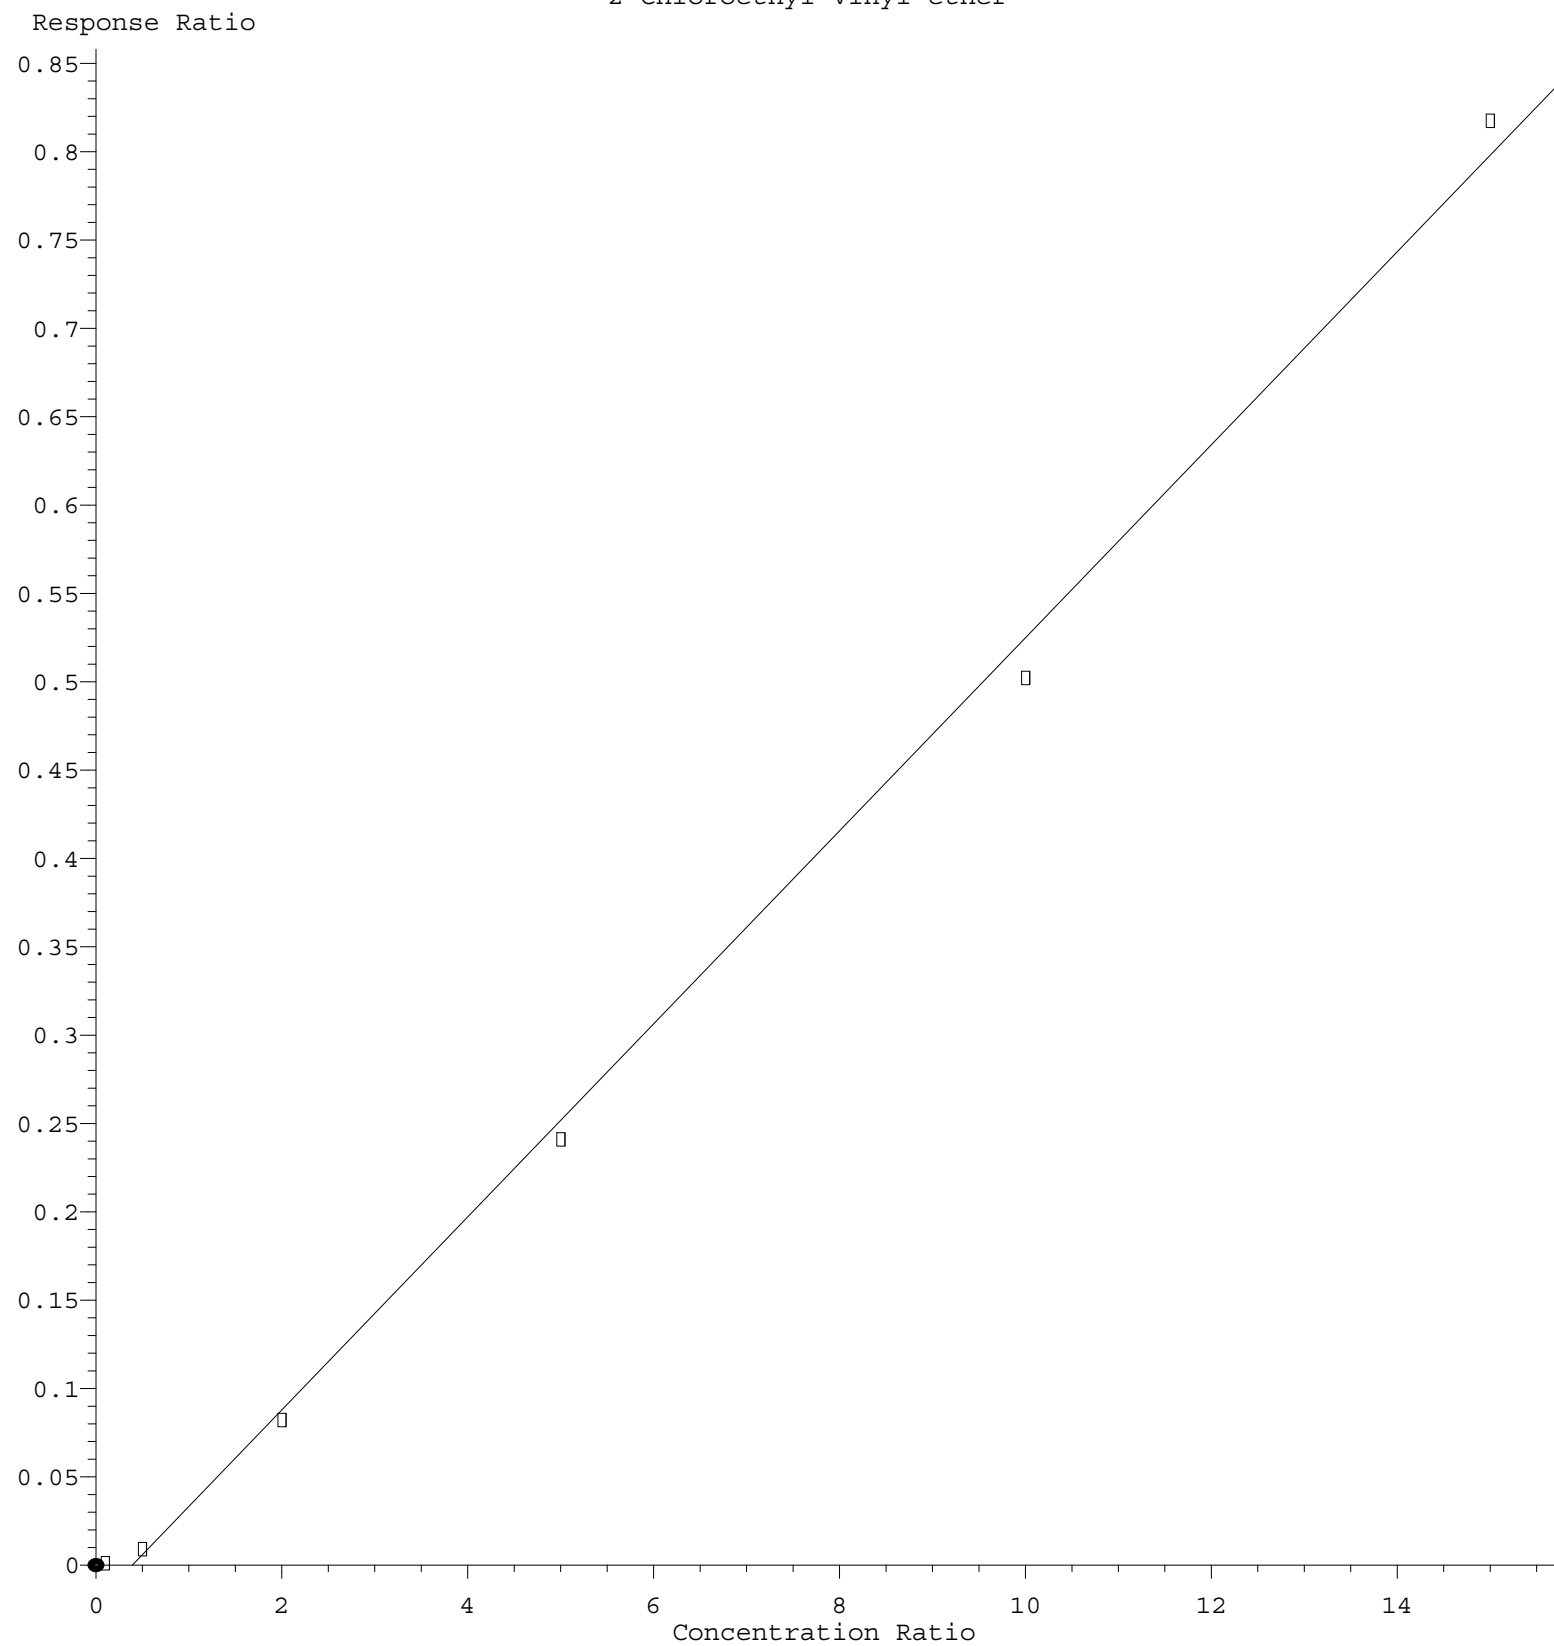

Response = $5.463 \times 10^{-2} \times \text{Amt} - 2.135 \times 10^{-2}$
Coef of Det (r^2) = 0.997461 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U033022W.M
Calibration Table Last Updated: Thu Mar 31 11:49:29 2022

Cyclohexane

Response Ratio

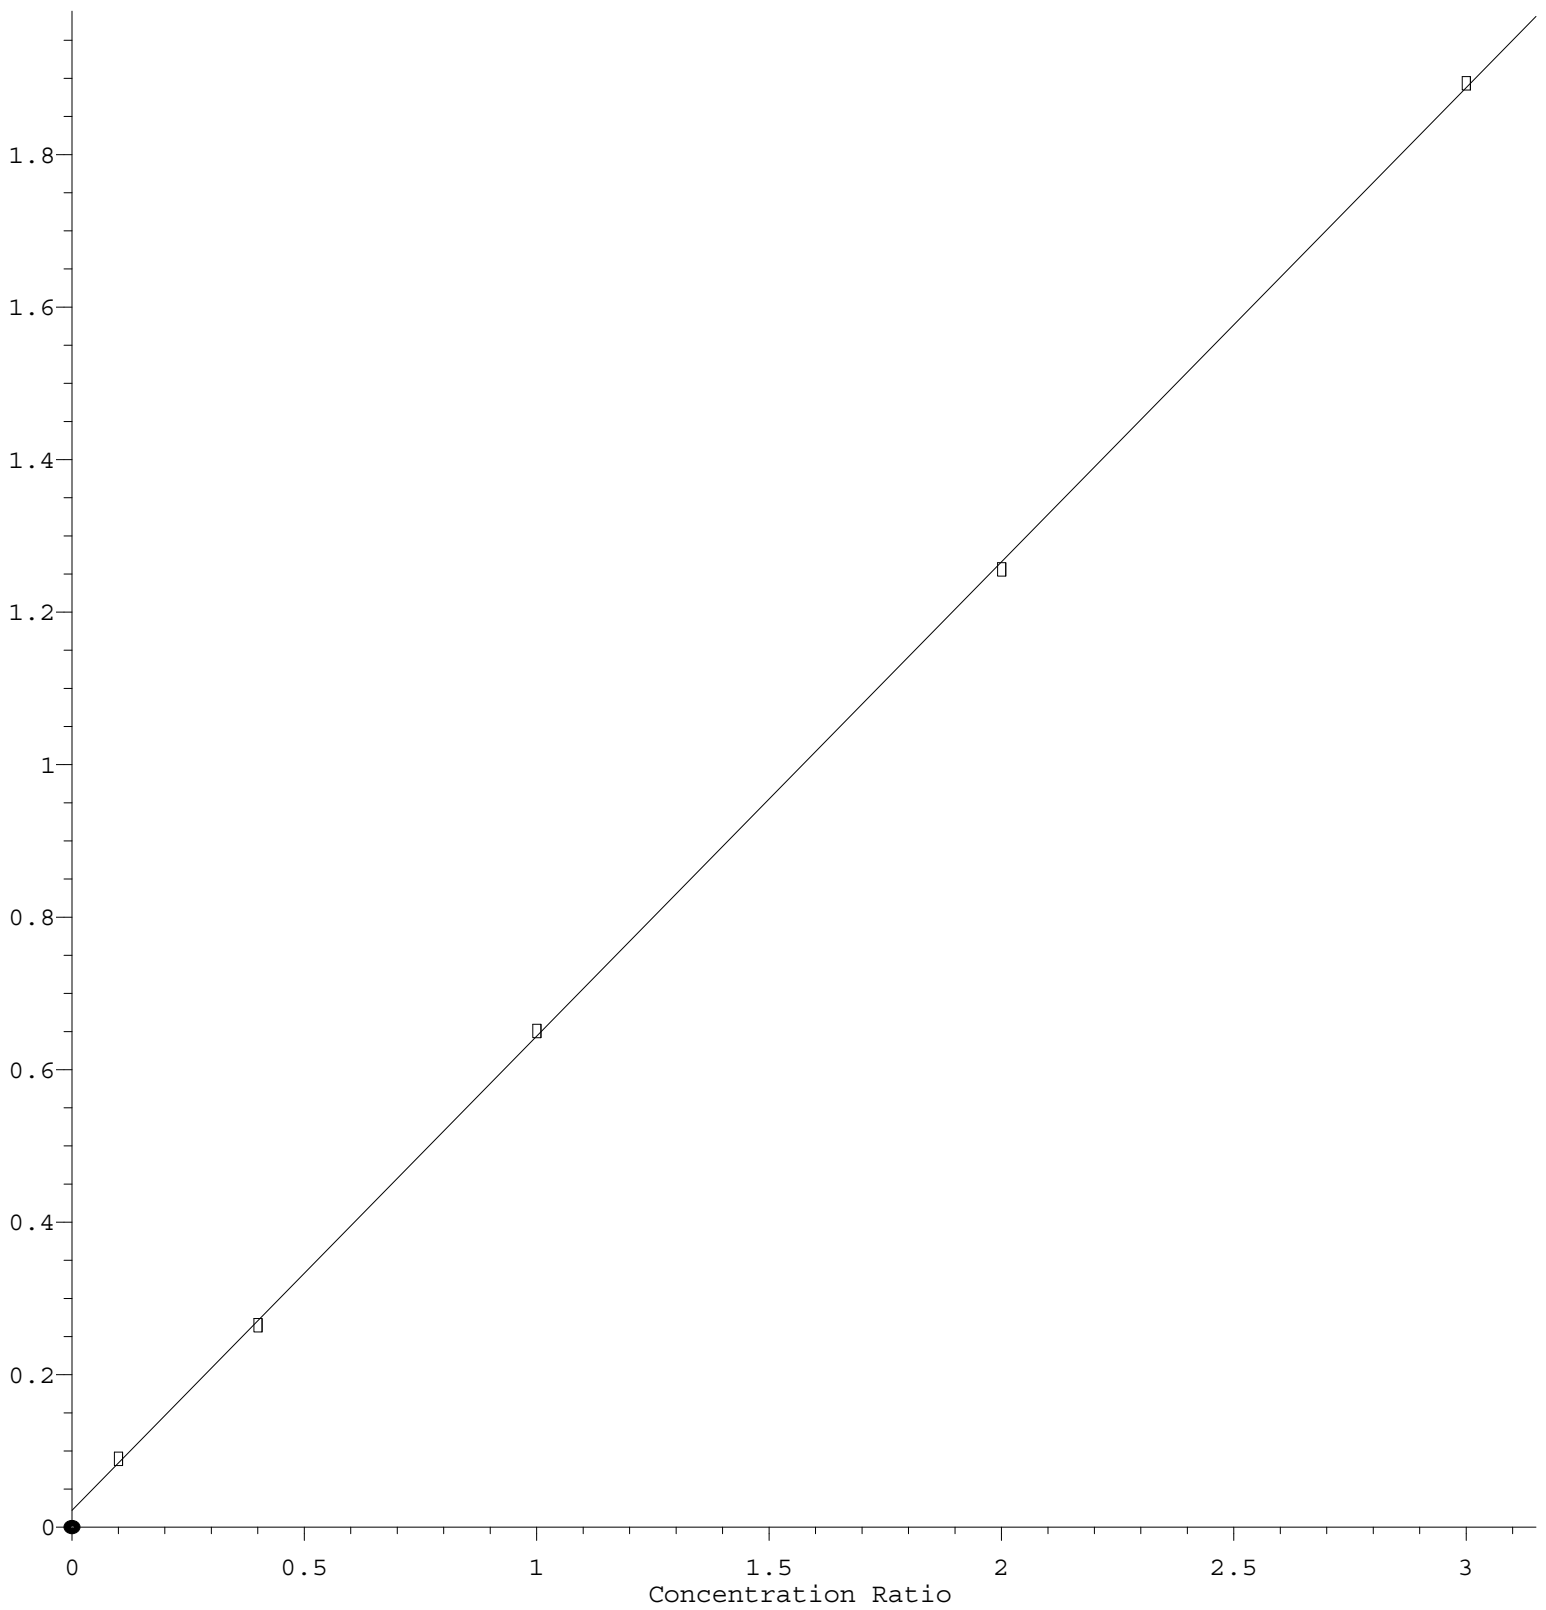

$$\text{Response} = 6.219\text{e-}001 * \text{Amt} + 2.241\text{e-}002$$


Coef of Det (r^2) = 0.999893 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U033022W.M

Calibration Table Last Updated: Thu Mar 31 11:49:29 2022

Carbon Disulfide

Response Ratio

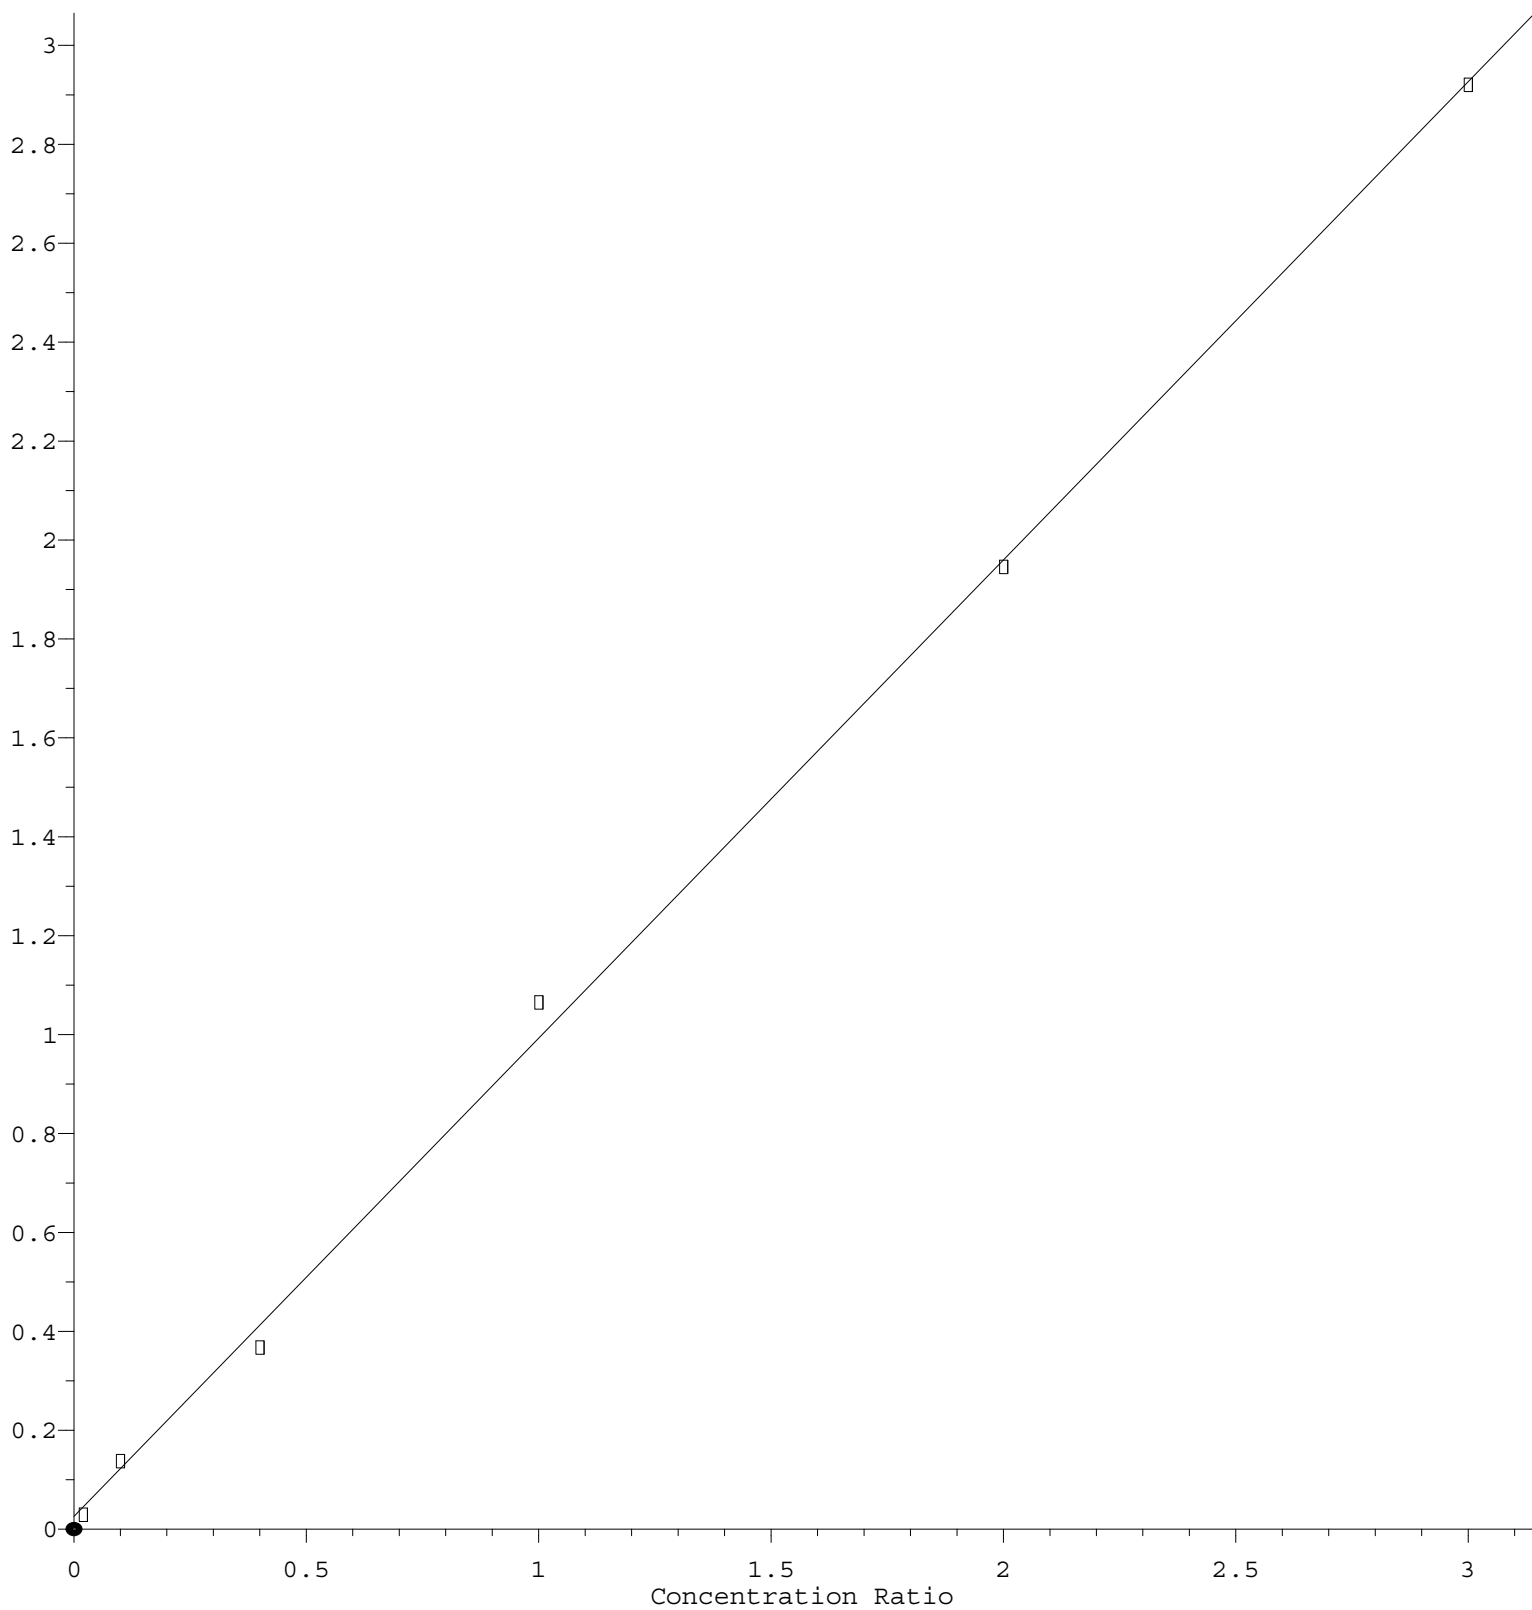

$$\text{Response} = 9.672\text{e-}001 * \text{Amt} + 2.630\text{e-}002$$

Coef of Det (r^2) = 0.998798 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U033022W.M

Calibration Table Last Updated: Thu Mar 31 11:49:29 2022