


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU033022\
 Data File : VU047757.D
 Acq On : 30 Mar 2022 08:58
 Operator : SY/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U033022W.M
 Title : SW846 8260
 Last Update : Thu Mar 31 11:49:29 2022

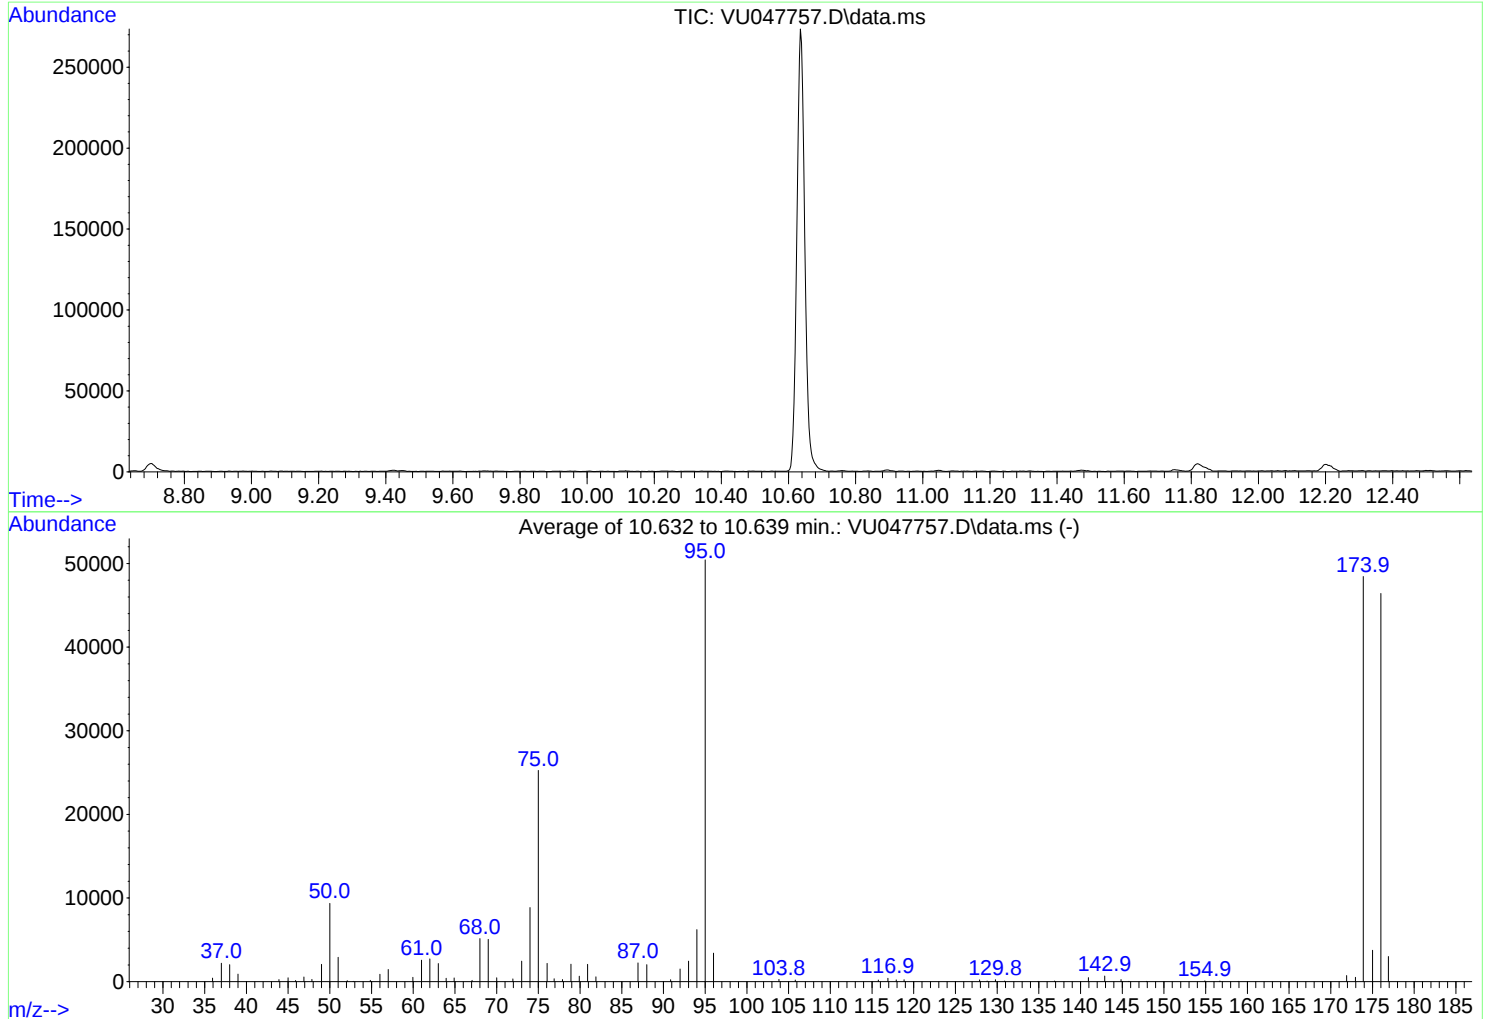

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	9359	PASS
75	95	30	60	50.1	25248	PASS
95	95	100	100	100.0	50440	PASS
96	95	5	9	6.8	3411	PASS
173	174	0.00	2	1.1	519	PASS
174	95	50	100	96.0	48443	PASS
175	174	5	9	7.8	3760	PASS
176	174	95	101	95.8	46413	PASS
177	176	5	9	6.5	3003	PASS