

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU033023\
 Data File : VU053479.D
 Acq On : 30 Mar 2023 10:53
 Operator : JC/MD
 Sample : VU0330WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0330

Quant Time: Mar 30 12:29:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U032923DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Mar 30 11:46:56 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.112	96	39852	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.632	95	12190	0.847	ug/l	0.00
Spiked Amount 1.000			Recovery	=	85.000%	
68) 1,2-Dichlorobenzene-d4	12.189	152	11161	0.773	ug/l	0.00
Spiked Amount 1.000			Recovery	=	77.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU033023\
Data File : VU053479.D
Acq On : 30 Mar 2023 10:53
Operator : JC/MD
Sample : VU0330WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0330

Quant Time: Mar 30 12:29:24 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U032923DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Mar 30 11:46:56 2023
Response via : Initial Calibration




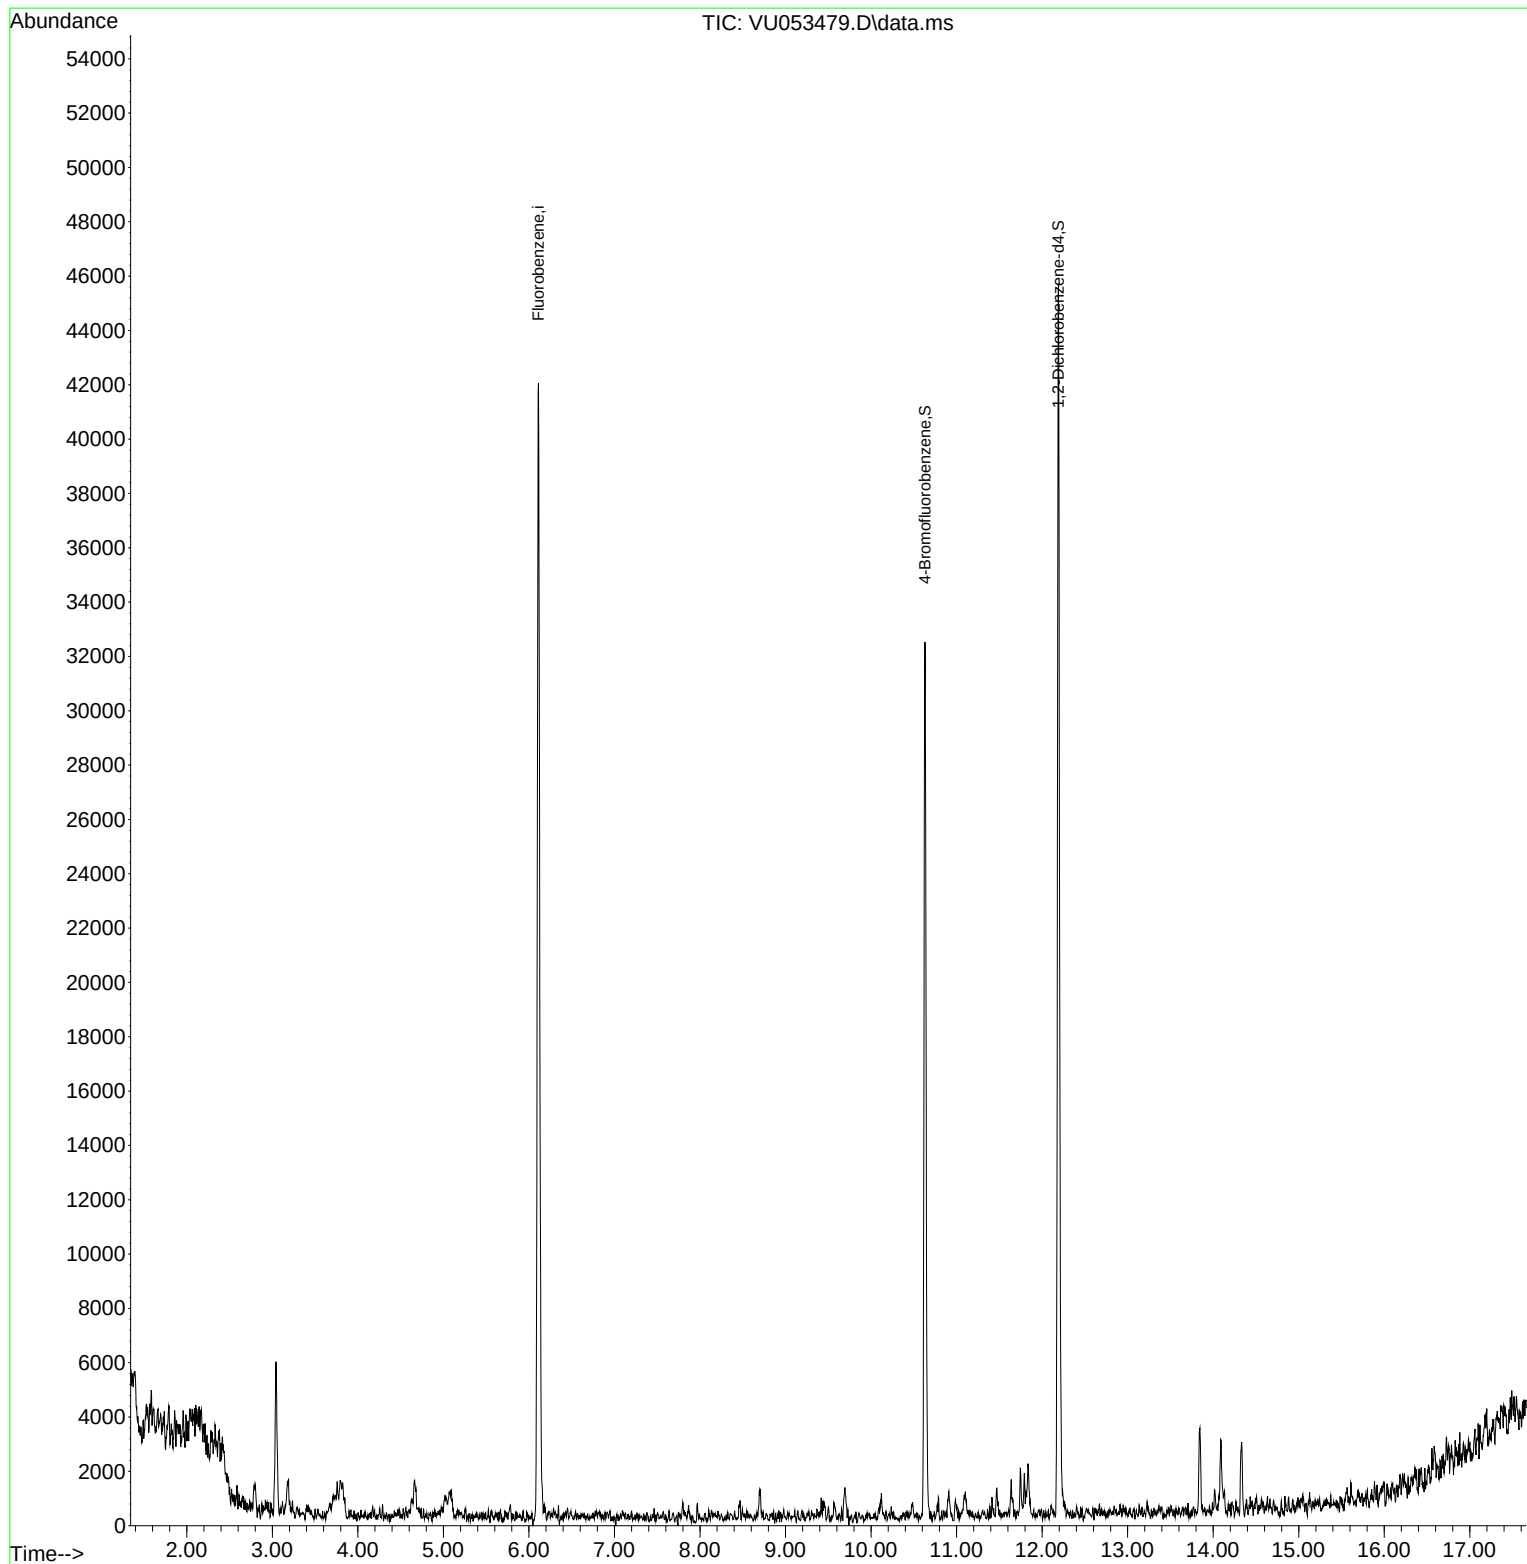


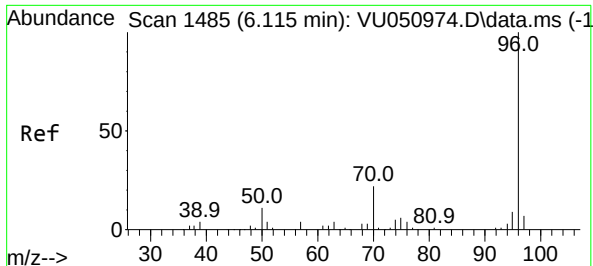

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.112 min Scan# 1484
Delta R.T. -0.003 min
Lab File: VU053479.D
Acq: 30 Mar 2023 10:53




Instrument :
MSVOA_U
ClientSampleId :
VU0330


Tgt Ion: 96	Resp: 39852
Ion Ratio	Lower Upper
96 100	
70 20.6	16.5 24.7
95 9.1	7.4 11.0
97 7.1	0.0 0.0

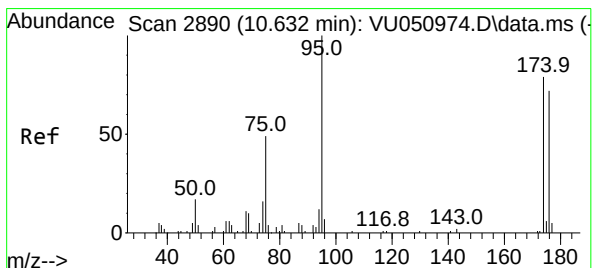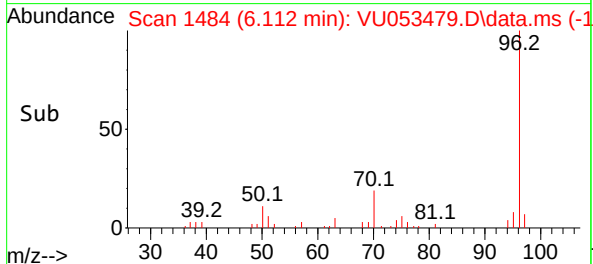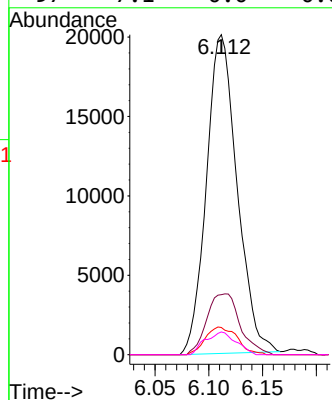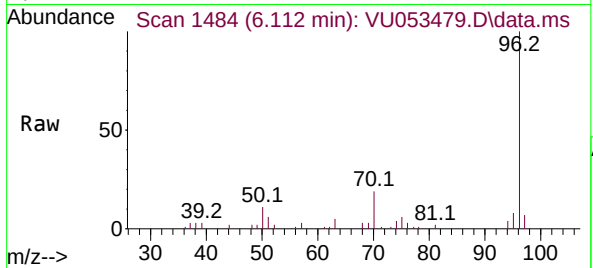

#57
4-Bromofluorobenzene
Concen: 0.847 ug/l
RT: 10.632 min Scan# 2890
Delta R.T. 0.000 min
Lab File: VU053479.D
Acq: 30 Mar 2023 10:53


Tgt Ion: 95	Resp: 12190
Ion Ratio	Lower Upper
95 100	
174 64.4	63.3 94.9
176 68.2	59.3 88.9

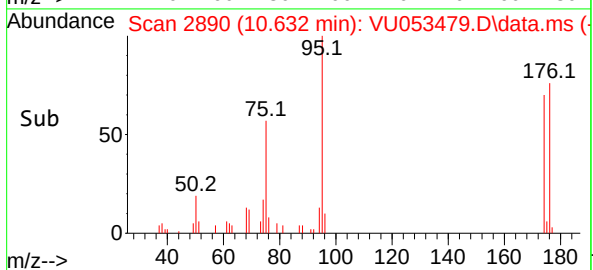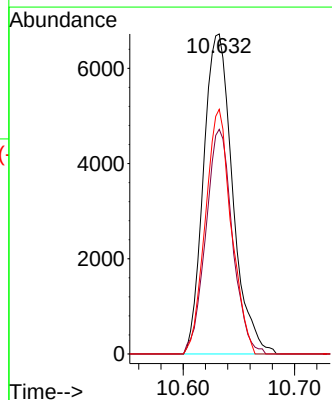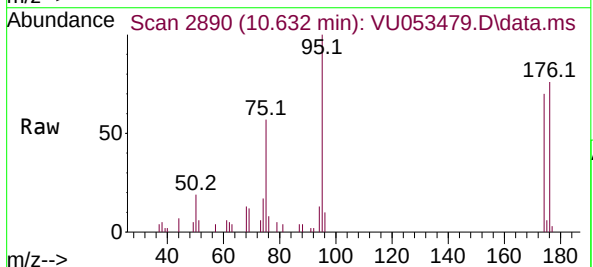

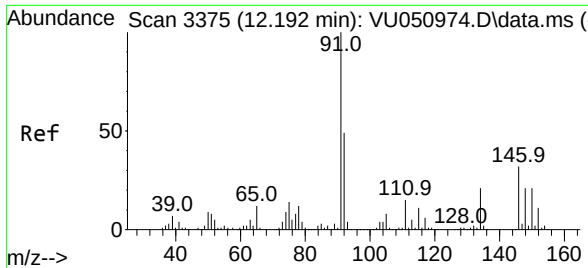

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.773 ug/l
 RT: 12.189 min Scan# 31
 Delta R.T. -0.003 min
 Lab File: VU053479.D
 Acq: 30 Mar 2023 10:53

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0330

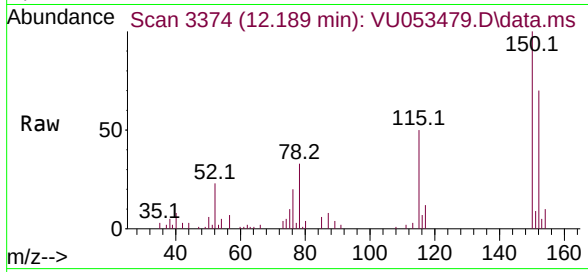

Tgt Ion:	152	Resp:	11161
Ion	Ratio	Lower	Upper
152	100		
115	70.7	0.0	308.8
150	162.3	0.0	635.0

