

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU033119\
Data File : VU030576.D
Acq On : 30 Mar 2019 17:00
Operator : JC/SP
Sample : VU0331WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0331WBL01

Quant Time: Mar 31 01:38:51 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\524U033119DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Sun Mar 31 01:11:51 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene	5.74	96	43992	1.00	ug/l	0.00

System Monitoring Compounds

57) 4-Bromofluorobenzene	10.31	95	15074	0.90	ug/l	0.00
Spiked Amount 1.000			Recovery	=	90.00%	
68) 1,2-Dichlorobenzene-d4	11.86	152	14299	0.92	ug/l	0.00
Spiked Amount 1.000			Recovery	=	92.00%	


Target Compounds	Ovalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU033119\
Data File : VU030576.D
Acq On : 30 Mar 2019 17:00
Operator : JC/SP
Sample : VU0331WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0331WBL01

Quant Time: Mar 31 01:38:51 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U033119DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Sun Mar 31 01:11:51 2019
Response via : Initial Calibration

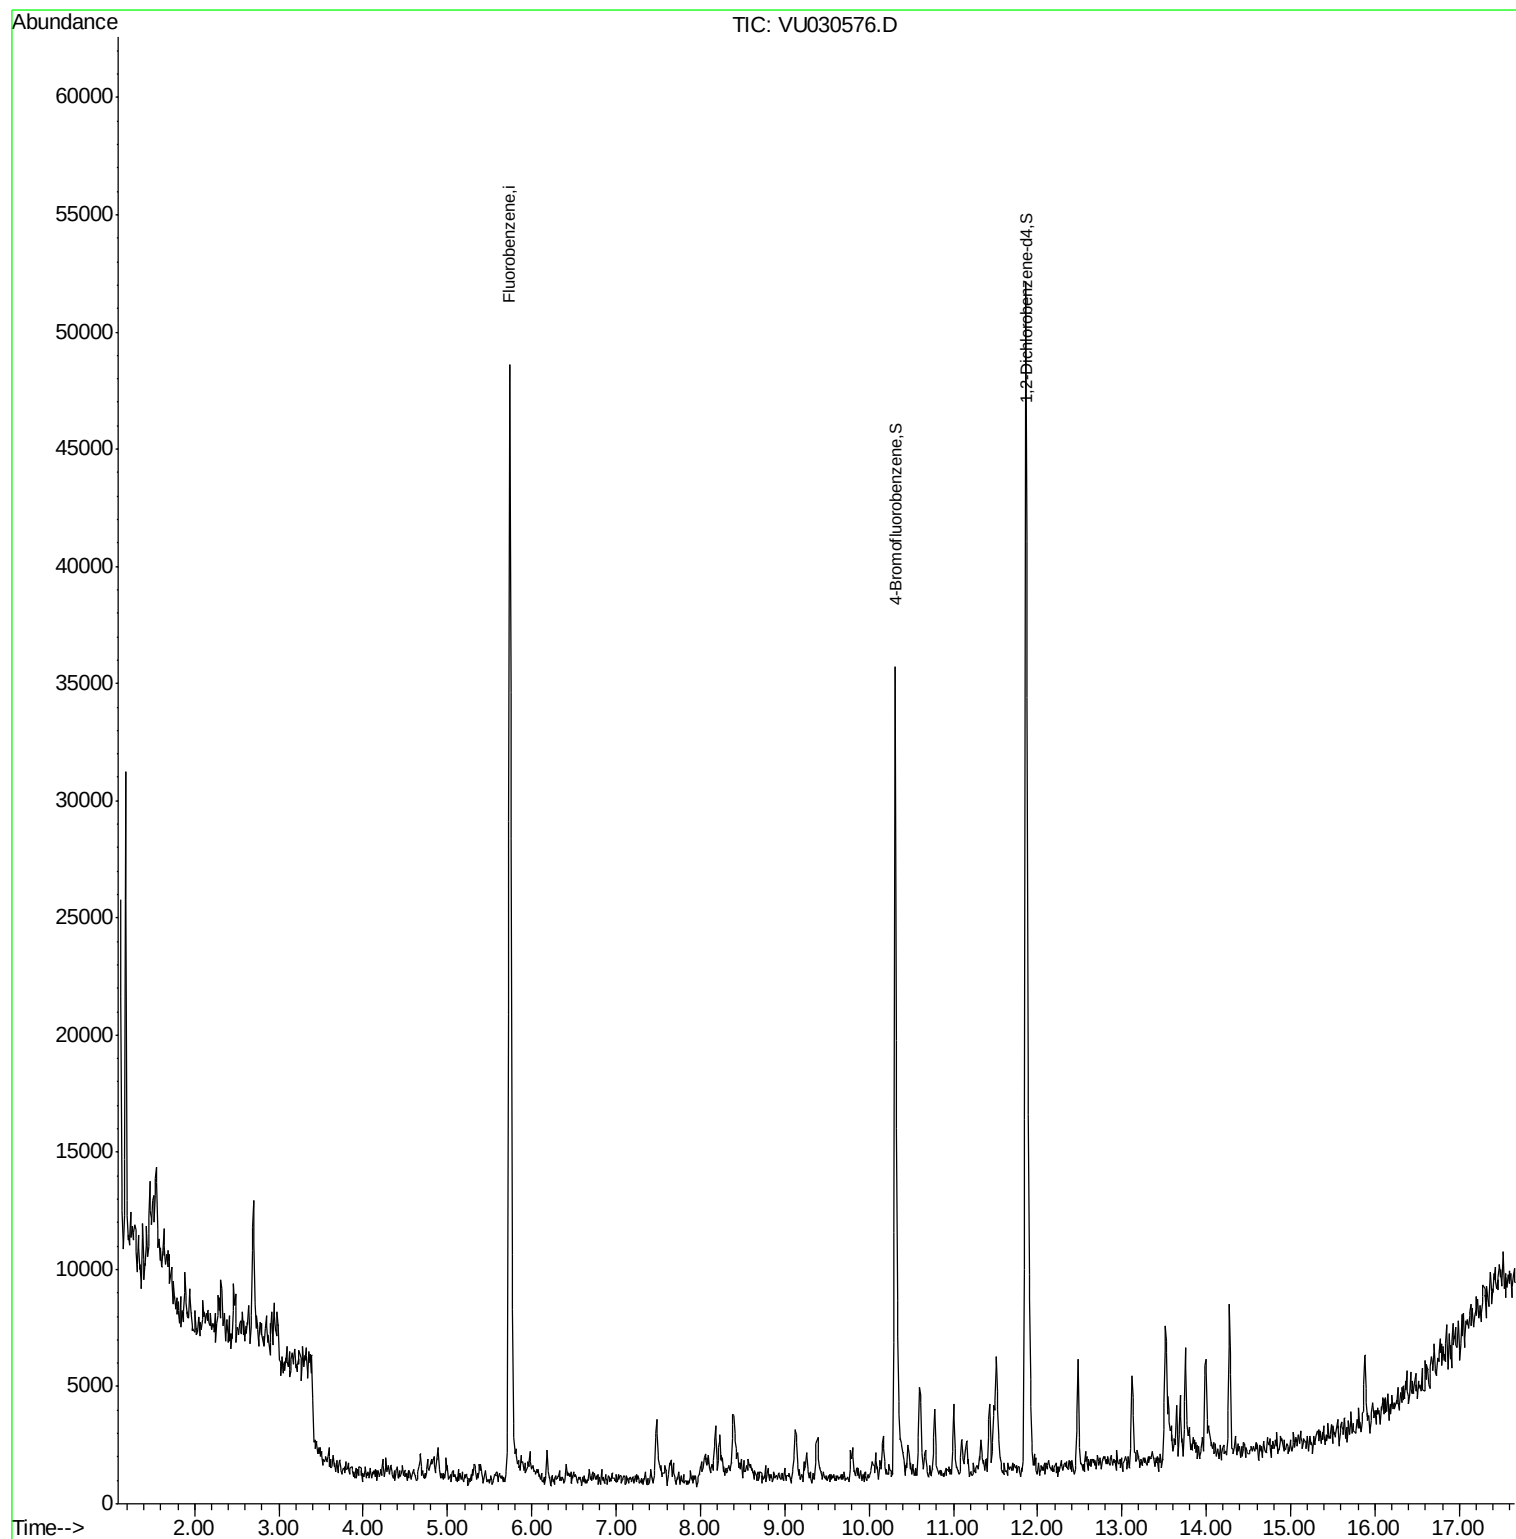

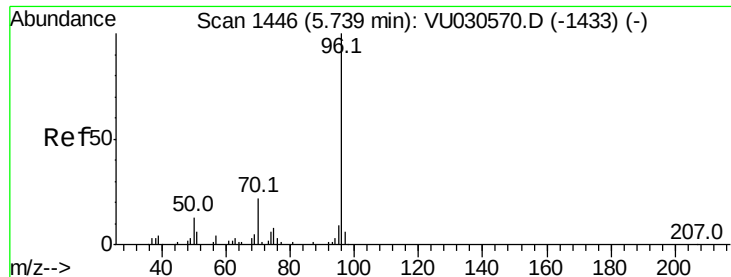

#1

Fluorobenzene

Concen: 1.000 ug/l

RT: 5.74 min Scan# 1446

Delta R.T. -0.00 min

Lab File: VU030576.D

Acq: 30 Mar 2019 17:00

Instrument :

MSVOA_U

ClientSampleId :

VU0331WBL01

Tot Ion: 96 Resp: 43992





Ion Ratio Lower Upper

96 100

70 21.9 15.6 23.4

95 9.8 7.3 10.9

97 6.4 0.0 0.0#

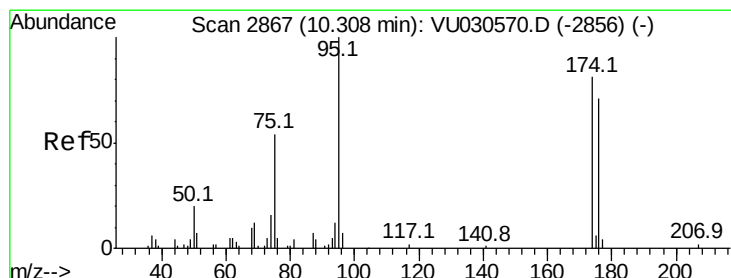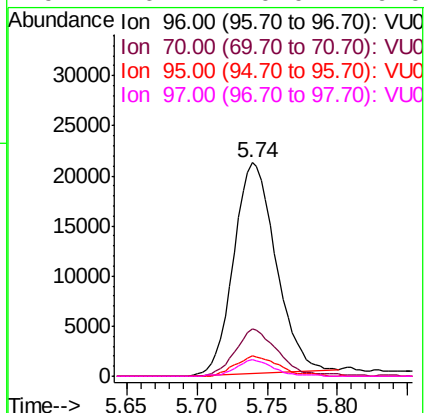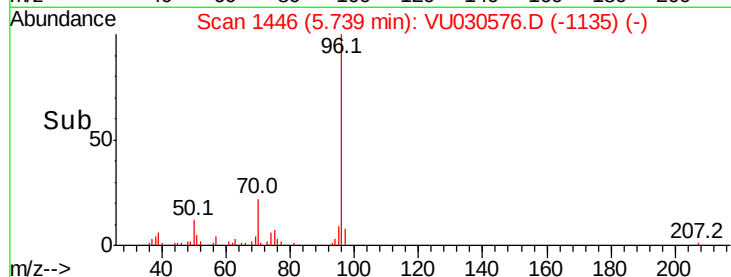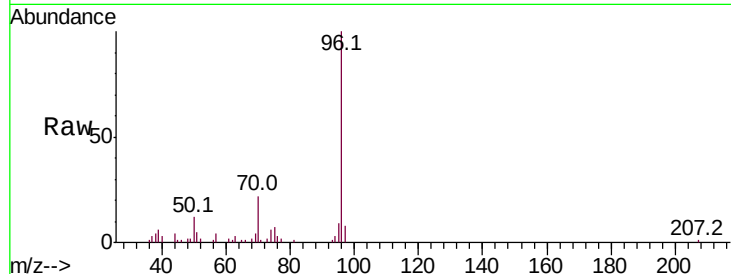

#57

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 10.31 min Scan# 2868

Delta R.T. 0.00 min

Lab File: VU030576.D

Acq: 30 Mar 2019 17:00




Tgt Ion: 95 Resp: 15074


Ion Ratio Lower Upper

95 100

174 70.3 60.5 90.7

176 69.5 57.9 86.9

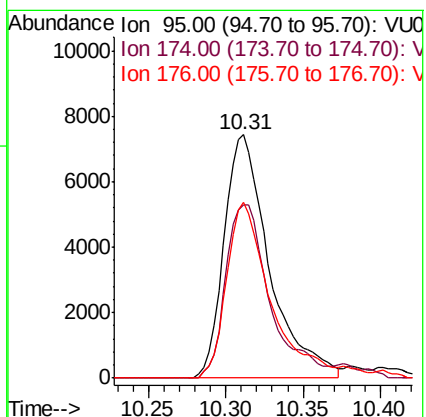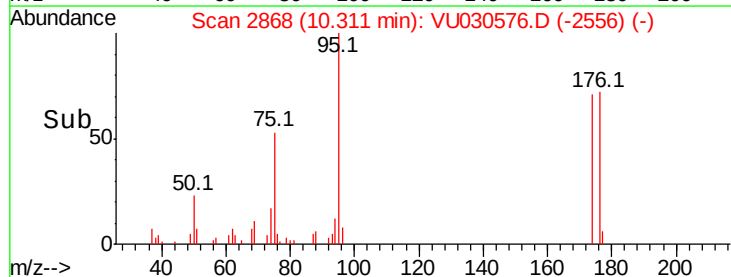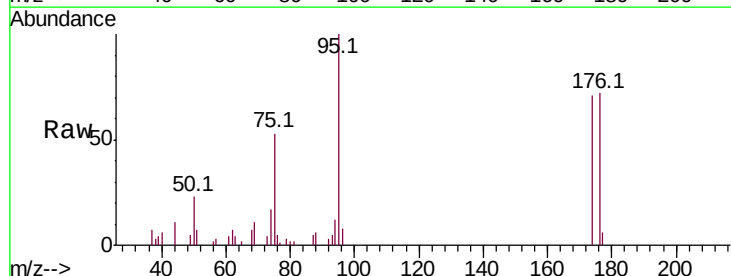


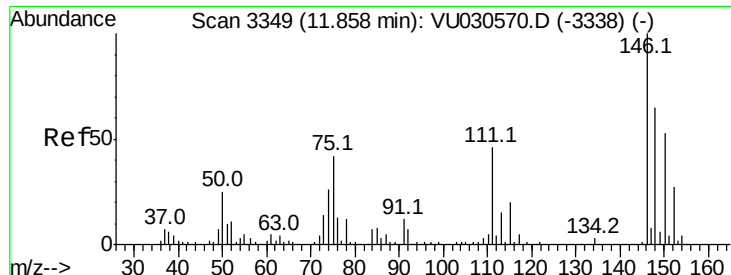

#68
 1,2-Dichlorobenzene-d4
 Concen: N.D. ug/l
 RT: 11.86 min Scan# 3350
 Delta R.T. 0.00 min
 Lab File: VU030576.D
 Acq: 30 Mar 2019 17:00

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0331WBL01

Tot Ion	Ratio	Lower	Upper
152	100		
115	71.2	0.0	136.2
150	170.0	0.0	634.6

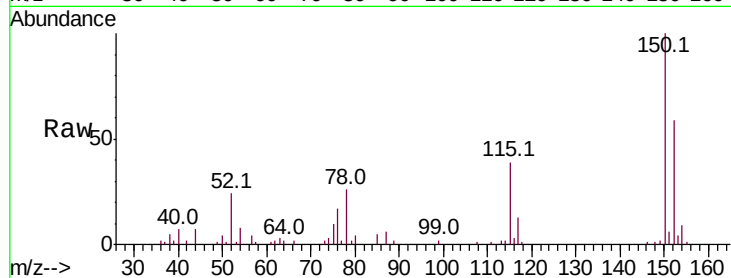

Abundance

Ion 152.00 (151.70 to 152.70): V

Ion 115.00 (114.70 to 115.70): V

Ion 150.00 (149.70 to 150.70): V

