

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU033119\
 Data File : VU030576.D
 Acq On : 30 Mar 2019 17:00
 Operator : JC/SP
 Sample : VU0331WBL01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0331WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\524U033119DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.698	494	500	510	rVB5	5446	8397	7.62%	2.065%
2	2.939	572	575	582	rBV6	1784	1955	1.77%	0.481%
3	3.386	712	714	723	rVB3	3731	4202	3.81%	1.033%
4	4.887	1172	1181	1187	rBV4	1095	1796	1.63%	0.442%
5	5.739	1434	1446	1463	rBV	47242	98772	89.60%	24.289%
6	6.180	1575	1583	1590	rBV6	1440	1980	1.80%	0.487%
7	7.479	1978	1987	2001	rBV5	2497	5046	4.58%	1.241%
8	7.678	2045	2049	2058	rVB3	966	1201	1.09%	0.295%
9	8.180	2195	2205	2213	rVB6	1921	3195	2.90%	0.786%
10	8.234	2213	2222	2225	rBV9	1557	2246	2.04%	0.552%
11	8.385	2263	2269	2272	rBV5	2084	2245	2.04%	0.552%
12	9.125	2494	2499	2501	rBV5	1240	1204	1.09%	0.296%
13	9.260	2536	2541	2550	rVB3	1105	1715	1.56%	0.422%
14	9.373	2572	2576	2579	rBV3	1439	1405	1.27%	0.346%
15	9.392	2579	2582	2589	rVB2	1455	1461	1.33%	0.359%
16	10.167	2817	2823	2832	rVB6	1645	2491	2.26%	0.613%
17	10.311	2858	2868	2887	rBV3	34462	65749	59.65%	16.169%
18	10.459	2910	2914	2922	rVB5	1064	1474	1.34%	0.362%
19	10.604	2948	2959	2973	rBV10	3768	8502	7.71%	2.091%
20	10.778	3007	3013	3020	rVB6	2415	3301	2.99%	0.812%
21	11.003	3076	3083	3092	rBV5	2973	4588	4.16%	1.128%
22	11.096	3107	3112	3121	rBV3	1381	2290	2.08%	0.563%
23	11.157	3122	3131	3135	rVV4	1476	2523	2.29%	0.620%
24	11.327	3180	3184	3193	rVB5	1035	1370	1.24%	0.337%
25	11.430	3207	3216	3223	rBV7	2892	4721	4.28%	1.161%
26	11.472	3225	3229	3230	rBV3	1857	1140	1.03%	0.280%
27	11.504	3235	3239	3240	rBV4	1760	1279	1.16%	0.315%
28	11.861	3338	3350	3373	rBV3	50778	110232	100.00%	27.107%
29	12.479	3532	3542	3552	rBV	4715	7651	6.94%	1.881%
30	13.125	3732	3743	3751	rBV5	3984	7067	6.41%	1.738%
31	13.520	3857	3866	3872	rBV6	5414	9830	8.92%	2.417%
32	13.549	3872	3875	3879	rVB2	1501	1411	1.28%	0.347%
33	13.649	3901	3906	3913	rVB2	2169	2283	2.07%	0.561%
34	13.691	3913	3919	3924	rBV7	2612	3064	2.78%	0.753%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU033119\
Data File : VU030576.D
Acq On : 30 Mar 2019 17:00
Operator : JC/SP
Sample : VU0331WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0331WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U033119DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

35	13.752	3930	3938	3948	rBV5	4634	7533	6.83%	1.852%
36	13.987	4005	4011	4012	rBV4	3911	2948	2.67%	0.725%
37	14.279	4094	4102	4111	rVB2	6278	9173	8.32%	2.256%
38	15.601	4506	4513	4518	rBV4	1039	1664	1.51%	0.409%
39	15.880	4594	4600	4609	rVB8	2619	4121	3.74%	1.013%
40	16.880	4908	4911	4915	rBV6	1505	1388	1.26%	0.341%
41	16.922	4920	4924	4928	rBV5	1936	2035	1.85%	0.500%


Sum of corrected areas: 406648

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU033119\
Data File : VU030576.D
Acq On : 30 Mar 2019 17:00
Operator : JC/SP
Sample : VU0331WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0331WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U033119DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

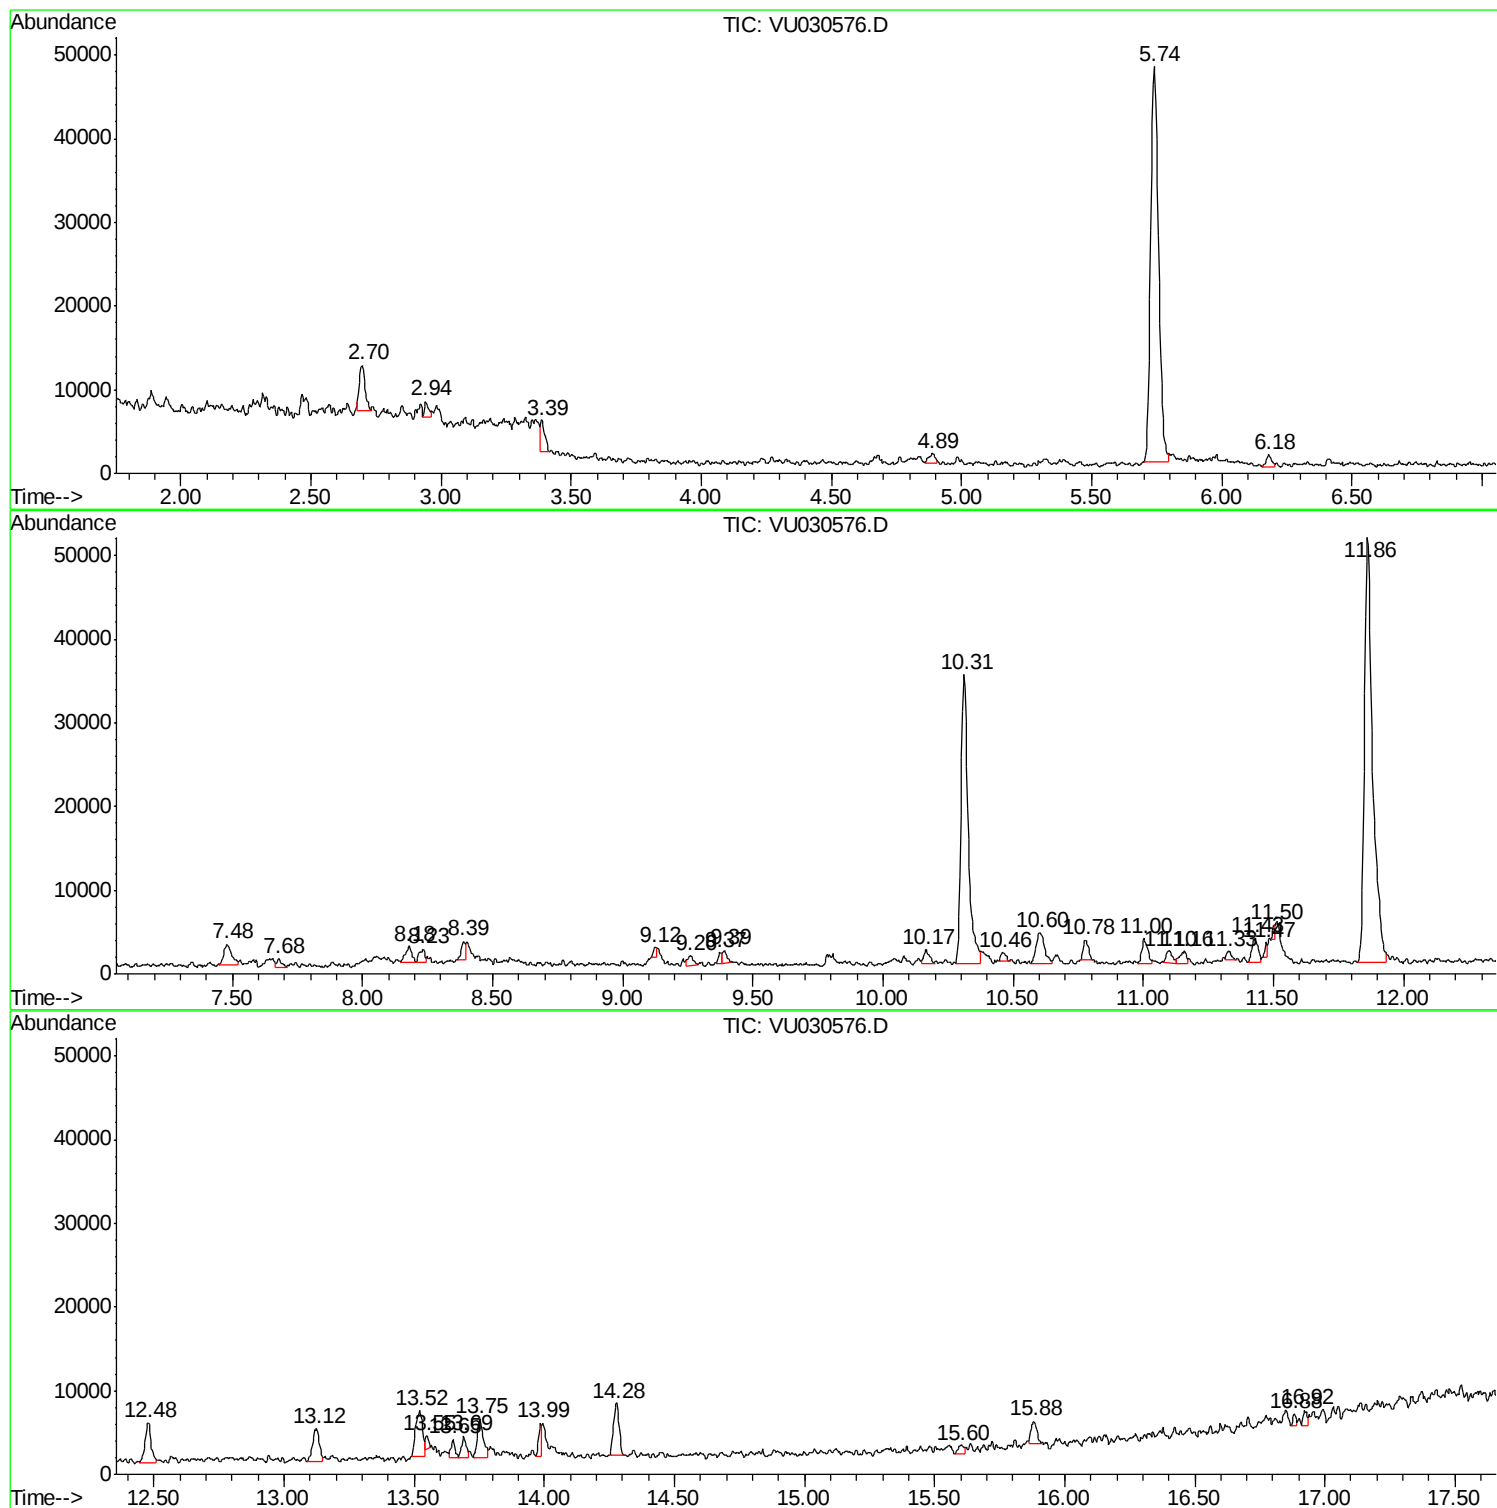

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU033119\
Data File : VU030576.D
Acq On : 30 Mar 2019 17:00
Operator : JC/SP
Sample : VU0331WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0331WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U033119DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU033119\
Data File : VU030576.D
Acq On : 30 Mar 2019 17:00
Operator : JC/SP
Sample : VU0331WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0331WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U033119DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc