


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU033120\
 Data File : VU037491.D
 Acq On : 31 Mar 2020 08:37
 Operator : JC/MD
 Sample : BFB10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB10

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR033120WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Mar 31 10:58:13 2020

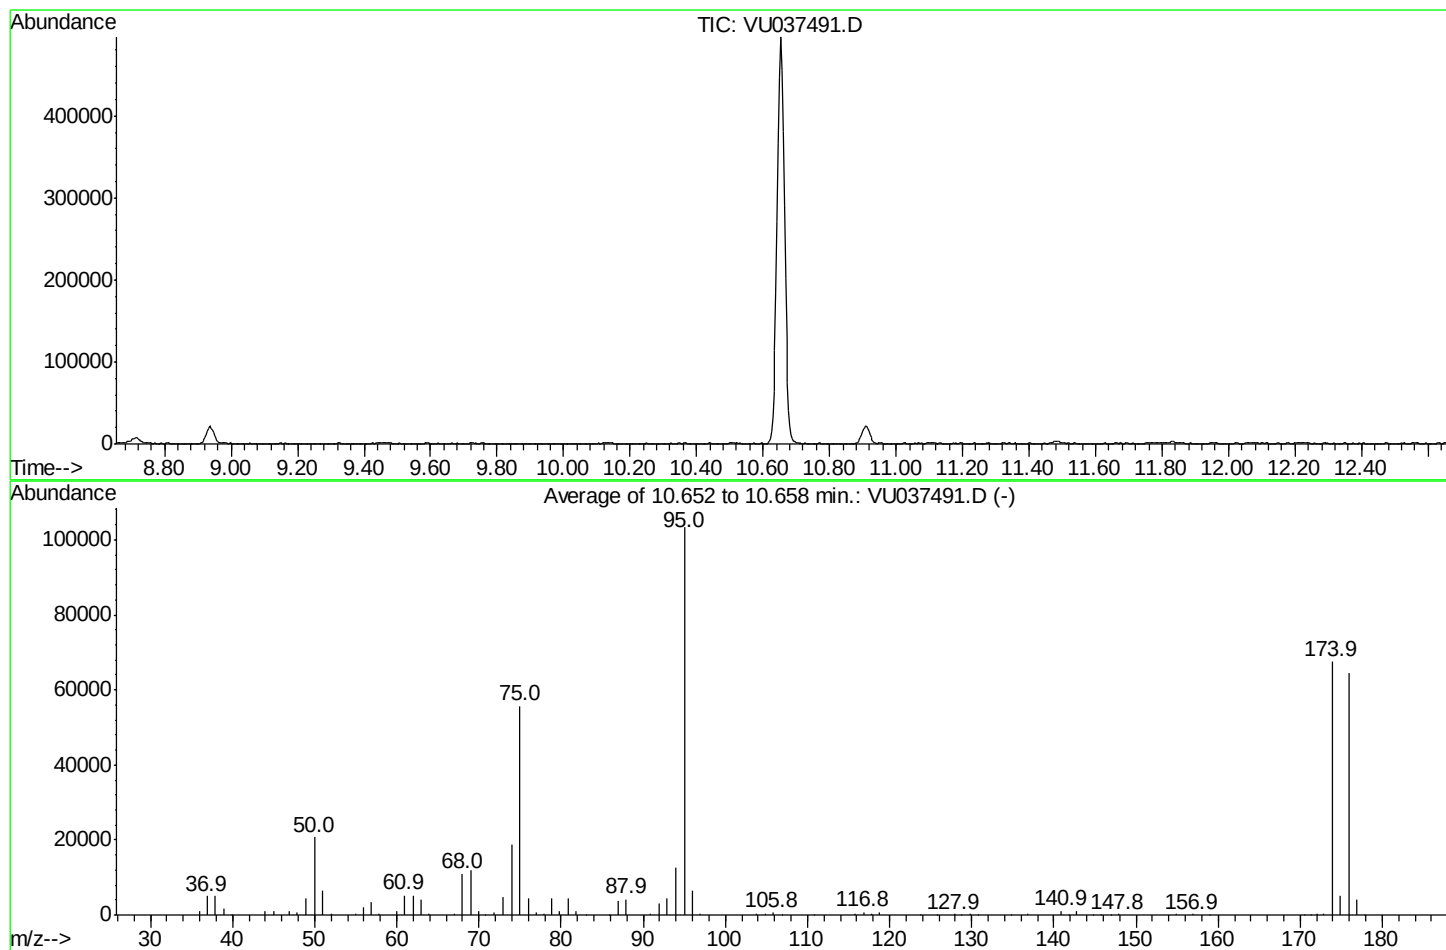

AutoFind: Scans 2896, 2897, 2898; Background Corrected with Scan 2882

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	20682	PASS
75	95	30	80	53.8	55637	PASS
95	95	100	100	100.0	103320	PASS
96	95	5	9	6.1	6353	PASS
173	174	0.00	2	0.8	522	PASS
174	95	50	120	65.3	67506	PASS
175	174	5	9	7.6	5113	PASS
176	174	95	101	95.4	64378	PASS
177	176	5	9	6.6	4256	PASS

Scan 2882 (10.607 min): VU037491.D
BFB10

m/z	Abundance
40.90	135.0
42.90	187.0
43.90	183.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

m/z	Abundance
35.90	877.0
36.90	5540.0
37.90	5053.0
39.00	1945.0
39.90	156.0
43.00	197.0
43.90	1099.0
45.00	1132.0
46.90	1091.0
47.80	728.0
48.90	4687.0
50.00	21648.0
51.00	7077.0
52.00	334.0
54.90	390.0
55.90	2135.0
56.90	3493.0
57.80	257.0
60.00	1164.0
60.90	5794.0
61.90	5479.0
63.00	4316.0
63.90	401.0
67.10	296.0
68.00	11780.0
69.00	12153.0
69.90	934.0
71.90	709.0
72.90	4896.0
74.00	19536.0
75.00	57792.0
76.00	4714.0
76.90	662.0
77.90	499.0
78.80	4261.0
79.90	1270.0
80.90	4876.0
81.80	993.0
83.00	167.0
85.80	137.0
86.90	3627.0
87.90	4118.0
90.80	493.0
91.90	3261.0
92.90	4525.0
94.00	12559.0
95.00	105872.0
95.90	6517.0
96.90	184.0
103.80	473.0
104.80	256.0
105.80	596.0
106.90	106.0
110.70	164.0
115.80	506.0
116.90	739.0
117.80	374.0
118.80	644.0
123.70	114.0
125.70	115.0
127.90	271.0
128.70	170.0
129.80	303.0
130.80	107.0
134.80	166.0
136.80	177.0
140.90	1225.0
141.90	105.0
142.80	1025.0
145.70	160.0
147.00	100.0
147.90	226.0
154.80	196.0
156.90	223.0
170.50	121.0
171.20	137.0
172.00	200.0
172.80	543.0
173.90	68288.0
174.90	4986.0
175.90	64328.0
176.90	4127.0
177.80	146.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

m/z	Abundance
35.90	945.0
36.90	5206.0
37.90	5223.0
39.00	1813.0
39.90	150.0
43.00	150.0
43.90	1099.0
45.00	1024.0
46.90	1059.0
47.80	700.0
48.90	4550.0
50.00	21168.0
51.00	6757.0
52.00	345.0
54.90	385.0
55.90	2056.0
56.90	3478.0
57.90	232.0
60.00	1146.0
60.90	5372.0
61.90	5345.0
62.90	4420.0
63.90	364.0
67.00	280.0
68.00	11451.0
69.00	12418.0
69.90	887.0
70.80	122.0
71.90	653.0
72.90	4881.0
74.00	19312.0
75.00	57120.0
76.00	4642.0
76.90	629.0
77.90	561.0
78.80	4434.0
79.90	1217.0
80.90	4713.0
81.80	1059.0
83.00	153.0
85.80	104.0
86.90	3947.0
87.90	4313.0
90.80	463.0
91.90	3395.0
92.90	4624.0
94.00	13106.0
95.00	106464.0
96.00	6548.0
96.90	229.0
103.80	503.0
104.80	284.0
105.80	621.0
106.90	119.0
110.70	141.0
115.80	483.0
116.90	798.0
117.70	371.0
118.80	609.0
123.70	156.0
125.70	119.0
127.90	332.0
128.80	151.0
129.90	307.0
130.70	127.0
134.80	156.0
136.80	202.0
140.90	1215.0
141.90	119.0
142.80	1096.0
144.80	108.0
145.70	175.0
147.80	190.0
154.90	217.0
156.90	237.0
170.60	105.0
171.20	195.0
172.00	218.0
172.90	532.0
173.90	69584.0
174.90	5270.0
175.90	66264.0
176.90	4377.0
177.80	154.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

m/z	Abundance
35.90	837.0
36.90	4495.0
37.90	4777.0
39.00	1660.0
41.00	108.0
42.90	128.0
43.90	973.0
44.90	899.0
46.90	937.0
47.80	580.0
48.90	4166.0
50.00	19232.0
51.00	5731.0
52.00	364.0
55.00	348.0
55.90	1811.0
56.90	3213.0
57.90	172.0
59.90	1059.0
60.90	4611.0
62.00	4817.0
62.90	3893.0
63.90	296.0
66.90	310.0
67.90	9997.0
69.00	11418.0
69.90	819.0
70.80	132.0
71.90	574.0
73.00	4405.0
74.00	17288.0
75.00	52000.0
76.00	4318.0
76.90	561.0
77.90	508.0
78.80	4155.0
79.80	1009.0
80.80	4148.0
81.90	1009.0
83.00	131.0
86.90	3771.0
87.90	3914.0
90.80	416.0
91.90	2984.0
92.90	4420.0
94.00	12312.0
95.00	97624.0
96.00	5996.0
96.80	197.0
103.80	523.0
104.80	263.0
105.80	563.0
110.80	103.0
115.70	423.0
116.80	727.0
117.70	374.0
118.80	585.0
123.80	130.0
127.90	344.0
128.80	125.0
129.90	271.0
130.70	135.0
134.80	155.0
136.80	197.0
140.90	1047.0
141.80	103.0
142.80	1075.0
144.80	118.0
145.70	170.0
147.80	163.0
155.00	256.0
156.90	217.0
159.00	124.0
171.30	201.0
172.00	220.0
172.90	492.0
173.90	64648.0
174.90	5085.0
175.90	62544.0
176.90	4265.0
177.80	147.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10