


Methyl Iodide

Response Ratio

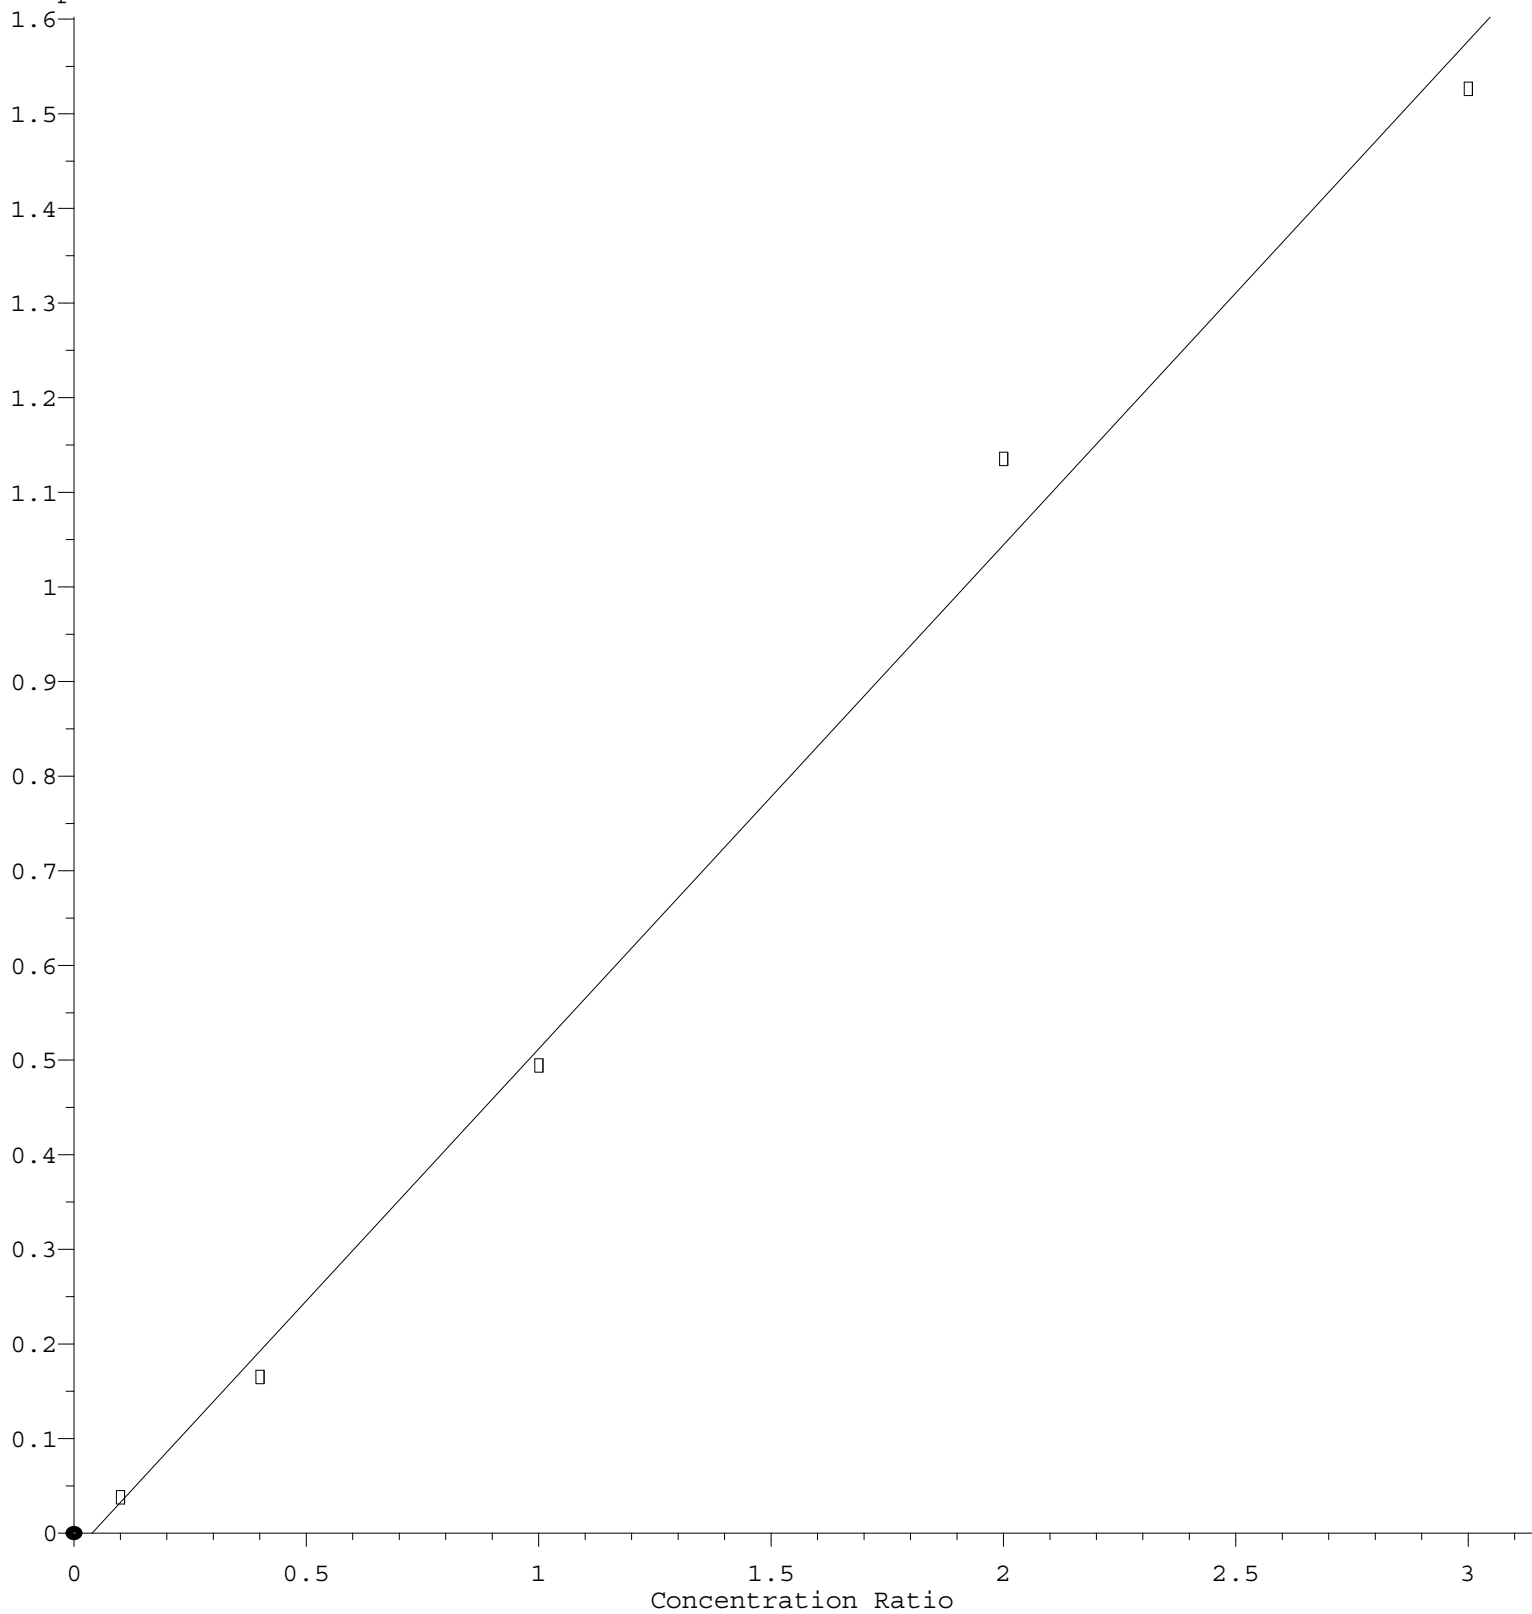

$$\text{Response} = 5.327\text{e-}001 * \text{Amt} - 2.082\text{e-}002$$


Coef of Det (r^2) = 0.992724 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U033122W.M

Calibration Table Last Updated: Thu Mar 31 13:50:29 2022

2-Chloroethyl Vinyl ether


Response Ratio

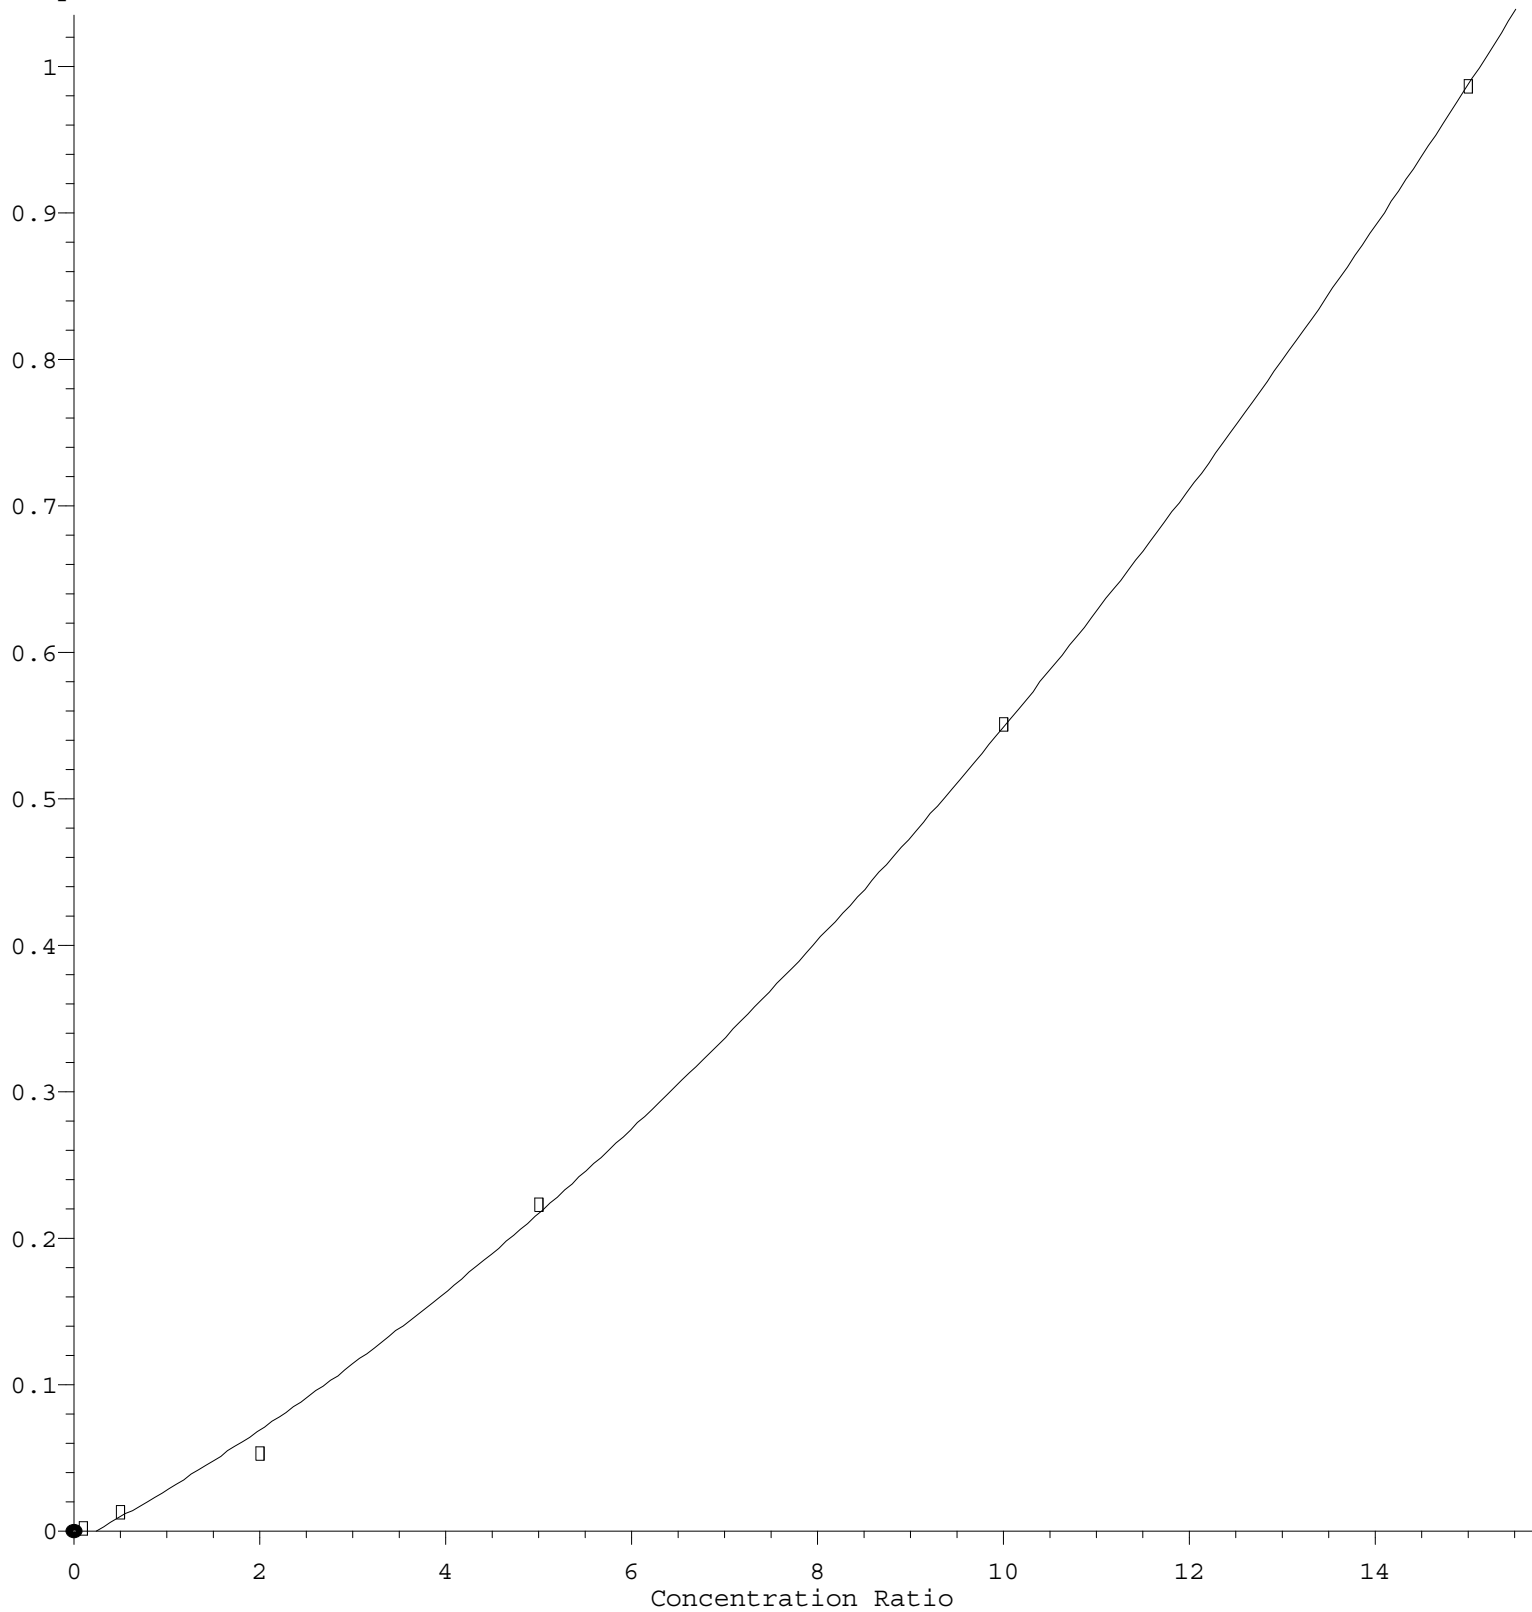

$R = 2.137e-003 A^2 + 3.432e-002 A - 8.023e-003$
Coef of Det (r^2) = 0.999542 Curve Fit: Quadratic
Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U033122W.M
Calibration Table Last Updated: Thu Mar 31 13:50:29 2022

Acrolein

Response Ratio

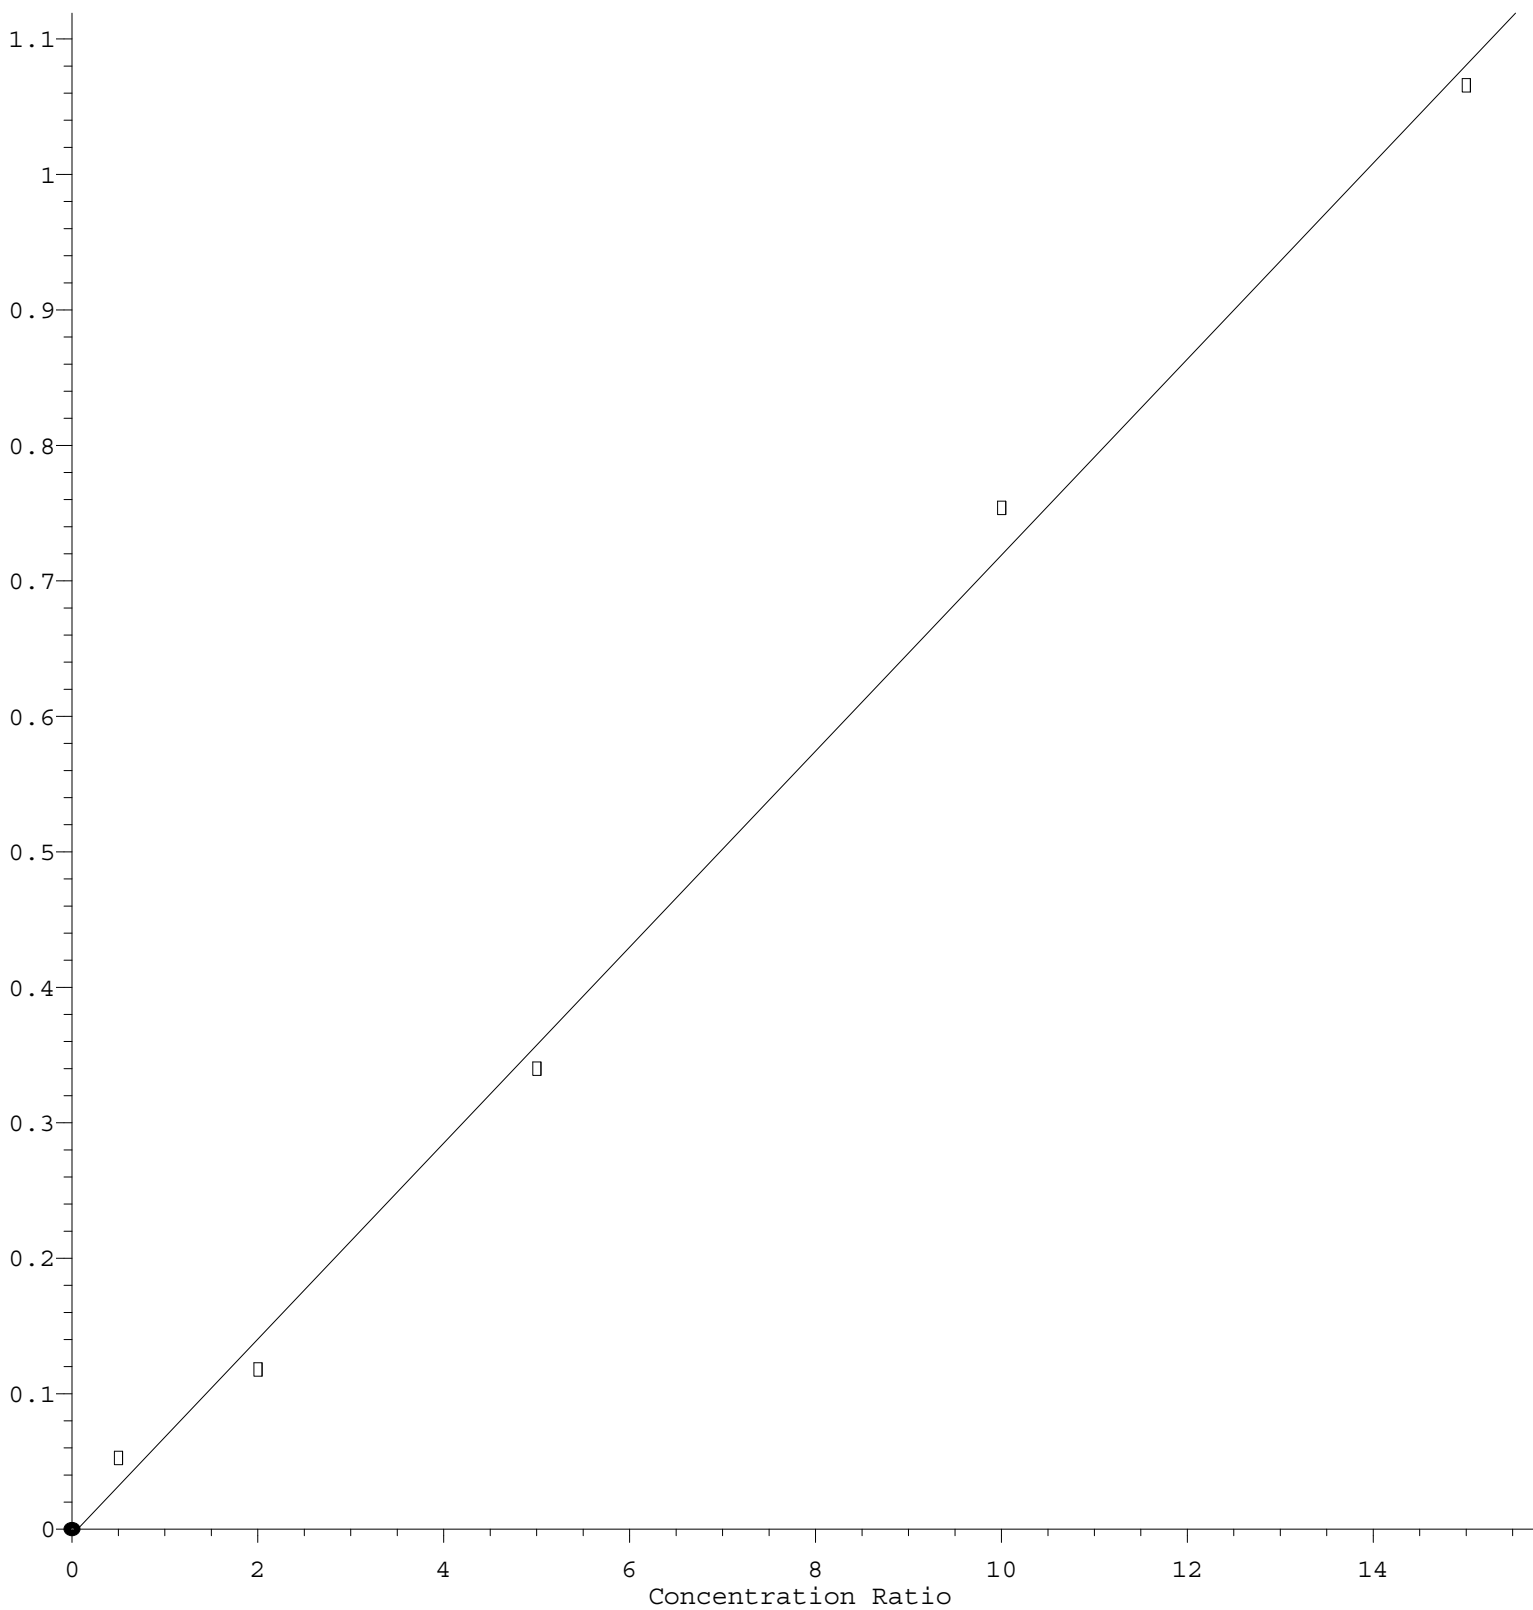

$$\text{Response} = 7.232\text{e-}002 * \text{Amt} - 4.085\text{e-}003$$

Coef of Det (r^2) = 0.996431 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U033122W.M

Calibration Table Last Updated: Thu Mar 31 13:50:29 2022