


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU033122\
 Data File : VU047765.D
 Acq On : 31 Mar 2022 08:59
 Operator : SY/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U033122W.M
 Title : SW846 8260
 Last Update : Thu Mar 31 13:50:29 2022

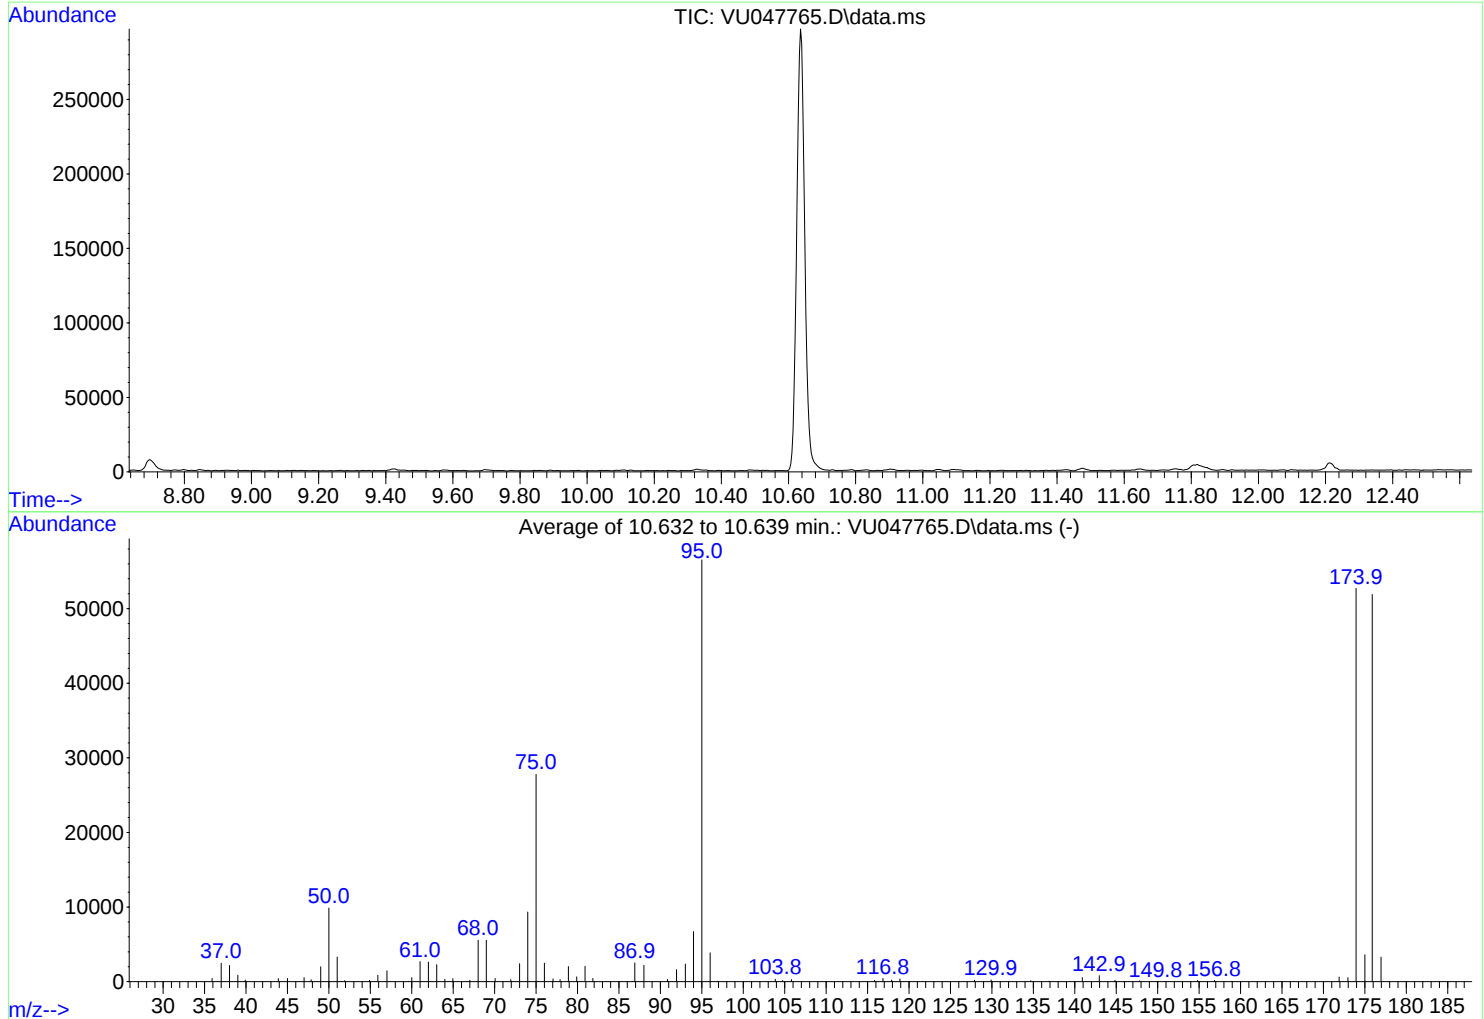

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	9873	PASS
75	95	30	60	49.1	27784	PASS
95	95	100	100	100.0	56541	PASS
96	95	5	9	6.8	3863	PASS
173	174	0.00	2	1.0	544	PASS
174	95	50	100	93.2	52717	PASS
175	174	5	9	6.8	3608	PASS
176	174	95	101	98.5	51901	PASS
177	176	5	9	6.3	3281	PASS