




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU033123\
 Data File : VU053501.D
 Acq On : 31 Mar 2023 18:58
 Operator : JC/MD
 Sample : 02121-07ME
 Misc : 5.46g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C1180ME

Manual IntegrationsAPPROVED

Quant Time: Apr 01 05:09:10 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 01 04:51:17 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/03/2023
 Supervised By :Mahesh Dadoda 04/03/2023

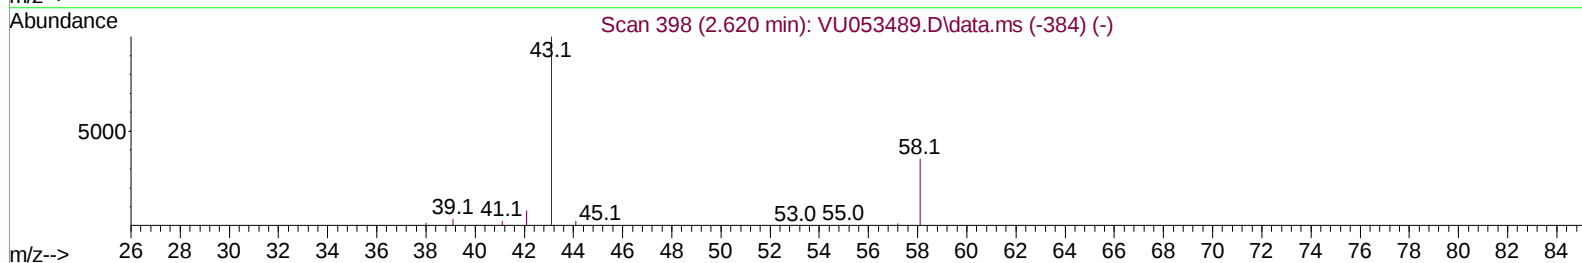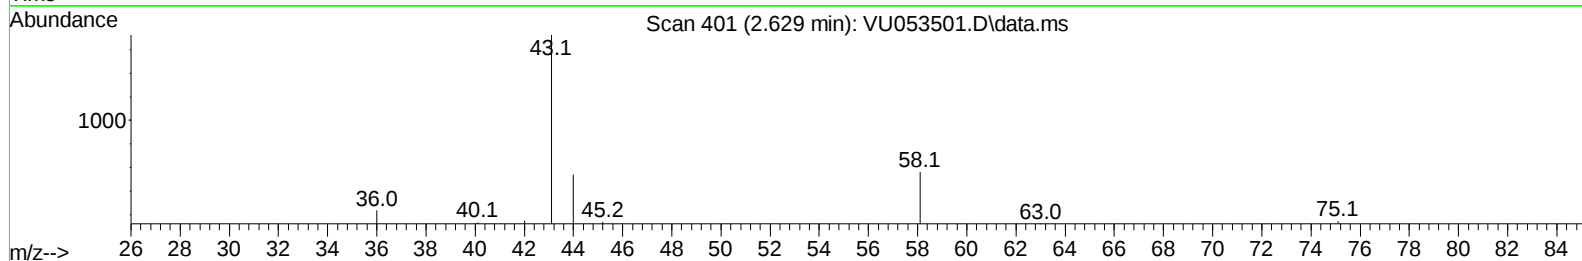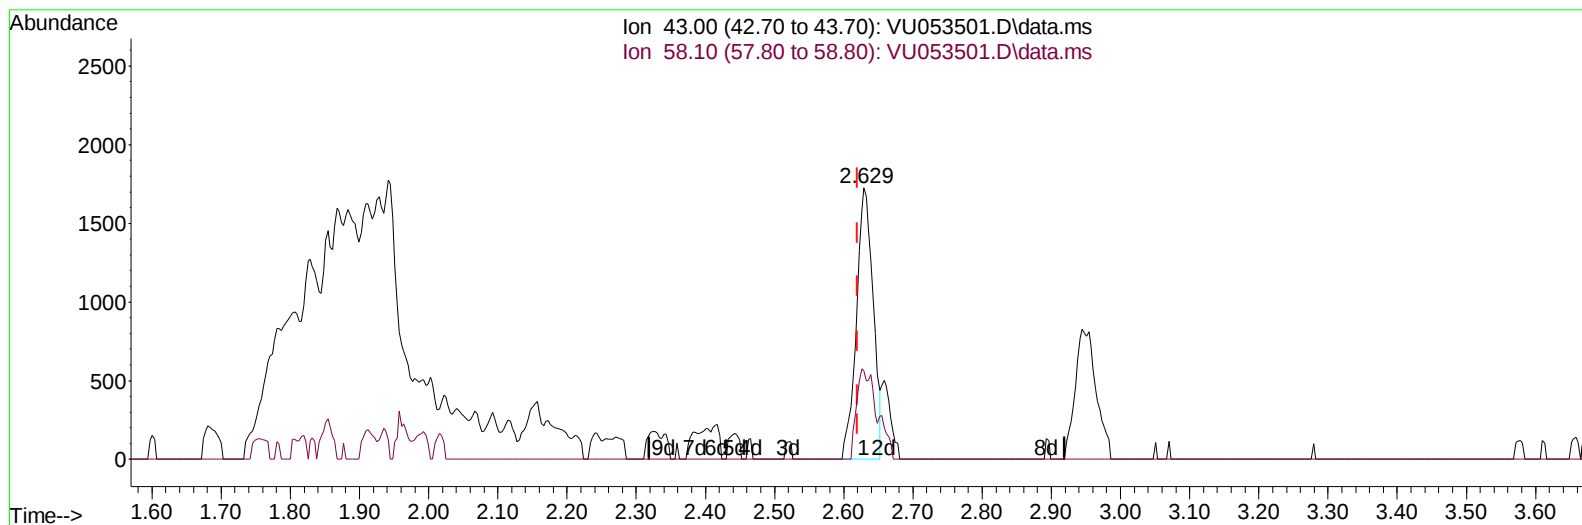

TIC: VU053501.D\data.ms

(13) Acetone (T)

2.629min (+ 0.010) 3.64 ug/L

response 2898

Ion	Exp%	Act%
43.00	100.00	100.00
58.10	35.10	20.01
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU033123\
 Data File : VU053501.D
 Acq On : 31 Mar 2023 18:58
 Operator : JC/MD
 Sample : 02121-07ME
 Misc : 5.46g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C1180ME

Manual IntegrationsAPPROVED

Quant Time: Apr 01 05:09:10 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 01 04:51:17 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/03/2023
 Supervised By :Mahesh Dadoda 04/03/2023

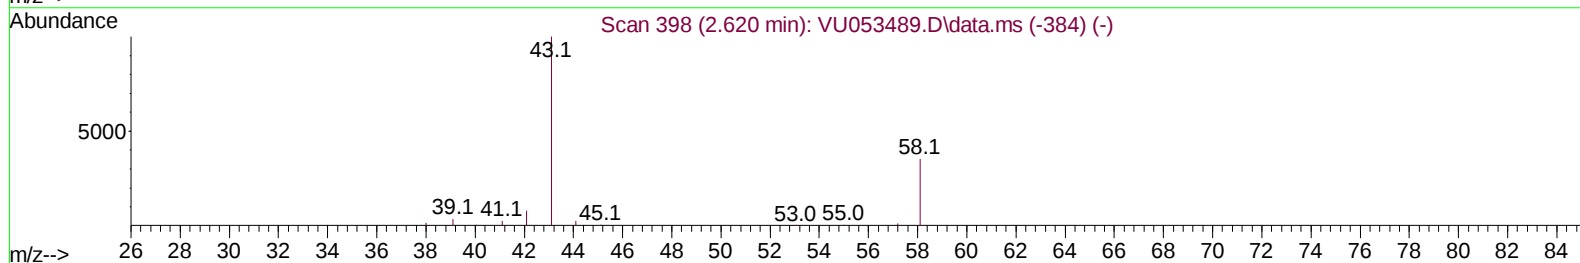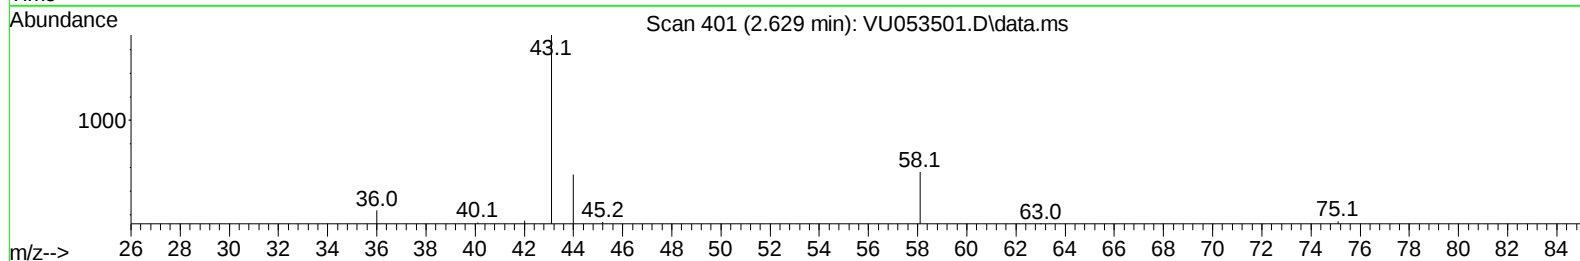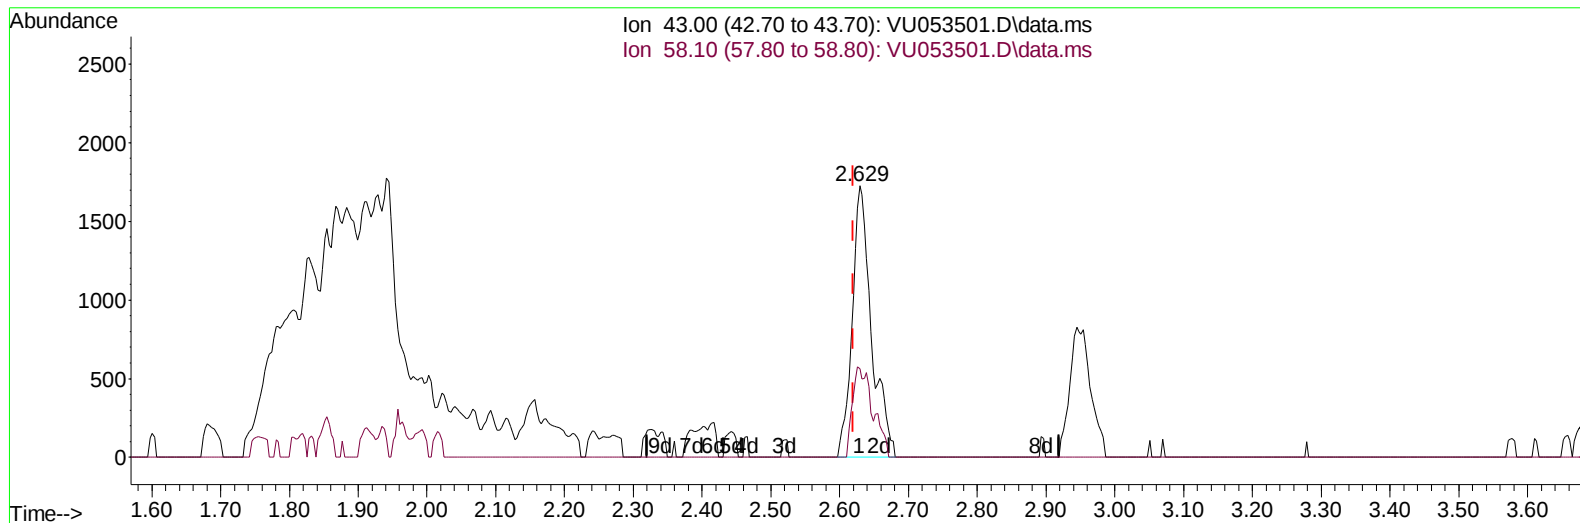

TIC: VU053501.D\data.ms

(13) Acetone (T)

2.629min (+ 0.010) 4.24 ug/L m

response 3372

Ion	Exp%	Act%
43.00	100.00	100.00
58.10	35.10	17.20
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU033123\
 Data File : VU053501.D
 Acq On : 31 Mar 2023 18:58
 Operator : JC/MD
 Sample : 02121-07ME
 Misc : 5.46g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C1180ME

Manual IntegrationsAPPROVED

Quant Time: Apr 01 05:09:10 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 01 04:51:17 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/03/2023
 Supervised By :Mahesh Dadoda 04/03/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.240	114	251137	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	246529	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	145147	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	137887	70.512	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	141.020%#	
7) Chloroethane-d5	1.871	69	39318	26.077	ug/L	-0.04
Spiked Amount 50.000	Range 70	- 130	Recovery	=	52.160%#	
11) 1,1-Dichloroethene-d2	2.543	63	180078	59.489	ug/L	-0.02
Spiked Amount 50.000	Range 60	- 125	Recovery	=	118.980%	
21) 2-Butanone-d5	4.620	46	155135	175.221	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	175.220%#	
24) Chloroform-d	5.054	84	238209	73.656	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	147.320%#	
26) 1,2-Dichloroethane-d4	5.694	65	154617	80.908	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	161.820%#	
32) Benzene-d6	5.716	84	506896	76.174	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	152.340%#	
36) 1,2-Dichloropropane-d6	6.684	67	153671	75.552	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	151.100%#	
41) Toluene-d8	7.893	98	506464	76.575	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	153.140%#	
43) trans-1,3-Dichloroprop...	8.176	79	80481	76.654	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	153.300%#	
47) 2-Hexanone-d5	8.639	63	138121	198.973	ug/L	0.01
Spiked Amount 100.000	Range 45	- 130	Recovery	=	198.970%#	
56) 1,1,2,2-Tetrachloroeth...	10.754	84	249914	87.176	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	174.360%#	
66) 1,2-Dichlorobenzene-d4	12.192	152	242451	80.024	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	160.040%#	
Target Compounds						
					Qvalue	
5) vinyl chloride	1.600	62	12350	6.362	ug/L #	72
13) Acetone	2.629	43	3372m	4.238	ug/L	
17) trans-1,2-Dichloroethene	3.337	96	15030	9.705	ug/L	95
20) cis-1,2-Dichloroethene	4.652	96	791775	442.623	ug/L	97
25) Chloroform	5.079	83	8946	3.040	ug/L	97
53) m,p-Xylene	9.690	106	5370	1.695	ug/L	97
54) o-xylene	10.102	106	4459	1.423	ug/L	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU033123\
Data File : VU053501.D
Acq On : 31 Mar 2023 18:58
Operator : JC/MD
Sample : 02121-07ME
Misc : 5.46g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C1180ME

Manual IntegrationsAPPROVED

Quant Time: Apr 01 05:09:10 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 01 04:51:17 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 04/03/2023
Supervised By :Mahesh Dadoda 04/03/2023

