

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU033123\
 Data File : VU053495.D
 Acq On : 31 Mar 2023 16:36
 Operator : JC/MD
 Sample : 02037-02DL2 1000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45E5DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053495.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	91	rBV	155392	177616	17.28%	2.166%
2	1.909	169	177	192	rVB	115376	154831	15.06%	1.888%
3	2.562	368	380	397	rBV	242604	391365	38.08%	4.773%
4	3.041	519	529	541	rBV2	7577	14436	1.40%	0.176%
5	3.105	547	549	550	rBV2	191	70	0.01%	0.001%
6	3.437	650	652	659	rBV	288	247	0.02%	0.003%
7	3.472	662	663	664	rBV	224	76	0.01%	0.001%
8	3.848	776	780	783	rBV3	352	266	0.03%	0.003%
9	4.028	834	836	838	rBV2	281	175	0.02%	0.002%
10	4.202	888	890	892	rBV	170	112	0.01%	0.001%
11	4.498	979	982	984	rBV	239	133	0.01%	0.002%
12	4.514	985	987	989	rBV	193	83	0.01%	0.001%
13	4.613	1006	1018	1021	rBV	84618	136570	13.29%	1.666%
14	4.954	1123	1124	1127	rBV	322	122	0.01%	0.001%
15	4.980	1130	1132	1136	rVB	323	171	0.02%	0.002%
16	5.002	1136	1139	1140	rBV	267	144	0.01%	0.002%
17	5.057	1140	1156	1177	rBV	193445	422785	41.13%	5.157%
18	5.244	1211	1214	1218	rVB3	471	303	0.03%	0.004%
19	5.427	1269	1271	1275	rVB3	285	167	0.02%	0.002%
20	5.469	1282	1284	1287	rBV	164	67	0.01%	0.001%
21	5.594	1321	1323	1326	rVB	220	75	0.01%	0.001%
22	5.719	1340	1362	1390	rBV2	373744	1027809	100.00%	12.536%
23	5.990	1444	1446	1447	rBV	93	19	0.00%	0.000%
24	6.035	1457	1460	1465	rBV3	417	432	0.04%	0.005%
25	6.147	1493	1495	1498	rBV	168	65	0.01%	0.001%
26	6.186	1505	1507	1509	rBV	192	70	0.01%	0.001%
27	6.244	1510	1525	1553	rBV	329323	632313	61.52%	7.712%
28	6.478	1596	1598	1604	rBV2	290	229	0.02%	0.003%
29	6.530	1604	1614	1626	rVB8	7369	16156	1.57%	0.197%
30	6.575	1626	1628	1631	rVB	463	236	0.02%	0.003%
31	6.588	1631	1632	1633	rBV	220	72	0.01%	0.001%
32	6.597	1633	1635	1638	rBV	254	130	0.01%	0.002%
33	6.626	1641	1644	1646	rVB	349	215	0.02%	0.003%
34	6.684	1646	1662	1680	rBV	231426	451922	43.97%	5.512%
35	6.880	1721	1723	1726	rBV	191	123	0.01%	0.002%
36	6.903	1726	1730	1734	rVB	275	188	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU033123\
 Data File : VU053495.D
 Acq On : 31 Mar 2023 16:36
 Operator : JC/MD
 Sample : 02037-02DL2 1000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45E5DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	6.989	1754	1757	1758	rBV	161	94	0.01%	0.001%
38	7.054	1774	1777	1779	rBV	172	110	0.01%	0.001%
39	7.166	1810	1812	1816	rBV	211	136	0.01%	0.002%
40	7.186	1816	1818	1821	rVV	454	233	0.02%	0.003%
41	7.231	1831	1832	1834	rBV	109	62	0.01%	0.001%
42	7.424	1889	1892	1894	rBV	189	123	0.01%	0.002%
43	7.478	1907	1909	1912	rBV	240	111	0.01%	0.001%
44	7.559	1922	1934	1959	rBV	135407	242517	23.60%	2.958%
45	7.729	1986	1987	1988	rBV	212	74	0.01%	0.001%
46	7.748	1988	1993	1996	rVV2	297	340	0.03%	0.004%
47	7.764	1996	1998	2001	rVV	248	136	0.01%	0.002%
48	7.893	2024	2038	2069	rBV	512766	889177	86.51%	10.845%
49	8.128	2109	2111	2114	rBV	194	75	0.01%	0.001%
50	8.176	2114	2126	2149	rVV	94253	162565	15.82%	1.983%
51	8.350	2178	2180	2185	rVB	288	156	0.02%	0.002%
52	8.404	2194	2197	2200	rBV	291	211	0.02%	0.003%
53	8.446	2208	2210	2213	rBV	274	144	0.01%	0.002%
54	8.549	2233	2242	2252	rBV4	11000	17433	1.70%	0.213%
55	8.626	2255	2266	2301	rBV2	240117	443703	43.17%	5.412%
56	8.829	2326	2329	2331	rBB2	257	120	0.01%	0.001%
57	8.861	2336	2339	2343	rVB	380	236	0.02%	0.003%
58	8.944	2363	2365	2367	rBV2	256	98	0.01%	0.001%
59	9.022	2387	2389	2392	rVB	247	122	0.01%	0.001%
60	9.411	2496	2510	2536	rBV	462126	767206	74.64%	9.357%
61	9.604	2568	2570	2572	rBV	219	92	0.01%	0.001%
62	9.694	2591	2598	2604	rBV2	1332	1845	0.18%	0.023%
63	10.231	2763	2765	2767	rVB	302	102	0.01%	0.001%
64	10.485	2837	2844	2853	rVB4	1160	1710	0.17%	0.021%
65	10.523	2853	2856	2860	rBV2	223	177	0.02%	0.002%
66	10.636	2888	2891	2899	rBV3	453	435	0.04%	0.005%
67	10.751	2915	2927	2947	rVB	330179	533672	51.92%	6.509%
68	10.893	2969	2971	2978	rBV	264	220	0.02%	0.003%
69	11.433	3132	3139	3142	rBV2	353	426	0.04%	0.005%
70	11.468	3142	3150	3157	rBV4	1664	2140	0.21%	0.026%
71	11.542	3171	3173	3175	rBV	245	97	0.01%	0.001%
72	11.745	3228	3236	3243	rBV5	3219	4361	0.42%	0.053%
73	11.806	3243	3255	3278	rBV	514294	804610	78.28%	9.814%
74	12.189	3360	3374	3392	rBV	535356	868403	84.49%	10.592%
75	12.433	3446	3450	3453	rBV2	349	243	0.02%	0.003%
76	12.501	3468	3471	3473	rBV	335	165	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU033123\
 Data File : VU053495.D
 Acq On : 31 Mar 2023 16:36
 Operator : JC/MD
 Sample : 02037-02DL2 1000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45E5DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M

Title : VOC Analysis

77	12.626	3508	3510	3515	rVB	202	147	0.01%	0.002%
78	12.787	3558	3560	3566	rVB	235	148	0.01%	0.002%
79	12.848	3576	3579	3582	rBV2	361	269	0.03%	0.003%
80	12.931	3602	3605	3607	rBV	271	170	0.02%	0.002%
81	13.221	3688	3695	3705	rBV6	3179	5096	0.50%	0.062%
82	13.327	3724	3728	3732	rVB3	279	265	0.03%	0.003%
83	13.391	3746	3748	3752	rBV	302	225	0.02%	0.003%
84	13.845	3882	3889	3899	rVB4	4699	7506	0.73%	0.092%
85	14.092	3958	3966	3980	rVB3	7289	11404	1.11%	0.139%




Sum of corrected areas: 8198903

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU033123\
Data File : VU053495.D
Acq On : 31 Mar 2023 16:36
Operator : JC/MD
Sample : 02037-02DL2 1000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45E5DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

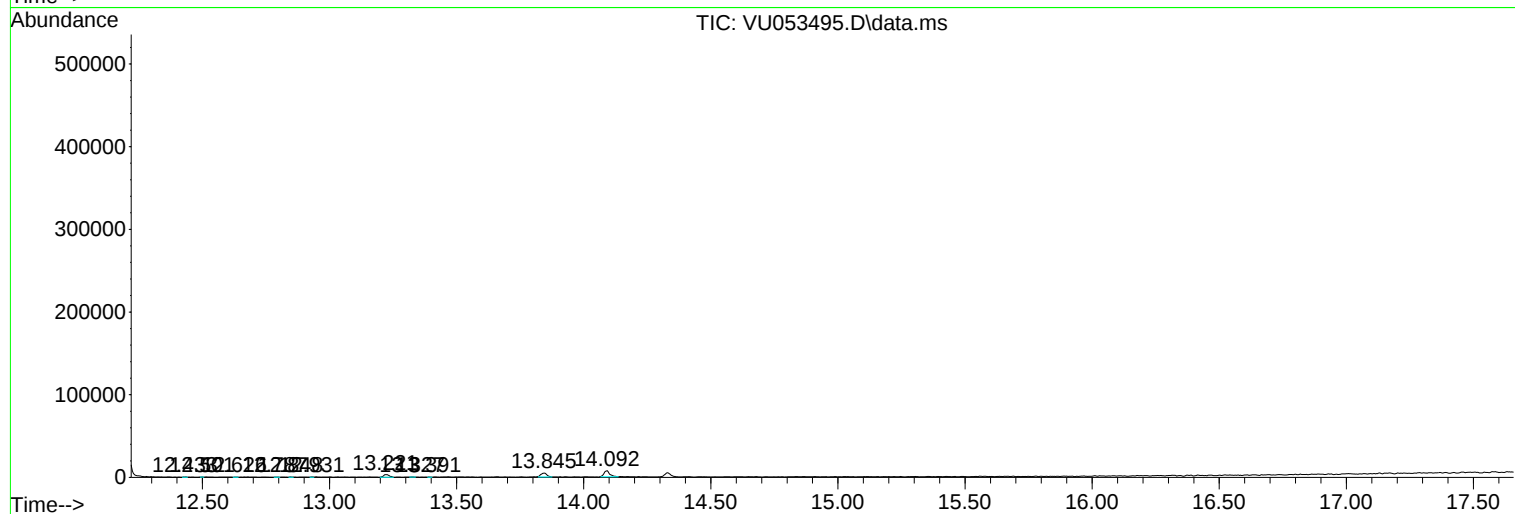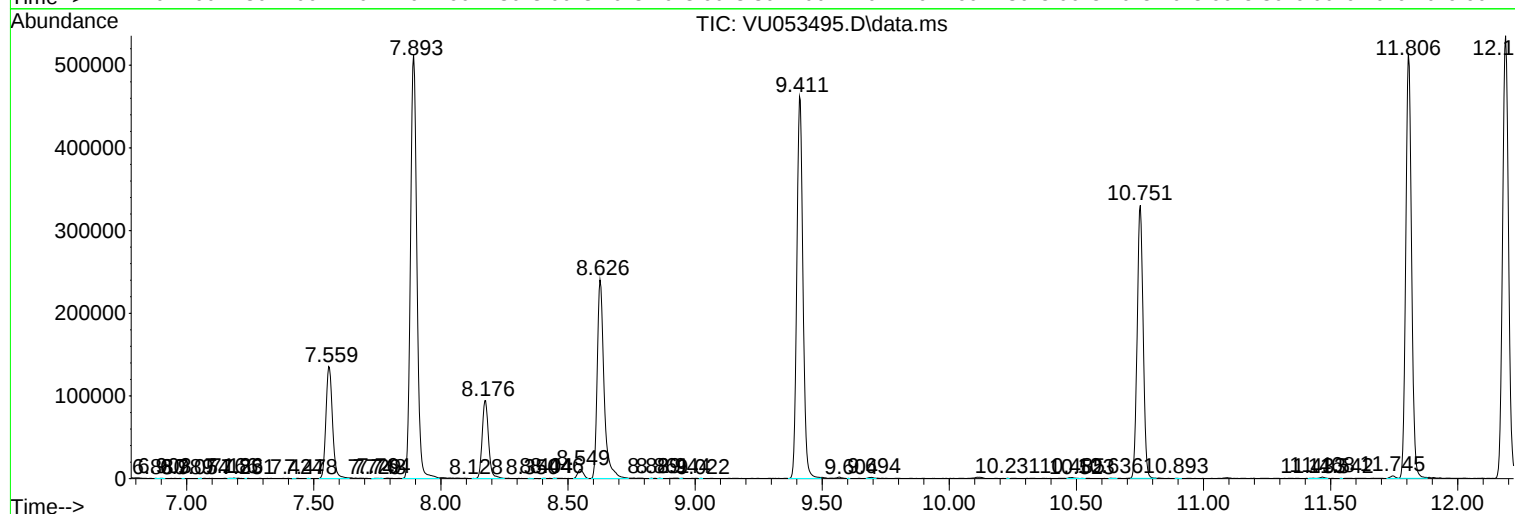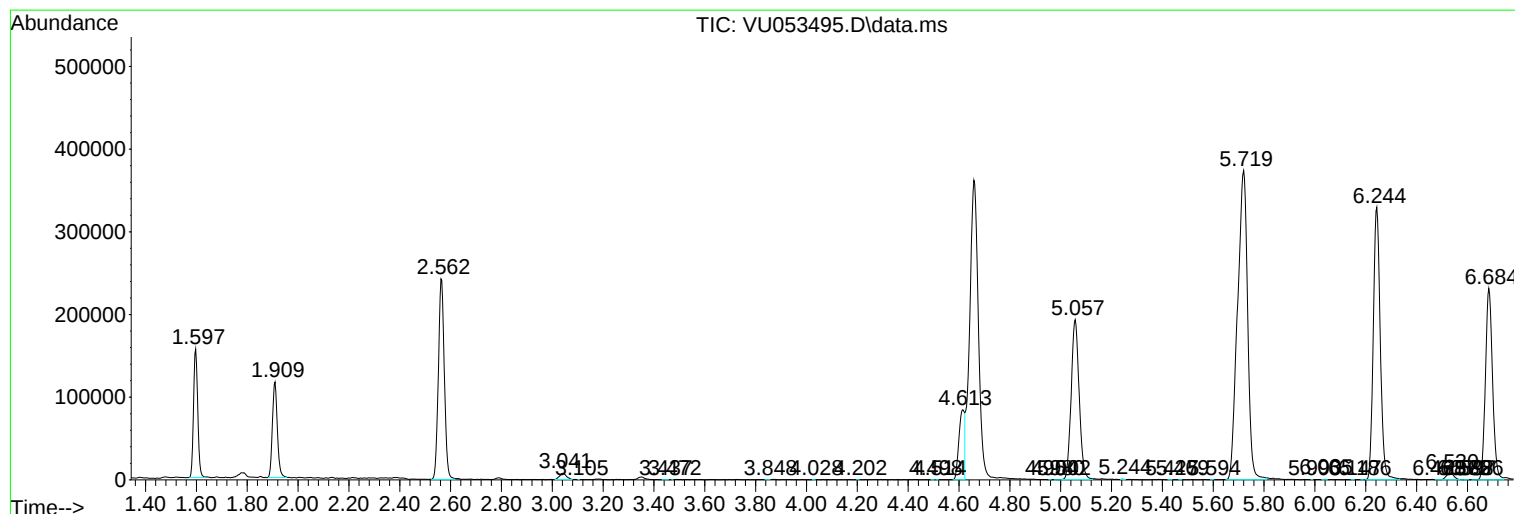

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU033123\
Data File : VU053495.D
Acq On : 31 Mar 2023 16:36
Operator : JC/MD
Sample : 02037-02DL2 1000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45E5DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU033123\
Data File : VU053495.D
Acq On : 31 Mar 2023 16:36
Operator : JC/MD
Sample : 02037-02DL2 1000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45E5DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------