

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU033123\
 Data File : VU053497.D
 Acq On : 31 Mar 2023 17:23
 Operator : JC/MD
 Sample : 02054-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053497.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	91	rVB	155755	172001	17.31%	2.244%
2	1.909	169	177	192	rBV	113717	150564	15.15%	1.965%
3	2.562	369	380	396	rBV	229768	376073	37.85%	4.907%
4	2.739	434	435	437	rBV2	471	267	0.03%	0.003%
5	2.858	468	472	475	rBV	299	231	0.02%	0.003%
6	3.041	521	529	539	rVB5	2024	3475	0.35%	0.045%
7	3.160	562	566	567	rBV	907	639	0.06%	0.008%
8	3.298	605	609	610	rBV	244	173	0.02%	0.002%
9	3.350	621	625	626	rBV3	577	440	0.04%	0.006%
10	3.700	728	734	737	rBV2	459	384	0.04%	0.005%
11	3.771	753	756	759	rBV	299	191	0.02%	0.002%
12	4.250	901	905	907	rBV	222	176	0.02%	0.002%
13	4.282	912	915	921	rBV2	303	317	0.03%	0.004%
14	4.613	1006	1018	1046	rBV	77939	192367	19.36%	2.510%
15	5.057	1140	1156	1177	rBV	190309	418131	42.08%	5.456%
16	5.237	1209	1212	1214	rBV	236	158	0.02%	0.002%
17	5.253	1214	1217	1223	rVB4	534	479	0.05%	0.006%
18	5.292	1224	1229	1232	rBV	412	287	0.03%	0.004%
19	5.543	1302	1307	1309	rBV2	275	222	0.02%	0.003%
20	5.616	1322	1330	1335	rBB2	228	264	0.03%	0.003%
21	5.719	1340	1362	1385	rBV2	365594	993544	100.00%	12.965%
22	6.044	1454	1463	1467	rVB2	405	530	0.05%	0.007%
23	6.115	1478	1485	1489	rBB2	320	315	0.03%	0.004%
24	6.182	1503	1506	1512	rBV2	216	241	0.02%	0.003%
25	6.243	1512	1525	1546	rBV	265679	510251	51.36%	6.658%
26	6.530	1604	1614	1625	rVB7	4652	9341	0.94%	0.122%
27	6.587	1625	1632	1634	rBV	294	207	0.02%	0.003%
28	6.684	1646	1662	1680	rBV	224302	438142	44.10%	5.717%
29	6.954	1741	1746	1749	rBV2	212	195	0.02%	0.003%
30	7.012	1759	1764	1766	rBV	207	204	0.02%	0.003%
31	7.160	1807	1810	1813	rVV	265	158	0.02%	0.002%
32	7.189	1814	1819	1825	rVV	641	640	0.06%	0.008%
33	7.301	1849	1854	1858	rVV2	196	197	0.02%	0.003%
34	7.346	1864	1868	1871	rBV	289	258	0.03%	0.003%
35	7.427	1890	1893	1899	rBV2	258	209	0.02%	0.003%
36	7.459	1899	1903	1909	rVB2	296	315	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU033123\
 Data File : VU053497.D
 Acq On : 31 Mar 2023 17:23
 Operator : JC/MD
 Sample : 02054-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.562	1922	1935	1952	rBV	132071	233433	23.49%	3.046%
38	7.690	1973	1975	1979	rVB3	524	314	0.03%	0.004%
39	7.742	1988	1991	1996	rBV2	342	292	0.03%	0.004%
40	7.787	2002	2005	2007	rBV	357	239	0.02%	0.003%
41	7.893	2024	2038	2056	rBV	502877	857700	86.33%	11.192%
42	8.092	2099	2100	2103	rVB2	548	213	0.02%	0.003%
43	8.112	2103	2106	2112	rVB	275	193	0.02%	0.003%
44	8.176	2113	2126	2144	rBV	90045	155672	15.67%	2.031%
45	8.330	2170	2174	2176	rBV2	301	170	0.02%	0.002%
46	8.472	2209	2218	2227	rVB4	933	1430	0.14%	0.019%
47	8.549	2238	2242	2248	rVB5	1202	1473	0.15%	0.019%
48	8.626	2255	2266	2295	rBV	227336	423669	42.64%	5.528%
49	8.829	2324	2329	2332	rBV2	229	181	0.02%	0.002%
50	8.989	2377	2379	2383	rVB	299	186	0.02%	0.002%
51	9.066	2396	2403	2409	rVB	346	357	0.04%	0.005%
52	9.160	2425	2432	2435	rBV2	337	379	0.04%	0.005%
53	9.414	2498	2511	2533	rBV	372455	618160	62.22%	8.066%
54	9.758	2614	2618	2623	rBV2	175	169	0.02%	0.002%
55	9.922	2666	2669	2673	rBV	259	184	0.02%	0.002%
56	9.944	2673	2676	2680	rVB	328	226	0.02%	0.003%
57	10.105	2722	2726	2727	rBV2	625	490	0.05%	0.006%
58	10.182	2742	2750	2753	rBV	358	370	0.04%	0.005%
59	10.340	2796	2799	2802	rVB	273	178	0.02%	0.002%
60	10.365	2802	2807	2809	rBV	301	233	0.02%	0.003%
61	10.478	2837	2842	2852	rVB2	1193	1567	0.16%	0.020%
62	10.562	2864	2868	2871	rBV	302	174	0.02%	0.002%
63	10.619	2883	2886	2888	rBV	295	163	0.02%	0.002%
64	10.751	2915	2927	2944	rBV	330420	523651	52.71%	6.833%
65	10.861	2957	2961	2964	rBV2	352	241	0.02%	0.003%
66	10.964	2989	2993	2998	rBV2	444	354	0.04%	0.005%
67	11.137	3044	3047	3050	rBV	364	258	0.03%	0.003%
68	11.176	3054	3059	3064	rVB2	339	330	0.03%	0.004%
69	11.288	3081	3094	3101	rBV3	2740	3772	0.38%	0.049%
70	11.362	3113	3117	3120	rBV	278	205	0.02%	0.003%
71	11.465	3139	3149	3161	rBV2	12422	18085	1.82%	0.236%
72	11.562	3176	3179	3182	rBV	243	246	0.02%	0.003%
73	11.616	3191	3196	3200	rBV	208	248	0.02%	0.003%
74	11.636	3200	3202	3205	rVV	417	279	0.03%	0.004%
75	11.661	3209	3210	3215	rVB	308	170	0.02%	0.002%
76	11.745	3229	3236	3243	rBV4	1852	2685	0.27%	0.035%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU033123\
 Data File : VU053497.D
 Acq On : 31 Mar 2023 17:23
 Operator : JC/MD
 Sample : 02054-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

77	11.806	3243	3255	3274	rBV	409684	660012	66.43%	8.613%
78	12.086	3339	3342	3343	rBV2	1054	549	0.06%	0.007%
79	12.189	3359	3374	3395	rBV	514626	836459	84.19%	10.915%
80	12.298	3406	3408	3415	rVB3	570	540	0.05%	0.007%
81	12.533	3478	3481	3484	rVB2	286	186	0.02%	0.002%
82	12.568	3484	3492	3502	rBV2	3273	4729	0.48%	0.062%
83	12.607	3502	3504	3507	rBV	270	167	0.02%	0.002%
84	12.748	3542	3548	3553	rBV	281	370	0.04%	0.005%
85	12.822	3567	3571	3574	rBV2	263	271	0.03%	0.004%
86	12.873	3582	3587	3591	rBV3	512	538	0.05%	0.007%
87	12.970	3610	3617	3627	rBV5	1749	3059	0.31%	0.040%
88	13.025	3627	3634	3643	rVV4	2131	3261	0.33%	0.043%
89	13.079	3647	3651	3652	rBV	270	182	0.02%	0.002%
90	13.111	3657	3661	3663	rBV	460	291	0.03%	0.004%
91	13.221	3689	3695	3704	rBV3	1926	2882	0.29%	0.038%
92	13.333	3728	3730	3734	rBV2	277	191	0.02%	0.002%
93	13.452	3759	3767	3776	rVB4	3356	5738	0.58%	0.075%
94	13.520	3785	3788	3792	rBV2	300	213	0.02%	0.003%
95	13.841	3880	3888	3899	rVV5	4454	6665	0.67%	0.087%
96	13.934	3915	3917	3919	rBV2	524	284	0.03%	0.004%
97	14.089	3957	3965	3979	rBV2	6056	11015	1.11%	0.144%
98	14.330	4034	4040	4051	rVB7	3278	5169	0.52%	0.067%
99	14.529	4099	4102	4104	rBV2	447	276	0.03%	0.004%
100	15.143	4291	4293	4296	rBV2	591	394	0.04%	0.005%




Sum of corrected areas: 7663366

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU033123\
Data File : VU053497.D
Acq On : 31 Mar 2023 17:23
Operator : JC/MD
Sample : 02054-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

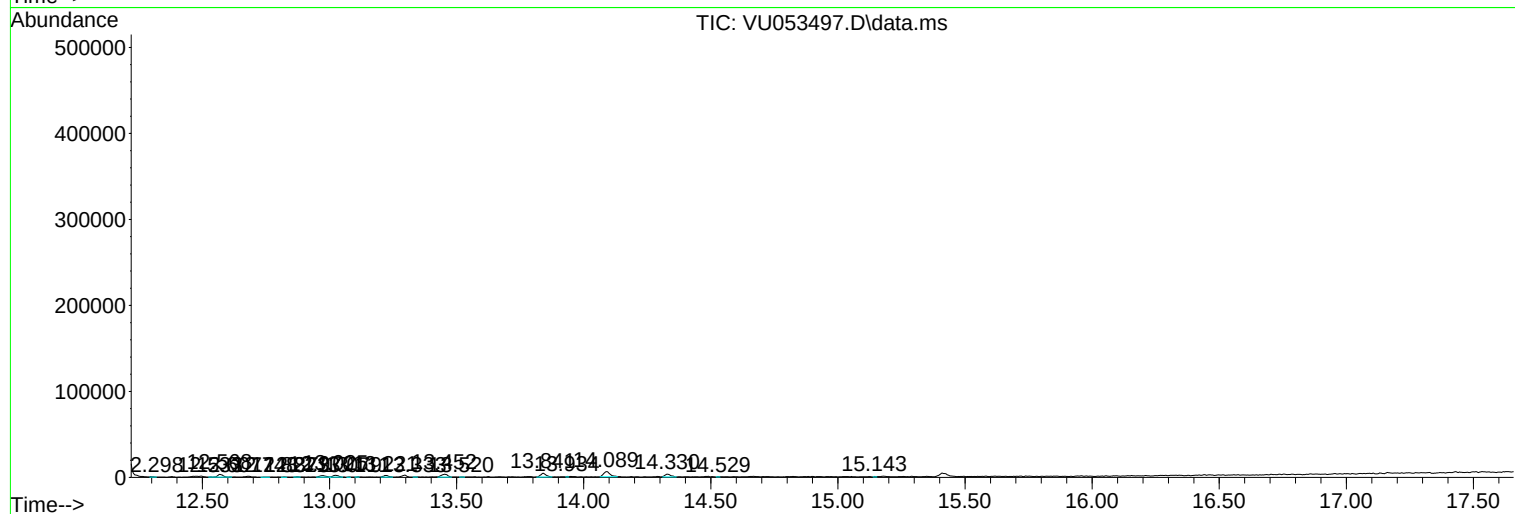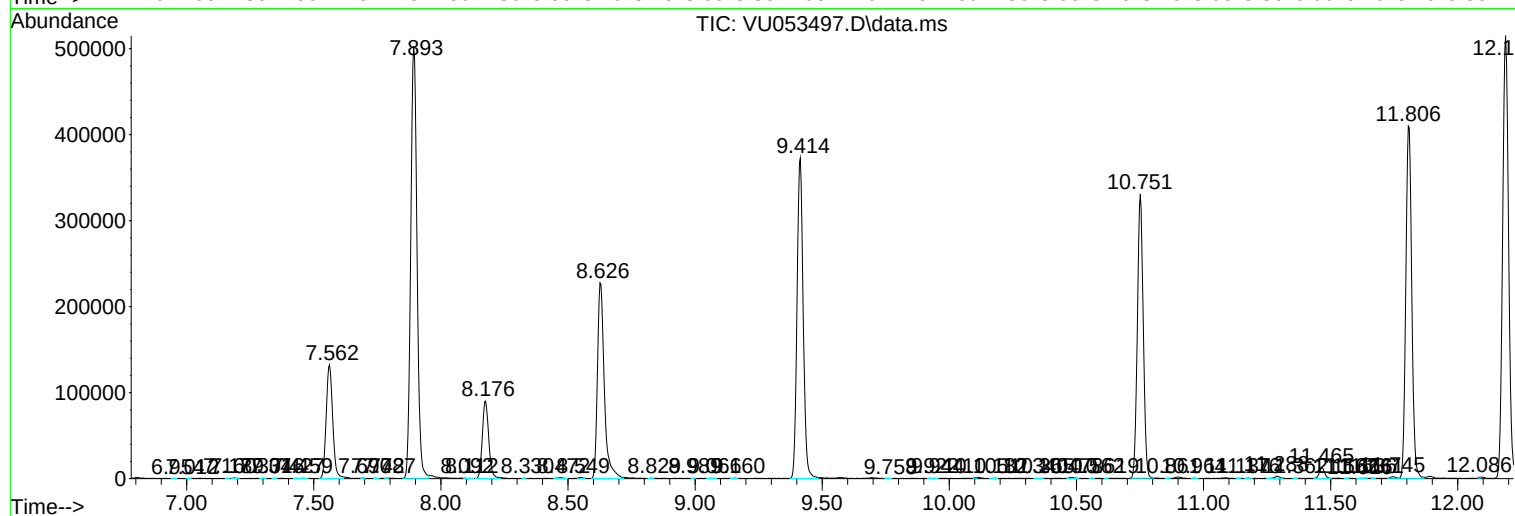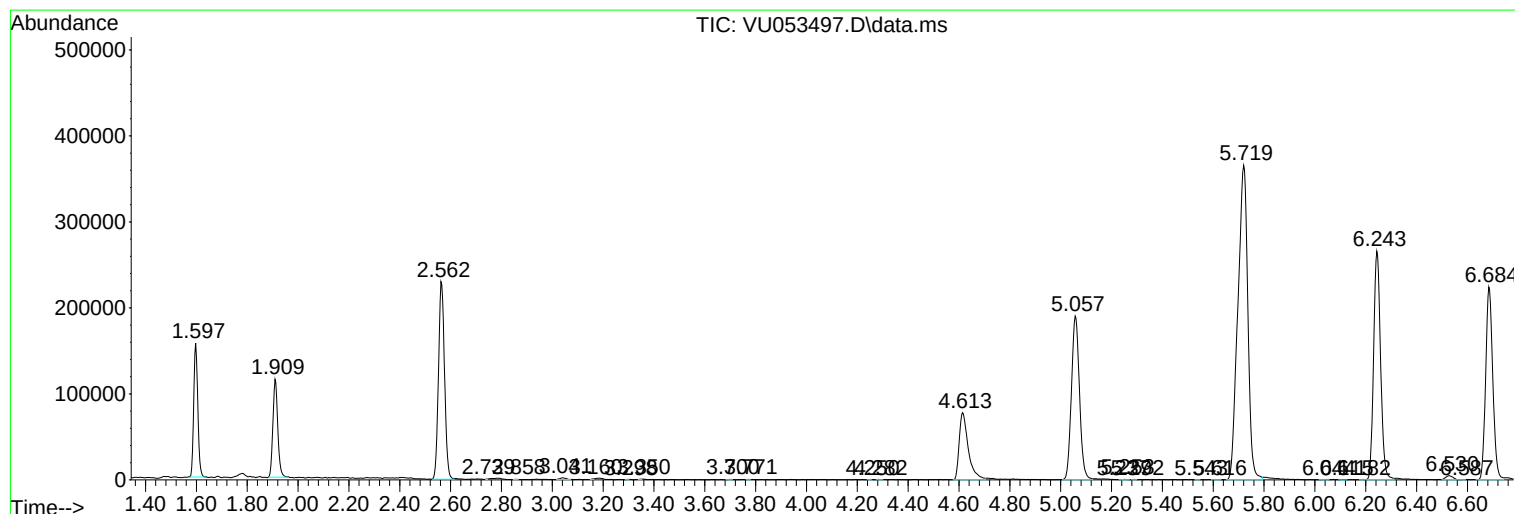

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU033123\
Data File : VU053497.D
Acq On : 31 Mar 2023 17:23
Operator : JC/MD
Sample : 02054-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU033123\
Data File : VU053497.D
Acq On : 31 Mar 2023 17:23
Operator : JC/MD
Sample : 02054-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------