

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU033123\
 Data File : VU053498.D
 Acq On : 31 Mar 2023 17:47
 Operator : JC/MD
 Sample : 02037-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053498.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.598	73	80	91	rVB	150586	169730	17.11%	2.189%
2	1.909	169	177	194	rVB	112578	153871	15.52%	1.985%
3	2.562	368	380	404	rVB	231669	378285	38.14%	4.879%
4	2.652	404	408	410	rBV2	502	372	0.04%	0.005%
5	3.038	521	528	539	rVB5	1876	3296	0.33%	0.043%
6	3.482	664	666	670	rVB	414	188	0.02%	0.002%
7	3.732	742	744	745	rBV	214	65	0.01%	0.001%
8	3.938	807	808	810	rBV	293	100	0.01%	0.001%
9	4.073	849	850	853	rBV	167	91	0.01%	0.001%
10	4.205	887	891	894	rBV2	254	281	0.03%	0.004%
11	4.292	915	918	920	rBV	260	192	0.02%	0.002%
12	4.523	988	990	991	rBV	155	78	0.01%	0.001%
13	4.613	1007	1018	1047	rBV	75748	185937	18.75%	2.398%
14	4.970	1123	1129	1134	rBV	213	314	0.03%	0.004%
15	5.057	1141	1156	1181	rBV	187370	410483	41.39%	5.294%
16	5.263	1217	1220	1222	rBV	260	203	0.02%	0.003%
17	5.330	1238	1241	1246	rBV	244	187	0.02%	0.002%
18	5.646	1337	1339	1341	rVB	192	77	0.01%	0.001%
19	5.720	1341	1362	1397	rBV3	362879	991754	100.00%	12.791%
20	6.054	1463	1466	1471	rBV2	291	280	0.03%	0.004%
21	6.118	1482	1486	1488	rBV2	299	271	0.03%	0.003%
22	6.147	1494	1495	1496	rVB	112	22	0.00%	0.000%
23	6.244	1512	1525	1546	rBV	296261	560685	56.53%	7.231%
24	6.530	1605	1614	1625	rVB5	4588	8531	0.86%	0.110%
25	6.607	1636	1638	1639	rBV	240	96	0.01%	0.001%
26	6.626	1640	1644	1645	rBV	153	94	0.01%	0.001%
27	6.684	1648	1662	1681	rBV	219878	432957	43.66%	5.584%
28	6.948	1741	1744	1747	rBV	217	225	0.02%	0.003%
29	6.974	1750	1752	1755	rVV	126	73	0.01%	0.001%
30	7.006	1759	1762	1763	rBV	168	77	0.01%	0.001%
31	7.083	1783	1786	1788	rBV	174	115	0.01%	0.001%
32	7.186	1813	1818	1820	rBV2	452	412	0.04%	0.005%
33	7.321	1857	1860	1863	rBV	266	196	0.02%	0.003%
34	7.366	1871	1874	1876	rVB	267	144	0.01%	0.002%
35	7.459	1901	1903	1907	rBV	152	54	0.01%	0.001%
36	7.562	1922	1935	1959	rBV	132417	233499	23.54%	3.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU033123\
 Data File : VU053498.D
 Acq On : 31 Mar 2023 17:47
 Operator : JC/MD
 Sample : 02037-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.691	1973	1975	1979	rVB2	369	209	0.02%	0.003%
38	7.800	2007	2009	2013	rVB2	576	353	0.04%	0.005%
39	7.826	2015	2017	2019	rVB	454	195	0.02%	0.003%
40	7.842	2019	2022	2024	rBV	119	82	0.01%	0.001%
41	7.893	2024	2038	2069	rBV	488457	854461	86.16%	11.020%
42	8.173	2114	2125	2143	rBV	91660	156724	15.80%	2.021%
43	8.401	2194	2196	2198	rBV	168	49	0.00%	0.001%
44	8.414	2198	2200	2205	rBV2	268	207	0.02%	0.003%
45	8.469	2208	2217	2226	rVV2	3484	5612	0.57%	0.072%
46	8.523	2232	2234	2235	rBV2	112	51	0.01%	0.001%
47	8.552	2238	2243	2248	rBV4	1445	1331	0.13%	0.017%
48	8.626	2255	2266	2298	rBV	233135	428963	43.25%	5.533%
49	9.160	2430	2432	2434	rBV2	178	93	0.01%	0.001%
50	9.237	2453	2456	2457	rBV	206	124	0.01%	0.002%
51	9.414	2498	2511	2532	rBV	406374	680425	68.61%	8.776%
52	9.565	2554	2558	2566	rVB5	1066	1191	0.12%	0.015%
53	9.642	2578	2582	2585	rBV	370	295	0.03%	0.004%
54	9.690	2593	2597	2599	rBV2	945	646	0.07%	0.008%
55	9.787	2623	2627	2631	rVB	460	399	0.04%	0.005%
56	9.899	2660	2662	2664	rVB	238	101	0.01%	0.001%
57	9.944	2674	2676	2680	rBV	206	107	0.01%	0.001%
58	10.192	2749	2753	2757	rBV2	260	257	0.03%	0.003%
59	10.234	2765	2766	2769	rVB	280	131	0.01%	0.002%
60	10.481	2839	2843	2852	rVB2	880	1070	0.11%	0.014%
61	10.633	2888	2890	2891	rBV	204	66	0.01%	0.001%
62	10.751	2915	2927	2945	rBV2	322976	521039	52.54%	6.720%
63	10.887	2964	2969	2981	rVB4	4110	5817	0.59%	0.075%
64	11.002	3002	3005	3007	rBV	200	99	0.01%	0.001%
65	11.234	3074	3077	3079	rBV	250	150	0.02%	0.002%
66	11.469	3142	3150	3159	rVB	3163	4364	0.44%	0.056%
67	11.626	3198	3199	3202	rBV	206	101	0.01%	0.001%
68	11.674	3210	3214	3215	rBV	316	224	0.02%	0.003%
69	11.745	3230	3236	3242	rBV3	1494	1613	0.16%	0.021%
70	11.806	3243	3255	3272	rBV	443619	707823	71.37%	9.129%
71	12.189	3361	3374	3397	rBV	521944	830740	83.76%	10.714%
72	12.343	3419	3422	3426	rBB2	339	244	0.02%	0.003%
73	12.706	3533	3535	3537	rVV	273	129	0.01%	0.002%
74	12.716	3537	3538	3539	rVB	254	49	0.00%	0.001%
75	13.115	3659	3662	3664	rBV	280	207	0.02%	0.003%
76	13.218	3688	3694	3706	rVB5	2244	3572	0.36%	0.046%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU033123\
Data File : VU053498.D
Acq On : 31 Mar 2023 17:47
Operator : JC/MD
Sample : 02037-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Title : VOC Analysis

77	13.295	3712	3718	3725	rBV4	672	965	0.10%	0.012%
78	13.636	3821	3824	3828	rBV2	350	242	0.02%	0.003%
79	13.841	3881	3888	3898	rVB8	3551	5699	0.57%	0.074%
80	14.333	4034	4041	4052	rVB4	2605	4029	0.41%	0.052%




Sum of corrected areas: 7753483

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU033123\
Data File : VU053498.D
Acq On : 31 Mar 2023 17:47
Operator : JC/MD
Sample : 02037-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

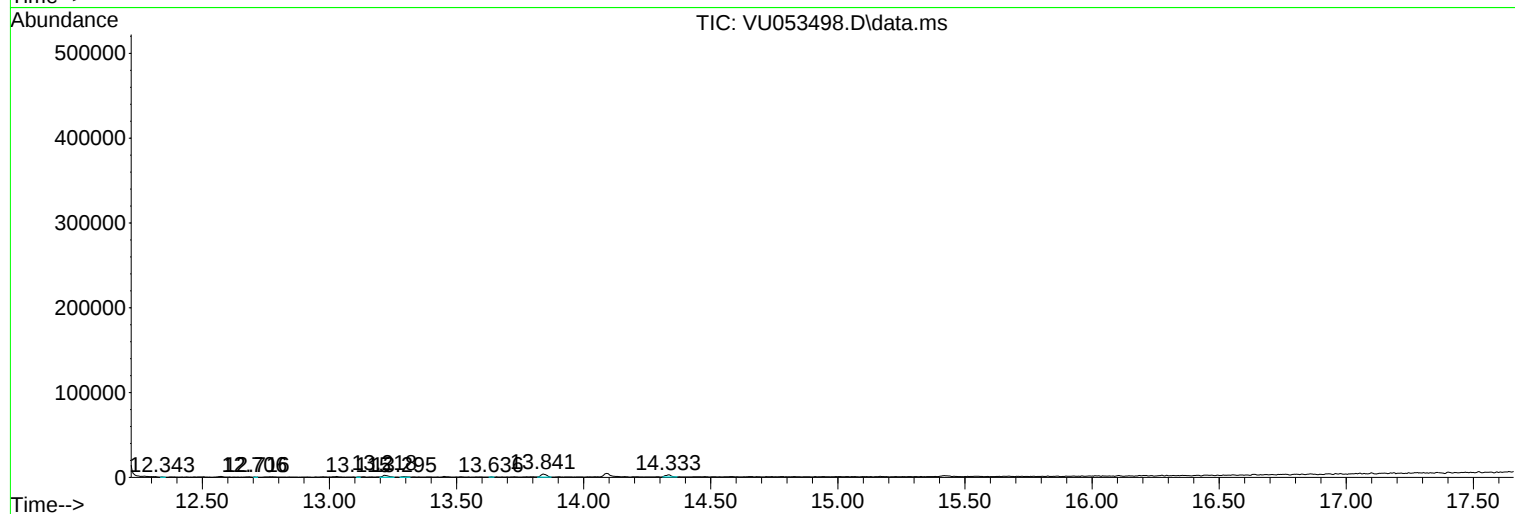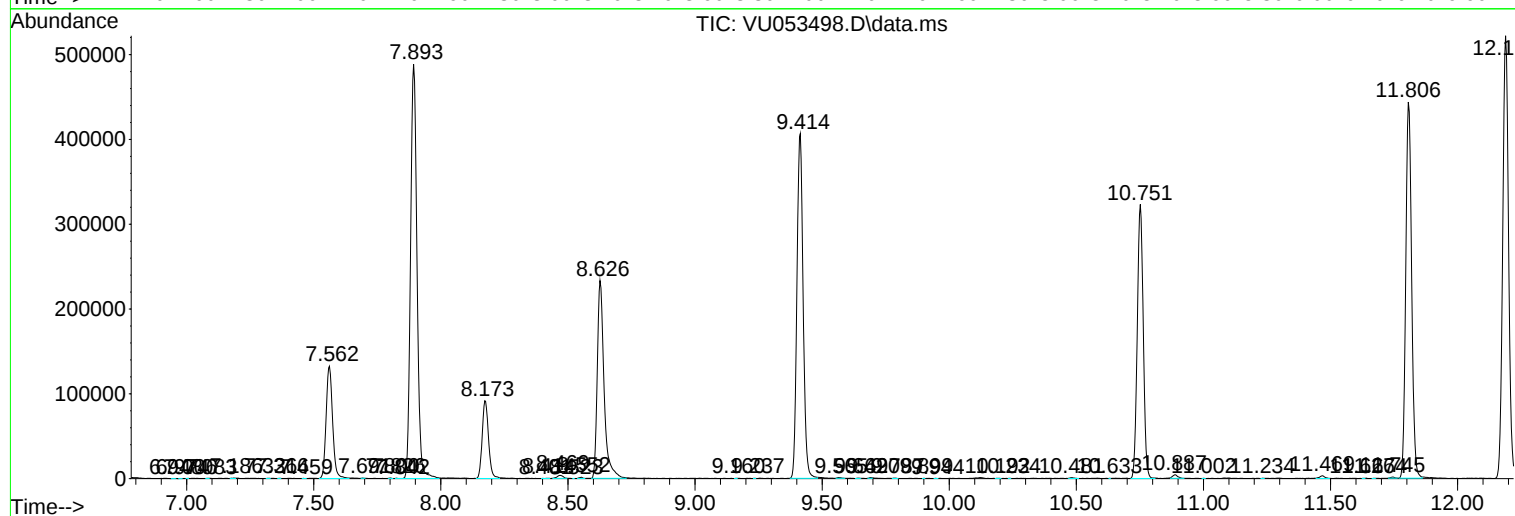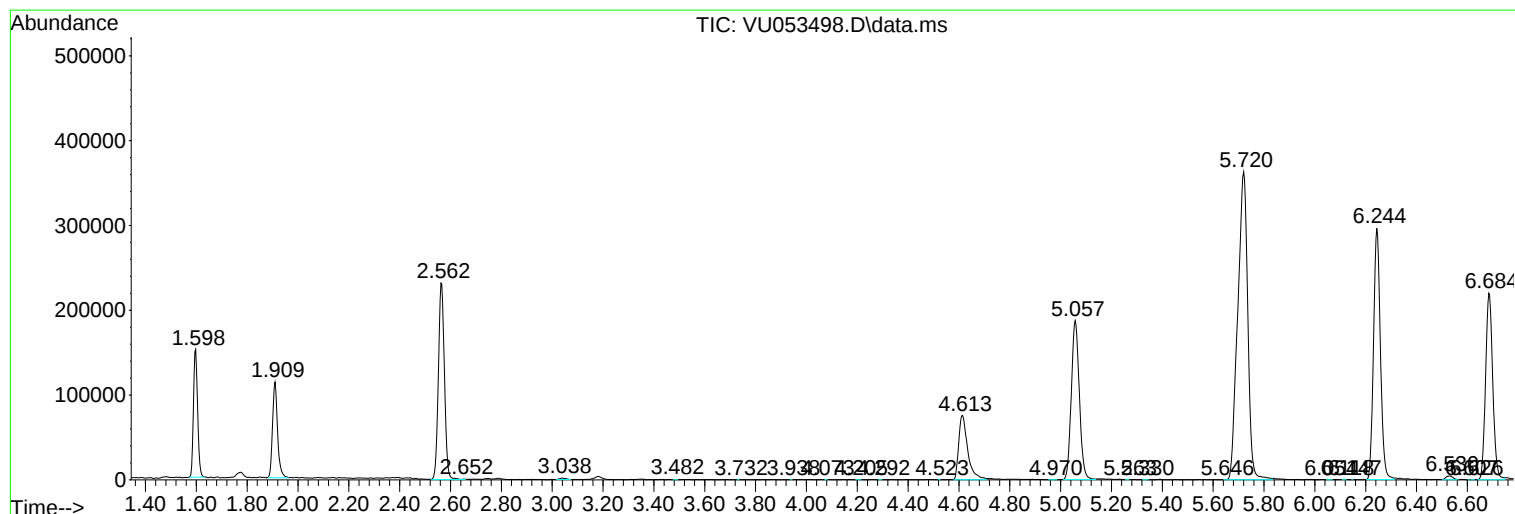

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU033123\
Data File : VU053498.D
Acq On : 31 Mar 2023 17:47
Operator : JC/MD
Sample : 02037-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU033123\
Data File : VU053498.D
Acq On : 31 Mar 2023 17:47
Operator : JC/MD
Sample : 02037-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------