


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU033123\
Data File : VU053486.D
Acq On : 31 Mar 2023 12:01
Operator : JC/MD
Sample : BFB171
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB171

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Title : VOC Analysis
Last Update : Sat Apr 01 04:51:17 2023

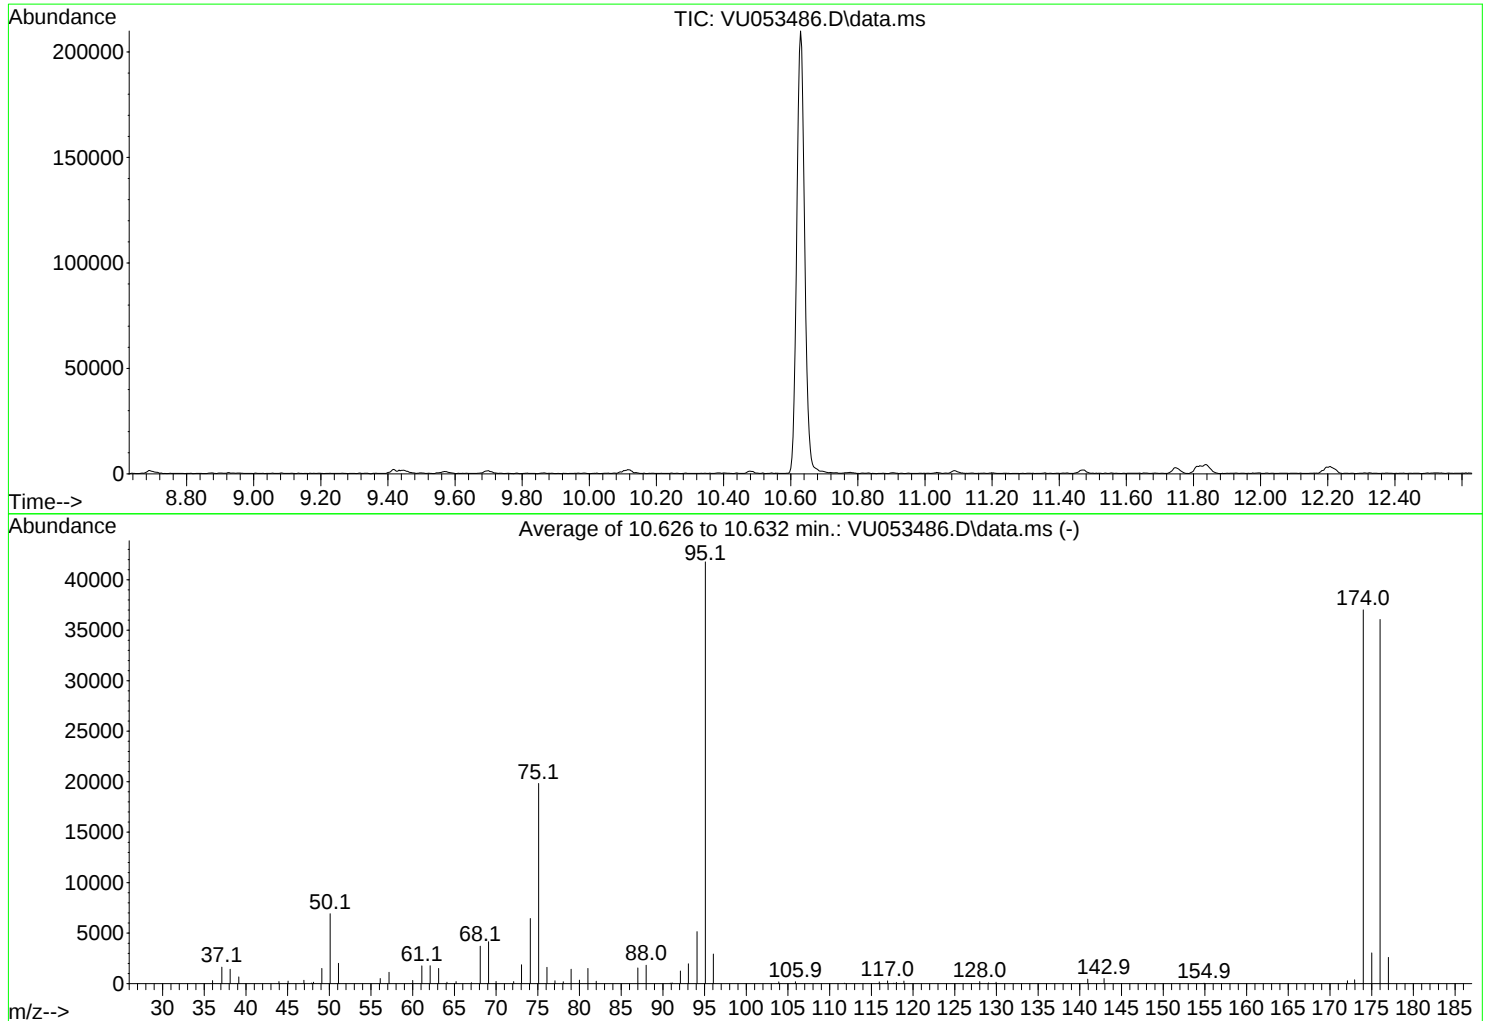

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2877

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.6	6919	PASS
75	95	30	80	47.4	19819	PASS
95	95	100	100	100.0	41773	PASS
96	95	5	9	7.0	2932	PASS
173	174	0.00	2	1.0	374	PASS
174	95	50	120	88.6	37019	PASS
175	174	5	9	8.2	3038	PASS
176	174	95	101	97.4	36064	PASS
177	176	5	9	7.2	2597	PASS

m/z	Abundance
40.10	122.0
44.10	190.0

Instrument :
MSVOA_U
ClientSampleId :
BFB171

m/z	Abundance
36.00	272.0
37.10	1562.0
38.10	1324.0
39.20	622.0
44.00	328.0
45.10	236.0
47.00	434.0
47.90	211.0
49.10	1572.0
50.10	7056.0
51.10	2032.0
56.10	467.0
57.20	1084.0
60.00	289.0
61.10	1777.0
62.10	1793.0
63.10	1370.0
64.10	159.0
65.20	193.0
67.00	148.0
68.10	3788.0
69.10	3959.0
70.00	229.0
72.10	180.0
73.00	1925.0
74.10	6760.0
75.10	19304.0
76.10	1585.0
77.00	236.0
78.00	193.0
79.00	1426.0
79.90	363.0
81.00	1399.0
82.00	248.0
87.00	1484.0
88.00	1787.0
90.90	152.0
92.10	1256.0
93.00	2068.0
94.10	5245.0
95.10	41008.0
96.00	2900.0
104.00	209.0
105.90	135.0
111.80	129.0
115.90	148.0
117.00	287.0
118.00	184.0
118.90	283.0
128.00	232.0
130.00	131.0
141.00	522.0
142.90	430.0
172.10	264.0
173.00	393.0
174.00	35784.0
175.00	2839.0
176.00	34656.0
177.00	2600.0

Instrument :
MSVOA_U
ClientSampleId :
BFB171

m/z	Abundance
36.00	313.0
37.10	1683.0
38.10	1471.0
39.20	681.0
43.90	404.0
45.00	255.0
47.00	317.0
48.10	207.0
49.10	1567.0
50.10	7052.0
51.10	2072.0
56.10	543.0
57.10	1143.0
60.00	329.0
61.10	1802.0
62.10	1808.0
63.10	1559.0
64.10	165.0
65.20	235.0
67.10	149.0
68.10	3780.0
69.10	4299.0
70.00	221.0
72.10	214.0
73.10	1927.0
74.10	6576.0
75.10	20480.0
76.10	1693.0
77.00	292.0
78.00	195.0
79.00	1469.0
80.00	373.0
81.00	1605.0
82.00	258.0
87.00	1581.0
88.00	1930.0
91.10	121.0
92.10	1299.0
93.10	2007.0
94.10	5271.0
95.10	43104.0
96.00	3029.0
103.90	165.0
105.90	213.0
116.00	188.0
116.90	275.0
118.00	186.0
118.90	271.0
128.00	226.0
129.10	120.0
129.90	141.0
141.00	463.0
142.90	537.0
148.00	105.0
172.10	295.0
172.90	412.0
174.00	38016.0
175.00	3090.0
176.00	37048.0
177.00	2677.0

Instrument :
MSVOA_U
ClientSampleId :
BFB171

m/z	Abundance
36.00	338.0
37.10	1679.0
38.10	1485.0
39.10	689.0
40.10	110.0
43.90	459.0
45.00	293.0
46.90	262.0
48.10	218.0
49.10	1398.0
50.10	6648.0
51.10	1957.0
56.10	524.0
57.10	1152.0
60.00	347.0
61.10	1712.0
62.10	1738.0
63.10	1574.0
64.10	122.0
65.20	197.0
68.10	3550.0
69.10	4188.0
70.00	214.0
72.10	240.0
73.00	1747.0
74.10	5991.0
75.10	19672.0
76.10	1562.0
77.10	311.0
78.10	192.0
79.00	1402.0
80.10	330.0
81.00	1520.0
82.00	211.0
87.00	1587.0
88.00	1743.0
91.10	106.0
92.10	1221.0
93.10	1813.0
94.10	4954.0
95.10	41208.0
96.10	2866.0
103.80	175.0
105.90	221.0
116.00	186.0
117.00	251.0
117.70	163.0
118.90	222.0
128.00	179.0
129.00	105.0
129.90	147.0
140.90	345.0
142.90	537.0
154.90	127.0
172.10	318.0
172.90	317.0
174.00	37256.0
175.00	3186.0
176.00	36488.0
177.00	2514.0

Instrument :
MSVOA_U
ClientSampleId :
BFB171