
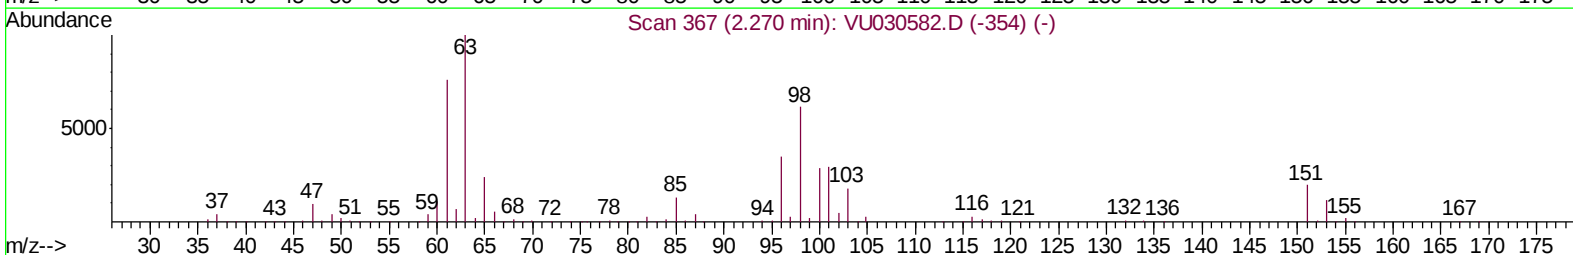
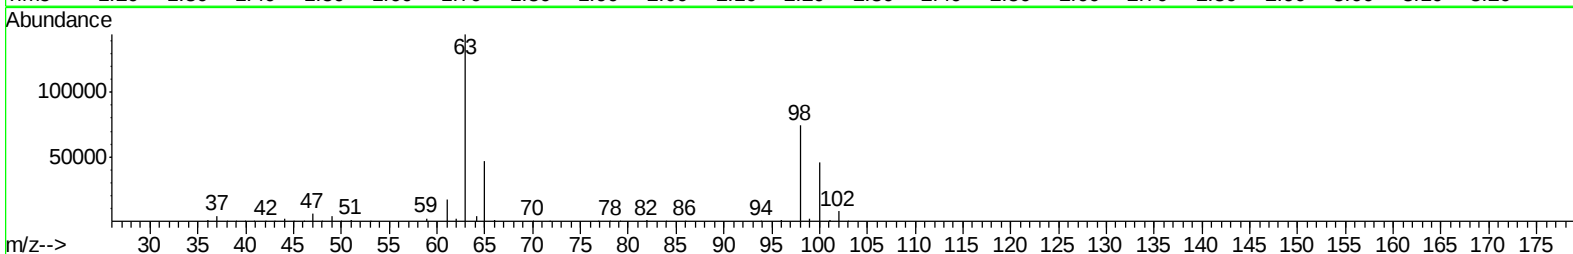


Data File : VU030600.D
Acq On : 31 Mar 2019 19:07
Operator : JC/SP
Sample : K2166-15ME
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Apr 01 02:12:20 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Apr 01 02:05:14 2019
Response via : Initial Calibration

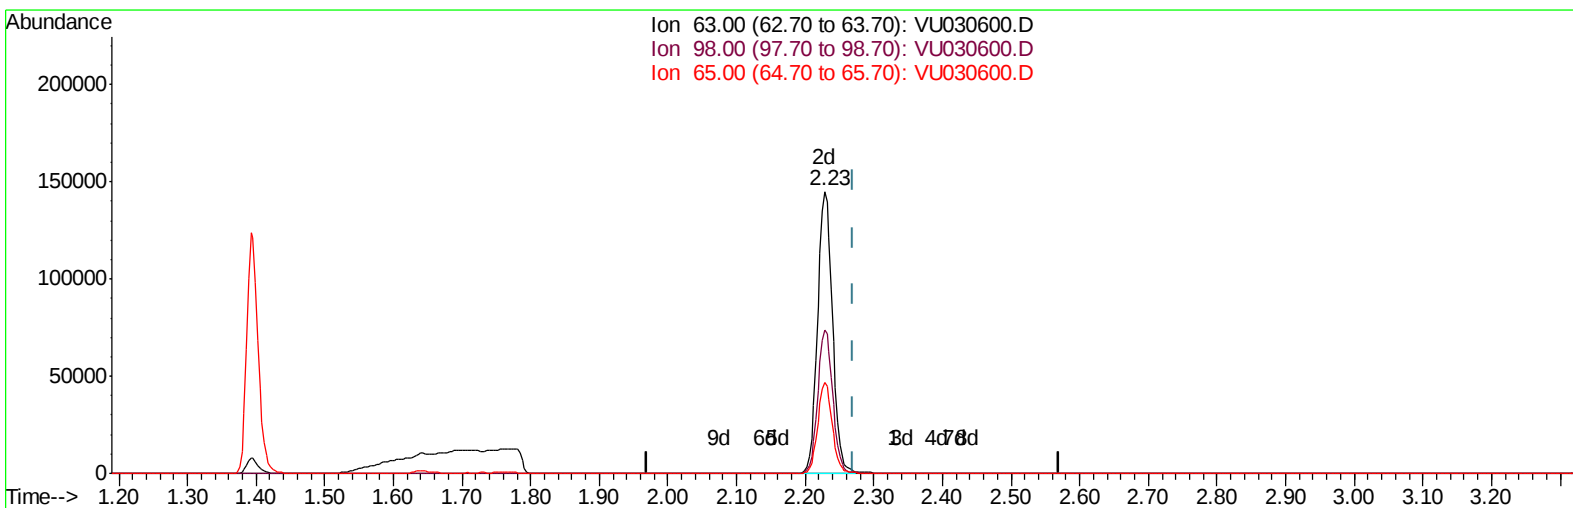

TIC: VU030600.D

(11) 1,1-Dichloroethene-d2 (S)

2.228min (-0.042) 30.94ug/L m

response 218931

Ion	Exp%	Act%
63.00	100	100
98.00	68.80	0.14#
65.00	23.30	0.00#
0.00	0.00	0.00