
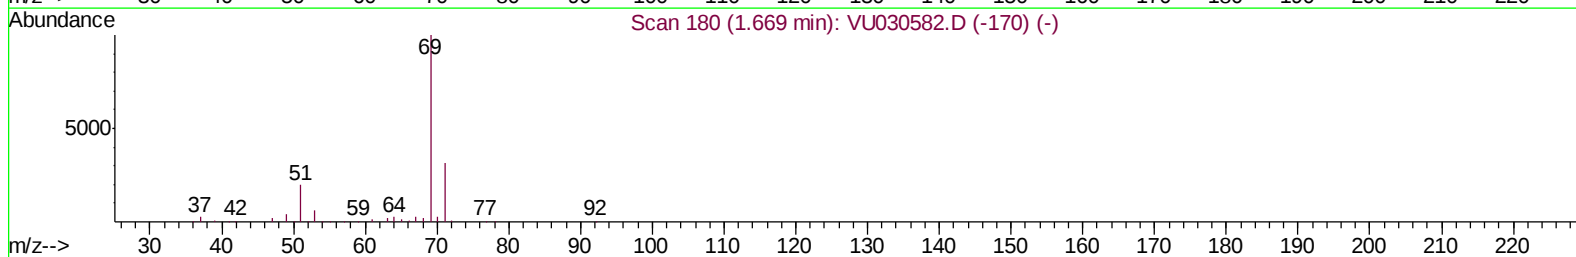
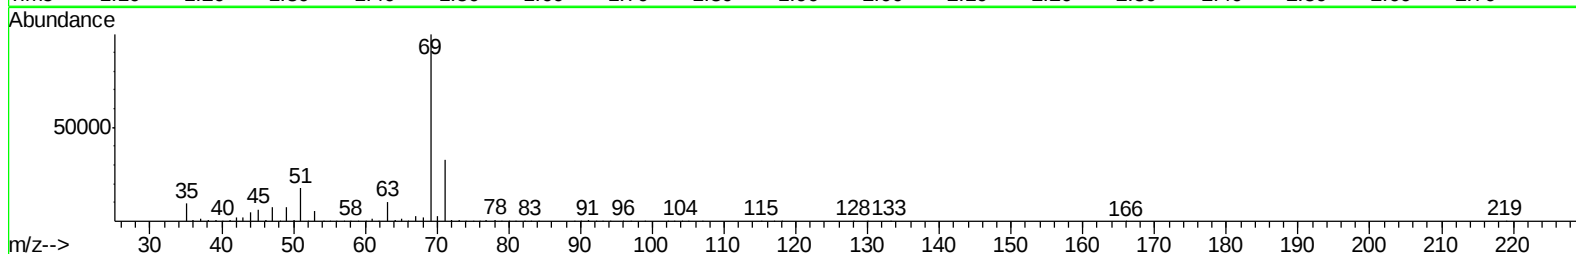


Data File : VU030602.D
Acq On : 31 Mar 2019 19:53
Operator : JC/SP
Sample : K2166-17ME
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Apr 01 02:12:43 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Apr 01 02:05:14 2019
Response via : Initial Calibration

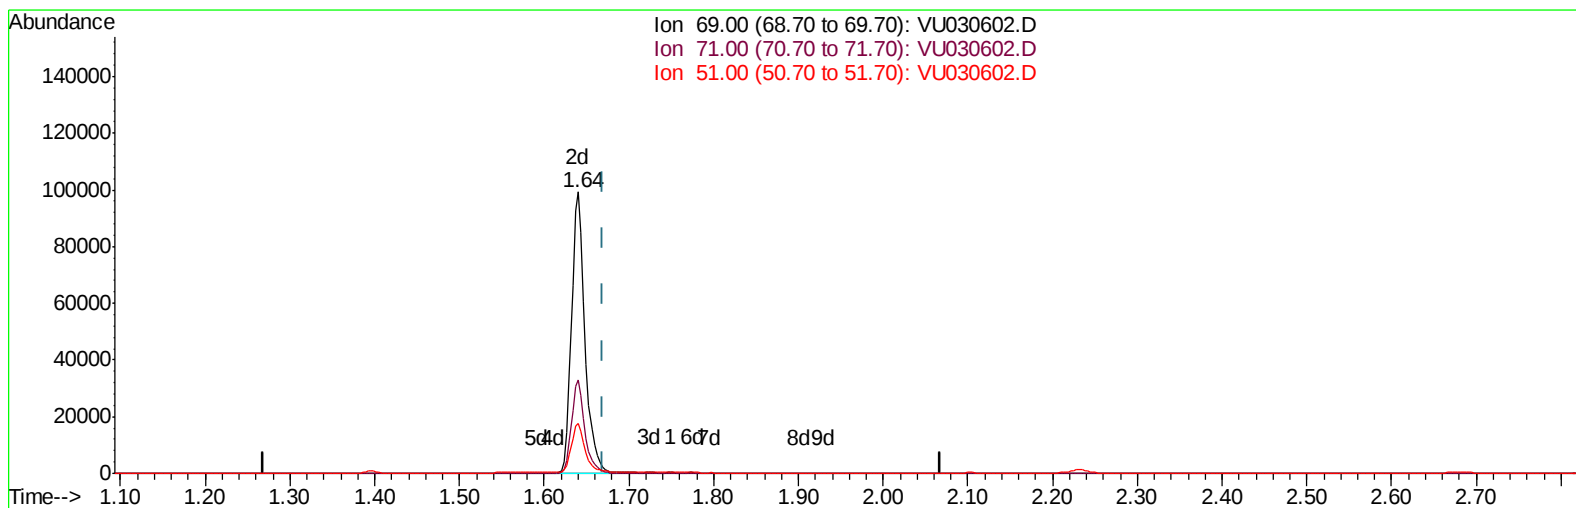

TIC: VU030602.D

(7) Chloroethane-d5 (S)

1.640min (-0.029) 37.16ug/L m

response 108932

Ion	Exp%	Act%
69.00	100	100
71.00	31.70	0.10#
51.00	28.60	0.08#
0.00	0.00	0.00