

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040119\
Quantitation Report (QT/LSC Reviewed)


Data File : VU030589.D
Acq On : 31 Mar 2019 14:53
Operator : JC/SP
Sample : K2167-15 25X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1C0

Manual Integrations
APPROVED

MMDadoda
4/1/2019 11:06:02 AM

Quant Time: Apr 01 02:44:11 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Apr 01 02:05:14 2019
Response via : Initial Calibration

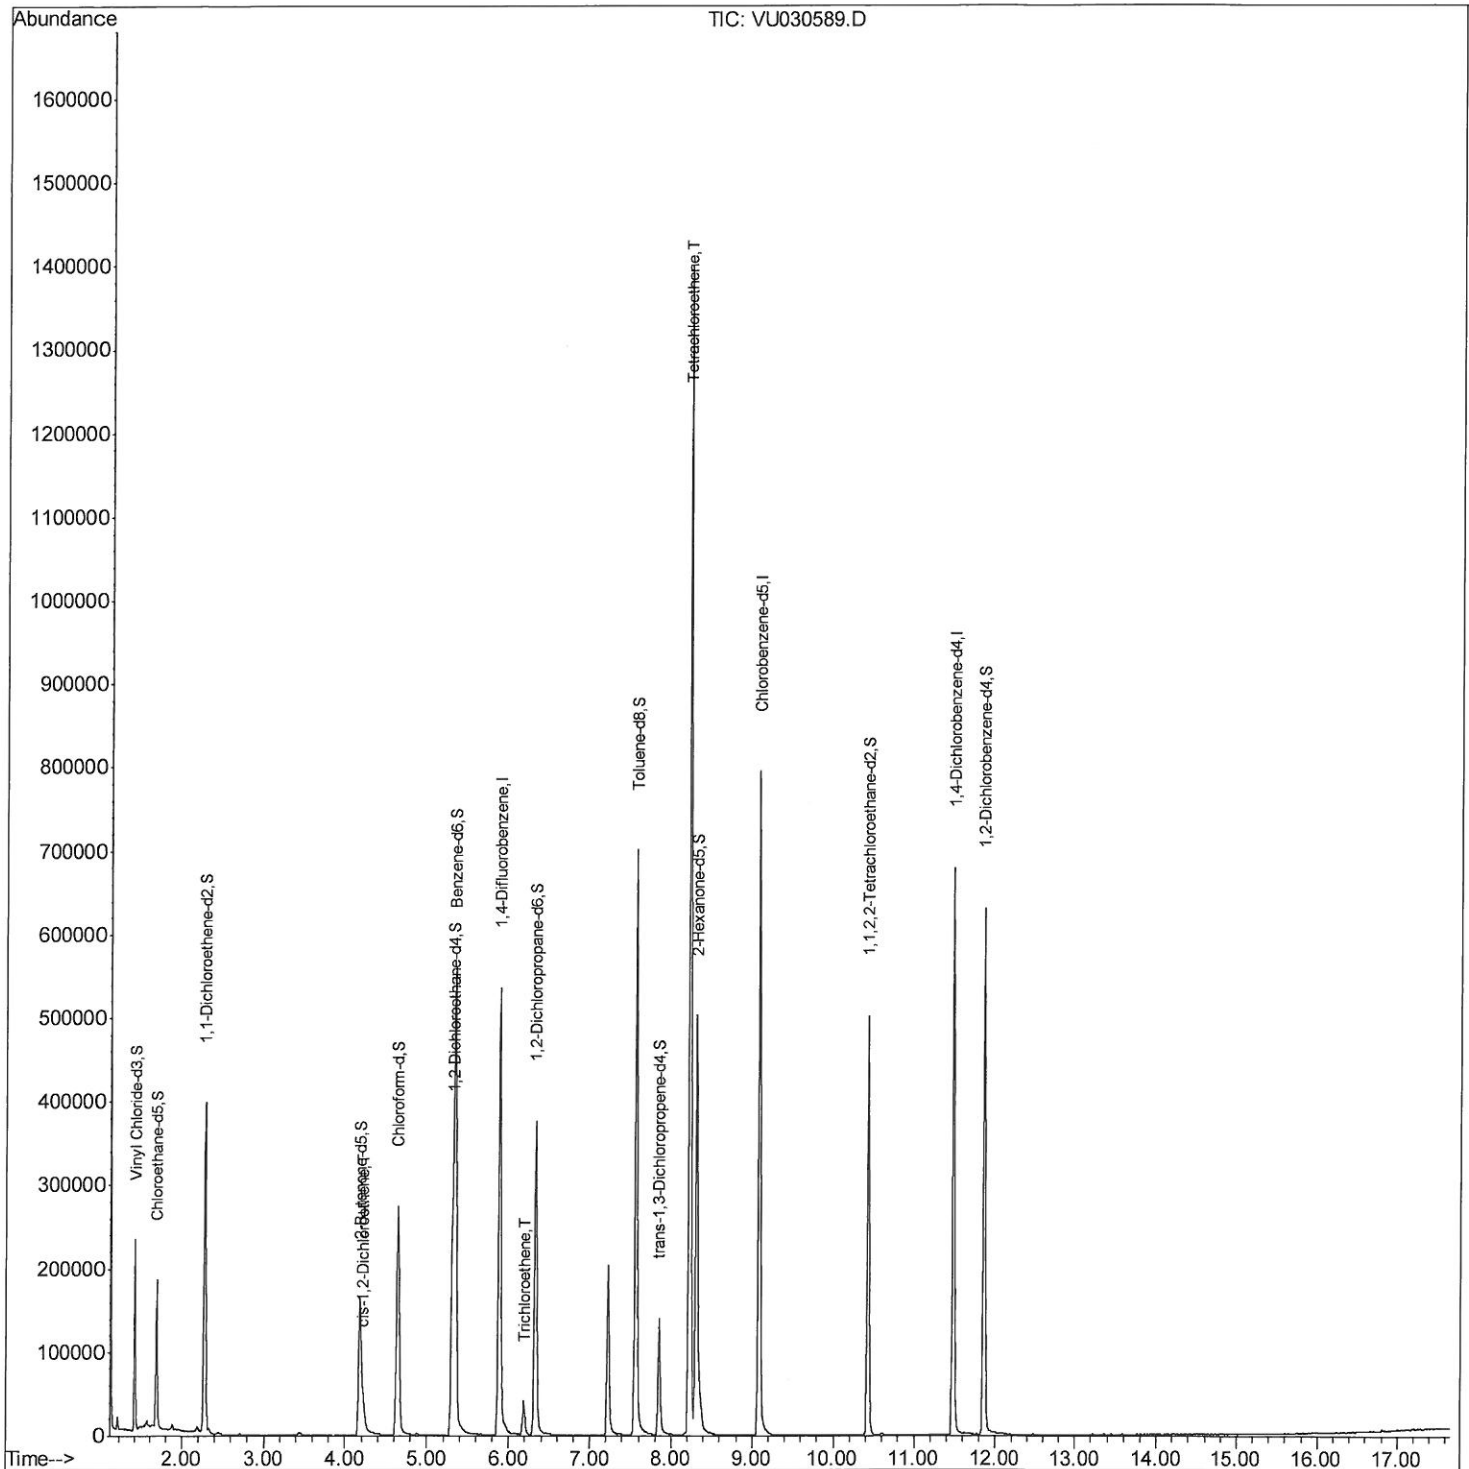

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU040119\
Quantitation Report (Qedit)




Data File : VU030589.D
Acq On : 31 Mar 2019 14:53
Operator : JC/SP
Sample : K2167-15 25X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1C0

Manual Integrations
APPROVED

MMDadoda
4/1/2019 11:06:02 AM

Quant Time: Apr 01 02:10:20 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Apr 01 02:05:14 2019
Response via : Initial Calibration

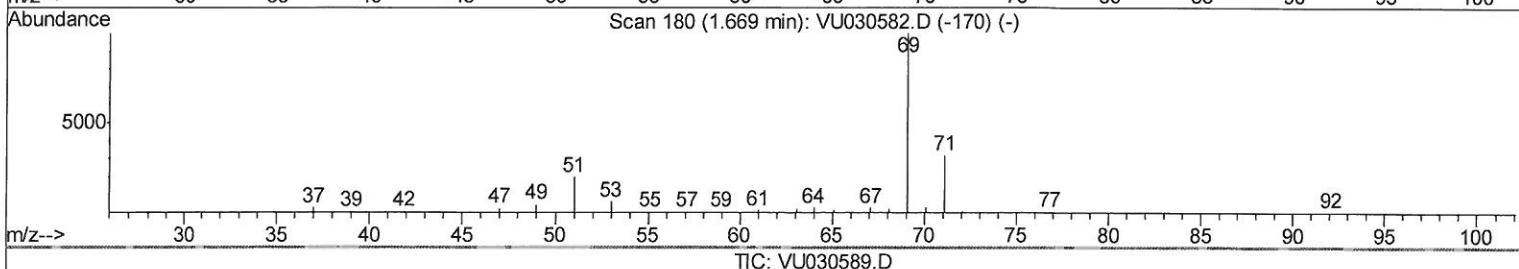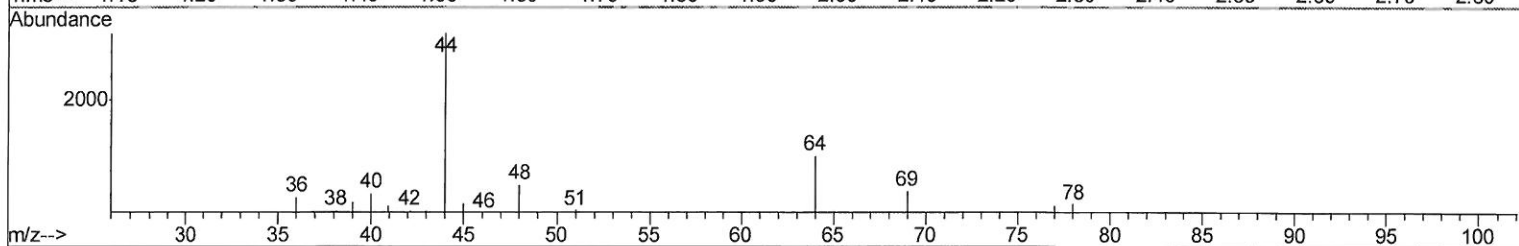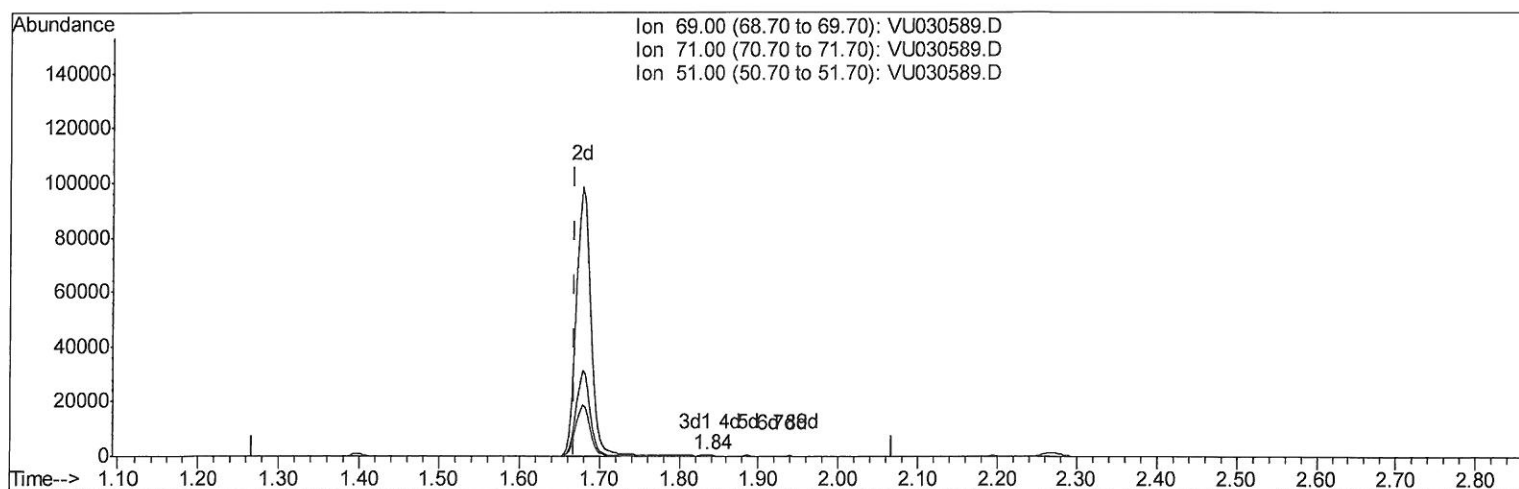

(7) Chloroethane-d5 (S)

1.836min (+0.167) 0.10ug/L

response 294

Ion	Exp%	Act%
69.00	100	100
71.00	31.70	31.63
51.00	28.60	26.53
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU040119\
Quantitation Report (Qedit)




Data File : VU030589.D
Acq On : 31 Mar 2019 14:53
Operator : JC/SP
Sample : K2167-15 25X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1C0

Manual Integrations
APPROVED

MMDadoda
4/1/2019 11:06:02 AM

Quant Time: Apr 01 02:10:20 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Apr 01 02:05:14 2019
Response via : Initial Calibration

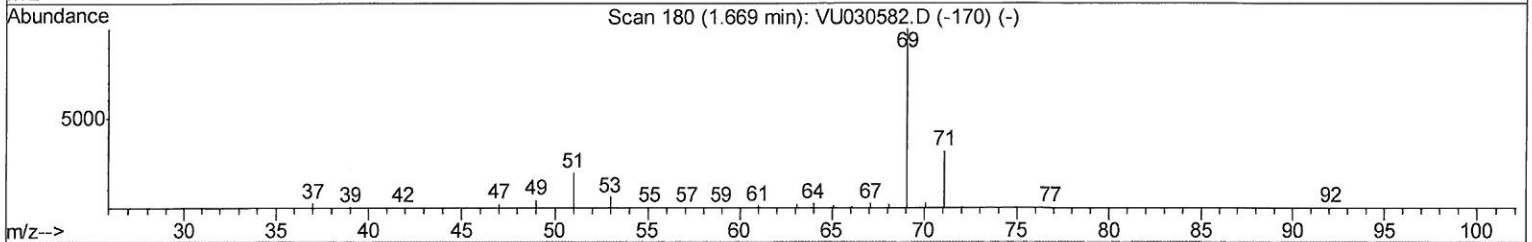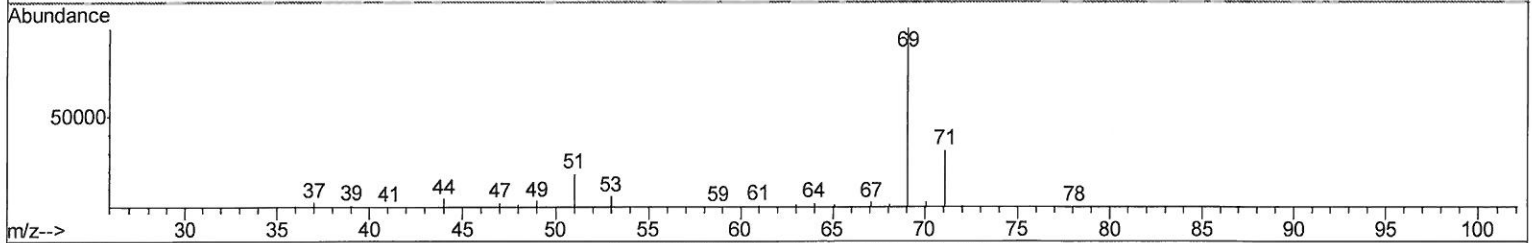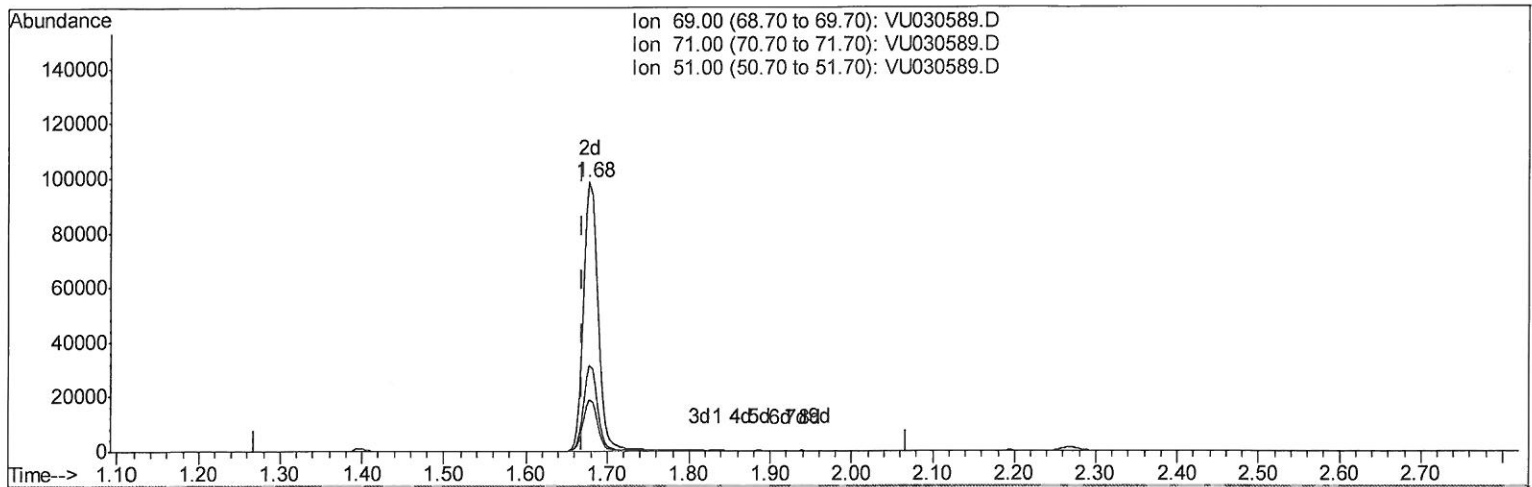

TIC: VU030589.D

(7) Chloroethane-d5 (S)

1.678min (+0.009) 42.24ug/L m

response 121115

Ion	Exp%	Act%
69.00	100	100
71.00	31.70	0.08#
51.00	28.60	0.06#
0.00	0.00	0.00

MMD
4/1/19

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040119\
Quantitation Report (QT/LSC Reviewed)

Data File : VU030589.D
Acq On : 31 Mar 2019 14:53
Operator : JC/SP
Sample : K2167-15 25X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1C0

Manual Integrations
APPROVED

MMDadoda
4/1/2019 11:06:02 AM

Quant Time: Apr 01 02:44:11 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Apr 01 02:05:14 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	449540	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	434635	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	175294	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	141479	39.11	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	78.22%
7) Chloroethane-d5	1.68	69	121115m	42.24	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	84.48%
11) 1,1-Dichloroethene-d2	2.27	63	228722	33.33	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	66.66%
21) 2-Butanone-d5	4.18	46	286364	84.20	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	84.20%
24) Chloroform-d	4.65	84	267995	42.99	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.98%
26) 1,2-Dichloroethane-d4	5.31	65	185261	45.42	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.84%
32) Benzene-d6	5.34	84	548092	43.97	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.94%
36) 1,2-Dichloropropane-d6	6.33	67	197052	46.21	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	92.42%
41) Toluene-d8	7.56	98	473151	42.27	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	84.54%
43) trans-1,3-Dichloropropene-	7.85	79	87321	43.55	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.10%
47) 2-Hexanone-d5	8.31	63	173526	75.09	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	75.09%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	264431	43.33	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	86.66%
64) 1,2-Dichlorobenzene-d4	11.86	152	163750	46.62	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.24%

7MD
4/9/19

Target Compounds					Qvalue
20) cis-1,2-Dichloroethene	4.22	96	10973	2.900	ug/L 100
34) Trichloroethene	6.19	95	14850	4.083	ug/L 97
46) Tetrachloroethene	8.22	164	312944	123.185	ug/L 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed