


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU040119\
 Data File : VU030581.D
 Acq On : 31 Mar 2019 10:08
 Operator : JC/SP
 Sample : BFB48
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB48

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis
 Last Update : Mon Apr 01 02:05:14 2019

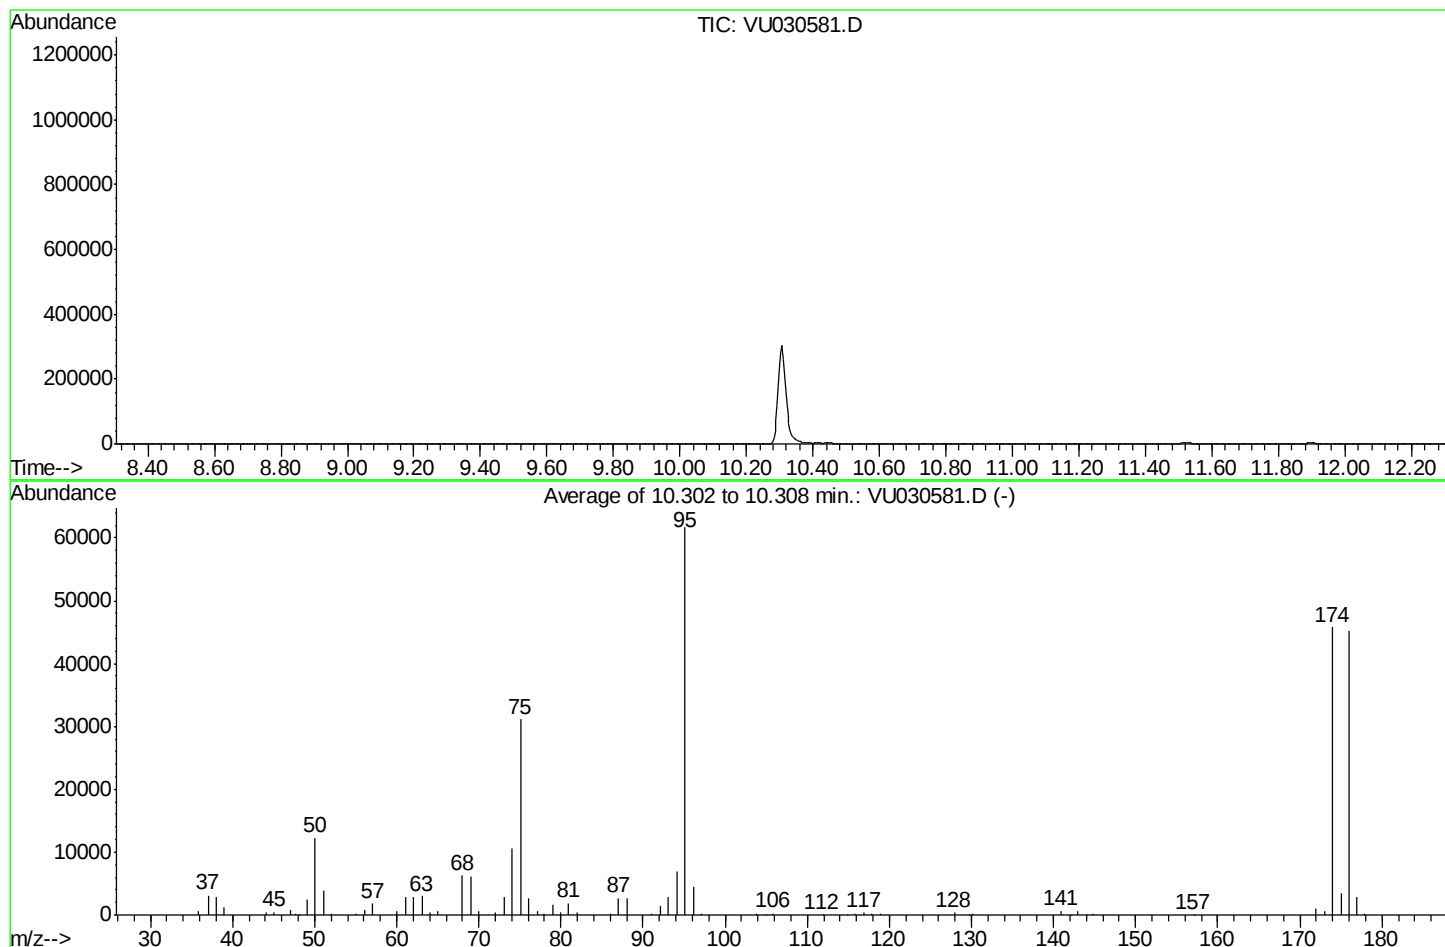

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	12248	PASS
75	95	30	80	50.5	31120	PASS
95	95	100	100	100.0	61680	PASS
96	95	5	9	7.2	4428	PASS
173	174	0.00	2	1.2	556	PASS
174	95	50	120	74.1	45733	PASS
175	174	5	9	7.7	3524	PASS
176	174	95	101	98.8	45197	PASS
177	176	5	9	6.2	2811	PASS

Scan 2854 (10.267 min): VU030581.D
BFB48

m/z	Abundance
39.90	362.0
44.00	578.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48

m/z	Abundance
35.90	536.0
37.00	3105.0
38.00	2802.0
39.00	1102.0
40.00	314.0
44.10	963.0
45.10	524.0
47.00	938.0
48.10	215.0
49.00	2193.0
50.10	12262.0
51.10	3705.0
52.00	208.0
55.00	162.0
56.10	814.0
57.10	1781.0
60.10	496.0
61.10	2700.0
62.10	2719.0
63.00	2932.0
64.00	442.0
64.90	694.0
68.00	6008.0
69.00	5921.0
70.00	594.0
72.00	402.0
73.10	2701.0
74.10	10608.0
75.10	30392.0
76.10	2742.0
77.20	456.0
78.10	214.0
78.90	1652.0
80.00	514.0
80.90	1751.0
82.00	478.0
86.00	153.0
87.00	2633.0
88.00	2516.0
91.00	115.0
92.00	1506.0
93.00	2918.0
94.10	6676.0
95.10	59744.0
96.10	4374.0
97.00	181.0
103.80	187.0
104.90	129.0
105.90	240.0
114.90	129.0
115.80	236.0
117.00	270.0
117.90	197.0
119.00	234.0
127.90	316.0
130.10	168.0
141.00	612.0
142.90	485.0
144.90	166.0
172.00	949.0
174.00	43448.0
175.10	3330.0
176.00	42096.0
177.00	2713.0
177.90	138.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48

m/z	Abundance
35.90	536.0
37.10	3265.0
38.00	2926.0
39.00	1254.0
40.00	343.0
44.10	964.0
45.10	520.0
47.00	946.0
47.70	365.0
49.00	2576.0
50.10	12815.0
51.10	4003.0
52.00	276.0
55.00	166.0
56.00	879.0
57.10	1909.0
60.00	666.0
61.00	2941.0
62.10	2827.0
63.00	3197.0
64.00	493.0
64.90	717.0
68.00	6513.0
69.00	6282.0
70.00	625.0
72.10	359.0
73.10	2934.0
74.10	10907.0
75.10	32176.0
76.10	2794.0
77.10	591.0
77.90	175.0
78.90	1721.0
80.00	501.0
80.90	1924.0
81.90	535.0
86.00	195.0
87.00	2764.0
88.00	2633.0
90.90	153.0
92.00	1504.0
93.00	3007.0
94.10	7125.0
95.10	63744.0
96.10	4635.0
97.10	207.0
103.90	191.0
104.90	134.0
105.90	297.0
114.90	121.0
115.80	257.0
116.90	320.0
117.90	186.0
119.00	257.0
128.00	345.0
130.10	157.0
141.00	714.0
143.00	580.0
144.00	114.0
144.80	205.0
157.10	102.0
172.00	980.0
173.10	842.0
174.00	47160.0
175.10	3632.0
176.00	46912.0
177.00	2840.0
177.80	179.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48

m/z	Abundance
35.90	481.0
37.10	3022.0
38.00	2806.0
39.00	1331.0
40.00	325.0
44.10	911.0
45.10	450.0
47.00	826.0
47.80	437.0
49.00	2703.0
50.00	11669.0
51.10	3943.0
52.10	277.0
55.00	128.0
56.00	877.0
57.00	1730.0
60.00	780.0
61.00	2877.0
62.00	2812.0
63.10	3009.0
64.00	556.0
65.00	722.0
68.00	6398.0
69.00	6342.0
70.00	553.0
72.10	321.0
73.10	2776.0
74.10	10131.0
75.10	30792.0
76.10	2607.0
77.10	647.0
77.80	173.0
79.00	1671.0
80.00	477.0
80.90	1900.0
81.90	453.0
86.00	168.0
87.00	2830.0
88.10	2566.0
90.90	223.0
92.10	1586.0
93.00	2677.0
94.10	6791.0
95.10	61552.0
96.10	4276.0
97.10	148.0
103.90	209.0
105.90	265.0
111.90	107.0
115.80	260.0
116.90	406.0
117.80	205.0
119.00	248.0
128.00	308.0
129.70	113.0
130.10	105.0
140.90	744.0
142.10	103.0
143.00	653.0
144.00	117.0
144.80	231.0
172.00	948.0
173.10	827.0
174.00	46592.0
175.10	3612.0
176.00	46584.0
177.00	2880.0
177.80	142.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48