


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU040120\
Data File : VU037519.D
Acq On : 01 Apr 2020 08:42
Operator : JC/MD
Sample : BFB11
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB11

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR040120WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Apr 02 01:37:22 2020

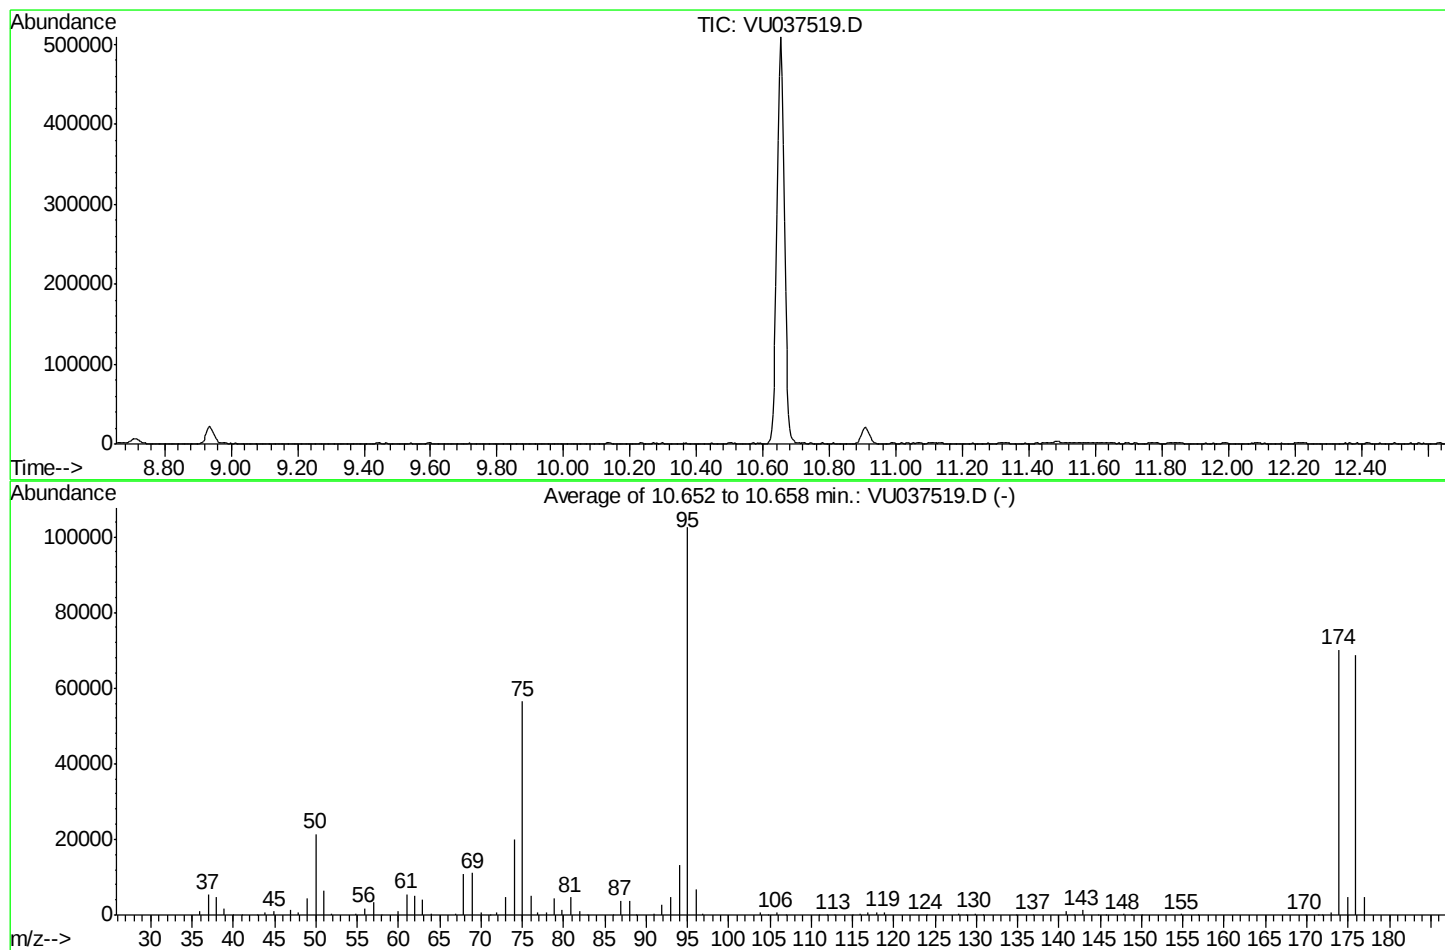

AutoFind: Scans 2896, 2897, 2898; Background Corrected with Scan 2881

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	21333	PASS
75	95	30	80	55.1	56461	PASS
95	95	100	100	100.0	102512	PASS
96	95	5	9	6.7	6855	PASS
173	174	0.00	2	0.9	598	PASS
174	95	50	120	68.4	70149	PASS
175	174	5	9	6.8	4804	PASS
176	174	95	101	97.8	68597	PASS
177	176	5	9	6.7	4617	PASS

m/z	Abundance
35.90	1315.0
37.00	5654.0
38.00	4993.0
38.90	2287.0
39.90	173.0
42.90	116.0
43.90	1060.0
44.90	972.0
46.90	1468.0
47.80	712.0
48.90	4912.0
50.00	22720.0
51.00	6960.0
51.90	321.0
54.90	412.0
55.90	1963.0
57.00	3472.0
57.90	133.0
59.90	1041.0
61.00	5574.0
62.00	5397.0
63.00	4427.0
64.00	462.0
66.90	330.0
67.90	11589.0
69.00	11694.0
70.00	804.0
71.10	100.0
72.00	634.0
72.90	5175.0
74.00	20368.0
75.00	58720.0
76.00	5339.0
76.90	725.0
77.80	577.0
78.90	4833.0
79.80	1402.0
80.90	4973.0
81.90	1059.0
86.00	101.0
86.90	4141.0
88.00	3927.0
88.70	121.0
90.90	444.0
91.90	3118.0
93.00	4726.0
94.00	13502.0
95.00	105184.0
96.00	7170.0
96.90	269.0
103.80	541.0
104.80	137.0
105.80	655.0
106.90	175.0
111.90	107.0
112.80	130.0
114.90	145.0
115.80	512.0
116.90	670.0
117.90	606.0
118.80	757.0
127.80	386.0
128.80	159.0
129.80	520.0
130.80	155.0
134.90	170.0
136.90	195.0
140.90	1140.0
141.90	200.0
142.80	1225.0
144.90	118.0
145.70	139.0
147.80	214.0
148.70	104.0
149.90	127.0
154.80	219.0
157.00	107.0
171.40	133.0
172.90	628.0
173.90	70720.0
174.90	5097.0
175.90	68968.0
176.90	4836.0

Instrument :
MSVOA_U
ClientSampleId :
BFB11

m/z	Abundance
35.90	1413.0
37.00	5469.0
38.00	5094.0
38.90	1986.0
39.90	138.0
41.00	100.0
42.90	103.0
43.90	1044.0
45.00	919.0
46.90	1366.0
47.90	638.0
49.00	4663.0
50.00	22200.0
51.00	6836.0
51.90	309.0
54.80	459.0
55.90	1888.0
57.00	3337.0
59.90	1040.0
61.00	5607.0
61.90	5362.0
62.90	4342.0
64.00	412.0
66.90	336.0
67.90	11118.0
69.00	11176.0
69.90	855.0
71.90	641.0
72.90	5018.0
74.00	20648.0
75.00	58376.0
76.00	5237.0
76.90	734.0
77.80	595.0
78.90	4654.0
79.80	1260.0
80.90	4794.0
81.90	1035.0
82.90	125.0
86.00	123.0
86.90	3994.0
87.90	3953.0
88.70	173.0
90.90	541.0
91.90	2908.0
92.90	4760.0
94.00	13761.0
95.00	105920.0
96.00	7086.0
96.90	209.0
103.80	573.0
104.80	165.0
105.80	584.0
106.90	168.0
112.80	145.0
114.90	154.0
115.80	532.0
116.90	705.0
117.90	533.0
118.80	790.0
123.90	134.0
127.80	424.0
128.80	175.0
129.80	535.0
130.80	143.0
134.70	150.0
136.90	173.0
140.90	1132.0
141.80	170.0
142.80	1306.0
144.80	104.0
145.70	126.0
147.80	202.0
149.90	136.0
154.80	249.0
156.90	125.0
171.50	161.0
171.80	156.0
172.90	593.0
173.90	72696.0
174.90	4991.0
175.90	71152.0
176.90	4751.0

Instrument :
MSVOA_U
ClientSampleId :
BFB11

m/z	Abundance
35.90	1228.0
37.00	5012.0
38.00	4486.0
39.00	1614.0
41.10	111.0
42.90	127.0
43.90	865.0
45.00	770.0
46.90	1181.0
47.90	561.0
48.90	4078.0
50.00	19080.0
51.00	6035.0
51.90	235.0
54.80	436.0
55.90	1623.0
57.00	2924.0
59.90	949.0
61.00	5154.0
61.90	4829.0
62.90	3871.0
64.00	320.0
66.90	340.0
67.90	9751.0
69.00	10239.0
69.90	837.0
71.90	621.0
72.90	4350.0
74.00	18440.0
75.00	52288.0
76.00	4594.0
76.90	661.0
77.90	551.0
78.90	4147.0
79.90	1017.0
80.80	4263.0
81.90	920.0
82.90	130.0
86.00	112.0
86.90	3418.0
87.90	3553.0
90.90	539.0
91.90	2633.0
92.90	4493.0
94.00	12589.0
95.00	96432.0
96.00	6311.0
96.90	181.0
103.80	604.0
104.80	192.0
105.80	501.0
106.90	123.0
110.90	104.0
112.80	133.0
114.90	120.0
115.90	457.0
116.80	669.0
117.90	433.0
118.80	671.0
123.90	139.0
127.80	413.0
128.80	182.0
129.80	477.0
130.80	139.0
134.70	124.0
136.90	134.0
140.90	1030.0
141.90	116.0
142.80	1238.0
144.70	102.0
147.80	165.0
150.00	108.0
154.90	231.0
156.80	154.0
169.80	101.0
171.90	197.0
172.90	574.0
173.90	67032.0
174.90	4325.0
175.90	65672.0
176.90	4264.0

Instrument :
MSVOA_U
ClientSampleId :
BFB11

Scan 2881 (10.603 min): VU037519.D
BFB11

m/z	Abundance
35.90	234.0
38.90	109.0
43.90	248.0
55.00	121.0

Instrument :
MSVOA_U
ClientSampleId :
BFB11