
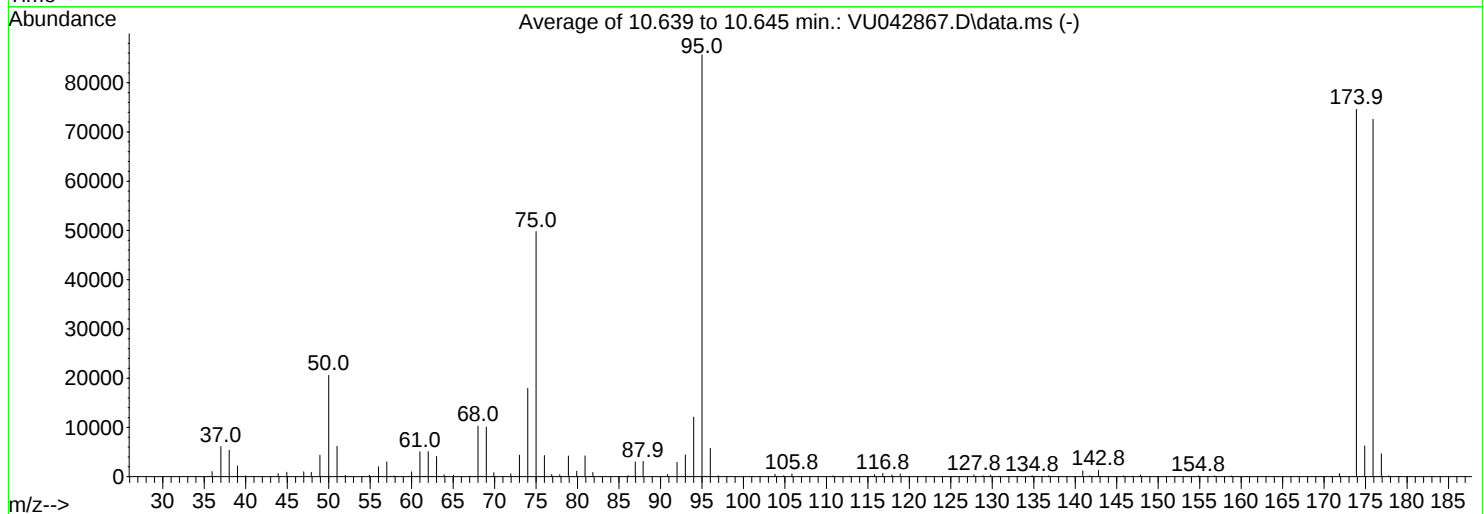


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040121\
Data File : VU042867.D
Acq On : 01 Apr 2021 09:21
Operator : SY/MD
Sample : BFB01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB01

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR040121WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Apr 02 05:16:37 2021

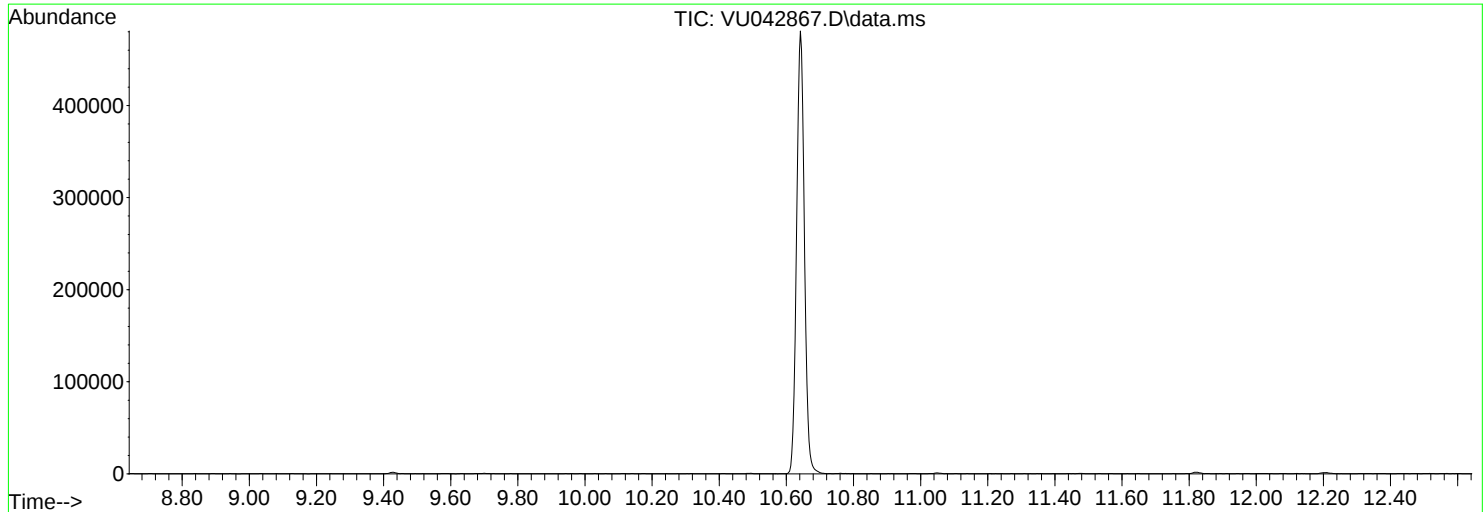

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.0	20584	PASS
75	95	30	80	58.1	49789	PASS
95	95	100	100	100.0	85664	PASS
96	95	5	9	6.7	5767	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	87.1	74621	PASS
175	174	5	9	8.4	6234	PASS
176	174	95	101	97.2	72555	PASS
177	176	5	9	6.4	4652	PASS

m/z	Abundance
43.90	256.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

m/z	Abundance
36.00	1043.0
37.00	5915.0
38.00	5402.0
39.00	2224.0
40.00	141.0
43.90	835.0
45.00	933.0
47.00	1004.0
47.90	919.0
48.90	4251.0
50.00	20664.0
51.00	6252.0
52.00	261.0
54.90	322.0
56.00	2025.0
57.00	3027.0
57.90	199.0
60.00	988.0
61.00	5028.0
62.00	5005.0
63.00	4071.0
63.90	405.0
65.00	337.0
68.00	10166.0
69.00	10070.0
69.90	784.0
72.00	534.0
73.00	4467.0
74.00	17544.0
75.00	49032.0
76.00	4199.0
76.90	427.0
77.80	339.0
78.90	4118.0
79.90	1096.0
80.90	4221.0
81.90	850.0
86.10	190.0
86.90	3052.0
87.90	3069.0
90.90	456.0
92.00	2810.0
93.00	4394.0
94.00	11748.0
95.00	84576.0
96.00	5827.0
97.00	195.0
103.80	510.0
104.90	193.0
105.80	529.0
110.80	167.0
112.80	100.0
115.80	355.0
116.80	664.0
117.80	327.0
118.90	571.0
127.80	342.0
128.90	152.0
129.80	336.0
134.80	258.0
136.80	180.0
140.90	1127.0
141.70	178.0
142.80	1276.0
143.80	118.0
144.80	119.0
145.80	169.0
147.90	320.0
154.80	189.0
156.80	157.0
158.80	196.0
171.90	566.0
173.90	71856.0
174.90	6215.0
175.90	70368.0
176.90	4707.0
177.80	152.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

m/z	Abundance
35.90	1093.0
37.00	6337.0
38.00	5539.0
39.00	2235.0
40.00	153.0
43.90	904.0
44.90	932.0
47.00	992.0
47.90	926.0
49.00	4450.0
50.00	21288.0
51.00	6297.0
52.00	292.0
54.90	346.0
56.00	2116.0
57.00	3085.0
57.90	162.0
60.00	979.0
61.00	5221.0
62.00	5228.0
63.00	4208.0
63.90	419.0
65.10	325.0
68.00	10567.0
69.00	10364.0
69.90	817.0
72.00	625.0
73.00	4492.0
74.00	18560.0
75.00	51432.0
76.00	4400.0
76.90	460.0
77.90	372.0
78.90	4305.0
79.90	1142.0
80.90	4329.0
81.80	880.0
86.10	200.0
87.00	3084.0
87.90	3125.0
90.80	452.0
92.00	2944.0
93.00	4637.0
94.00	12528.0
95.00	88488.0
96.00	5998.0
97.00	208.0
103.80	536.0
104.80	222.0
105.90	590.0
106.80	112.0
110.80	181.0
111.70	106.0
112.80	131.0
115.80	432.0
116.80	662.0
117.90	352.0
118.90	536.0
127.80	405.0
128.90	198.0
129.80	357.0
130.80	117.0
134.80	237.0
136.80	176.0
140.90	1171.0
141.70	198.0
142.80	1356.0
145.80	172.0
147.80	340.0
154.90	192.0
156.80	168.0
158.80	174.0
170.80	114.0
171.80	667.0
173.90	76808.0
174.90	6430.0
175.90	74856.0
176.90	4765.0
177.80	168.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

m/z	Abundance
35.90	1030.0
37.00	6062.0
38.00	5131.0
39.00	2054.0
40.00	171.0
43.90	897.0
44.90	837.0
46.00	109.0
47.00	929.0
47.90	800.0
49.00	4391.0
50.00	19800.0
51.00	5904.0
52.00	276.0
54.90	266.0
56.00	1922.0
57.00	2864.0
57.90	112.0
60.00	967.0
61.00	4954.0
62.00	5073.0
63.00	4030.0
63.90	397.0
65.10	296.0
67.10	260.0
68.00	10090.0
69.00	9774.0
69.90	801.0
71.90	604.0
73.00	4213.0
74.00	17640.0
75.00	48904.0
76.00	4280.0
76.90	434.0
77.90	416.0
78.90	4147.0
79.90	1092.0
80.90	4085.0
81.80	857.0
82.80	103.0
86.10	166.0
87.00	2876.0
87.90	3053.0
90.80	457.0
92.00	2957.0
93.00	4261.0
94.00	11981.0
95.00	83928.0
96.00	5475.0
96.90	199.0
103.80	443.0
104.90	201.0
105.90	549.0
110.80	176.0
112.80	110.0
114.80	121.0
115.80	471.0
116.80	583.0
118.00	399.0
118.90	512.0
127.80	401.0
128.90	198.0
129.80	359.0
130.80	143.0
134.80	232.0
136.80	199.0
140.90	1203.0
141.80	203.0
142.80	1253.0
145.80	156.0
146.90	116.0
147.80	313.0
154.90	195.0
156.80	122.0
158.80	142.0
160.70	111.0
170.90	169.0
171.80	656.0
173.90	75200.0
174.90	6056.0
175.90	72440.0
176.90	4483.0
177.80	134.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01