
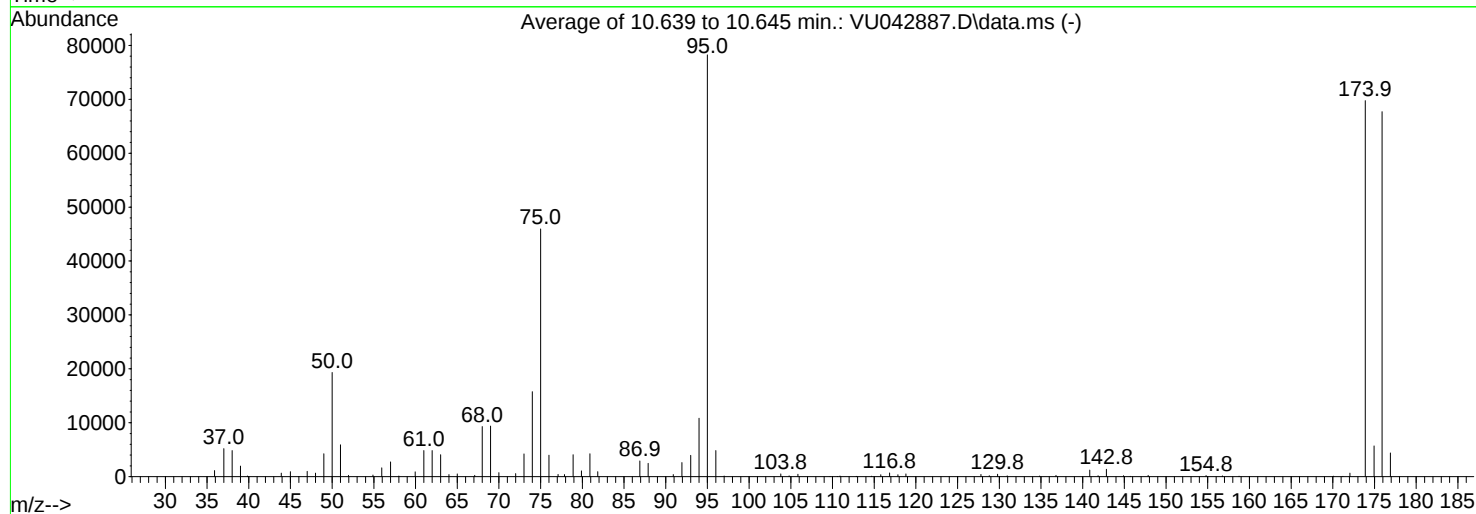


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040121\
Data File : VU042887.D
Acq On : 02 Apr 2021 08:30
Operator : SY/MD
Sample : BFB02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB02

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR040121WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Apr 02 05:16:37 2021

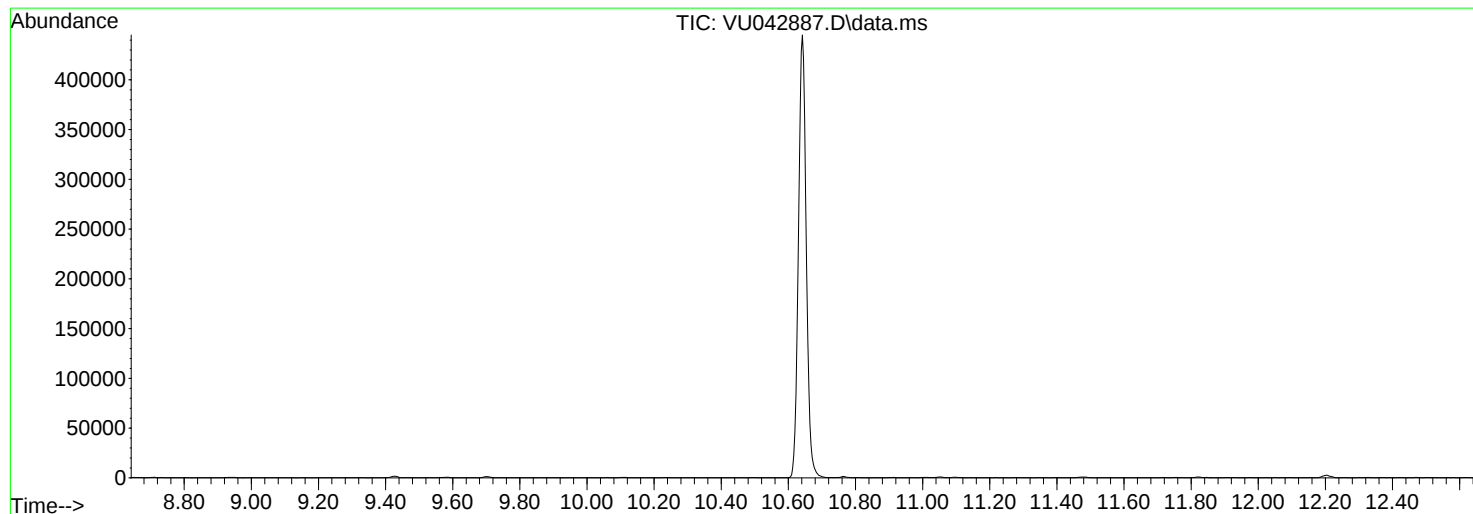

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.7	19325	PASS
75	95	30	80	58.7	45944	PASS
95	95	100	100	100.0	78253	PASS
96	95	5	9	6.2	4849	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	89.2	69765	PASS
175	174	5	9	8.2	5703	PASS
176	174	95	101	97.0	67701	PASS
177	176	5	9	6.5	4400	PASS

m/z	Abundance
44.10	171.0

Instrument :
MSVOA_U
ClientSampleId :
BFB02

m/z	Abundance
35.90	1122.0
37.00	5159.0
38.00	4833.0
39.00	1932.0
39.80	142.0
43.90	821.0
45.00	1039.0
46.00	111.0
47.00	988.0
48.00	680.0
49.00	4478.0
50.00	19704.0
51.00	5979.0
51.90	272.0
54.90	327.0
56.00	1634.0
57.00	2747.0
58.00	129.0
60.00	970.0
61.00	4836.0
62.00	4774.0
63.00	4048.0
64.00	454.0
65.00	513.0
68.00	9604.0
69.00	9303.0
70.00	751.0
72.00	557.0
73.00	4242.0
74.00	15868.0
75.00	45488.0
76.00	4036.0
77.10	482.0
77.80	425.0
78.90	4272.0
79.90	1087.0
80.90	4337.0
81.90	885.0
86.90	2791.0
87.90	2526.0
90.90	443.0
92.00	2666.0
93.00	3952.0
94.00	10808.0
95.00	77648.0
96.00	5013.0
97.10	138.0
103.80	500.0
104.80	149.0
105.80	391.0
109.70	110.0
110.80	136.0
112.90	121.0
115.80	342.0
116.90	716.0
117.90	332.0
118.80	502.0
127.80	413.0
128.80	142.0
129.80	474.0
131.00	161.0
134.90	135.0
136.80	205.0
140.80	1169.0
141.80	210.0
142.90	1315.0
144.90	185.0
147.90	232.0
154.80	184.0
156.70	157.0
158.70	142.0
172.00	709.0
173.90	68448.0
174.90	5814.0
175.90	65624.0
176.90	4370.0

Instrument :
MSVOA_U
ClientSampleId :
BFB02

m/z	Abundance
35.90	1172.0
37.00	5348.0
38.00	4980.0
39.00	2010.0
39.90	125.0
43.90	849.0
45.00	955.0
47.00	1048.0
48.00	649.0
49.00	4451.0
50.00	20008.0
51.00	6146.0
52.00	258.0
54.90	309.0
55.90	1639.0
57.00	2809.0
58.00	143.0
60.00	939.0
61.00	4993.0
62.00	5010.0
63.00	4139.0
64.00	408.0
65.00	514.0
67.10	350.0
68.00	9513.0
69.00	9645.0
70.00	746.0
72.00	594.0
73.00	4297.0
74.00	16101.0
75.00	47456.0
76.00	4110.0
77.10	440.0
77.80	410.0
78.90	4218.0
79.90	1117.0
80.90	4423.0
81.80	945.0
86.90	3024.0
87.90	2573.0
90.90	402.0
91.90	2689.0
93.00	4067.0
94.00	11209.0
95.00	80648.0
96.00	4932.0
97.00	119.0
103.80	509.0
104.80	147.0
105.80	474.0
110.90	140.0
112.80	100.0
114.70	107.0
115.80	372.0
116.80	690.0
117.90	376.0
118.80	512.0
127.80	438.0
128.80	179.0
129.80	465.0
131.00	161.0
134.90	126.0
136.80	262.0
140.90	1267.0
141.90	201.0
142.80	1390.0
144.90	185.0
145.70	101.0
147.80	251.0
154.80	202.0
156.80	150.0
158.80	109.0
170.10	121.0
172.10	690.0
173.90	72056.0
174.90	5881.0
175.90	69904.0
176.90	4532.0

Instrument :
MSVOA_U
ClientSampleId :
BFB02

m/z	Abundance
35.90	1055.0
37.00	5119.0
38.00	4710.0
39.00	1913.0
39.90	135.0
43.90	840.0
45.00	754.0
47.00	932.0
48.00	593.0
49.00	3834.0
50.00	18264.0
51.00	5627.0
51.90	205.0
54.90	278.0
55.90	1595.0
57.00	2634.0
58.00	115.0
59.90	794.0
61.00	4673.0
62.00	4707.0
63.00	4029.0
64.00	344.0
65.00	456.0
67.10	368.0
68.00	8761.0
69.00	9174.0
70.00	711.0
72.00	524.0
73.00	4072.0
74.00	15355.0
75.00	44888.0
76.00	3797.0
77.10	349.0
77.90	372.0
78.90	3740.0
79.90	1001.0
80.90	4011.0
81.80	960.0
86.90	2956.0
87.90	2291.0
90.90	319.0
91.90	2516.0
93.00	3871.0
94.00	10525.0
95.00	76464.0
96.00	4603.0
96.90	102.0
103.80	523.0
104.80	152.0
105.90	506.0
110.60	121.0
111.00	124.0
114.70	130.0
115.80	336.0
116.80	621.0
117.80	394.0
118.80	507.0
127.80	400.0
128.80	240.0
129.80	361.0
130.90	114.0
134.80	137.0
136.80	252.0
140.90	1183.0
141.90	151.0
142.80	1391.0
144.90	151.0
145.70	112.0
147.80	282.0
154.80	261.0
156.80	146.0
170.10	114.0
171.20	157.0
172.10	612.0
173.90	68792.0
175.00	5415.0
175.90	67576.0
176.90	4297.0

Instrument :
MSVOA_U
ClientSampleId :
BFB02