

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040122\
 Data File : VU047785.D
 Acq On : 01 Apr 2022 13:32
 Operator : SY/MD
 Sample : N2179-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0R37

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047785.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	100	rVB	194248	225277	15.38%	1.952%
2	1.919	171	180	203	rVB	147962	202852	13.85%	1.758%
3	2.571	370	383	406	rBV	323221	538182	36.73%	4.664%
4	2.758	438	441	445	rBV2	352	275	0.02%	0.002%
5	2.809	447	457	460	rBV4	1709	2973	0.20%	0.026%
6	3.192	561	576	590	rVB2	3870	9759	0.67%	0.085%
7	3.314	607	614	617	rBV3	306	375	0.03%	0.003%
8	3.362	627	629	631	rVV	525	269	0.02%	0.002%
9	3.584	690	698	701	rVB2	307	351	0.02%	0.003%
10	3.790	756	762	765	rBV2	251	287	0.02%	0.002%
11	3.932	802	806	813	rVB2	302	341	0.02%	0.003%
12	3.986	813	823	828	rBV2	222	429	0.03%	0.004%
13	4.221	893	896	899	rVB	375	254	0.02%	0.002%
14	4.256	899	907	911	rBV3	360	373	0.03%	0.003%
15	4.417	951	957	962	rBV2	195	229	0.02%	0.002%
16	4.468	966	973	978	rVB2	325	385	0.03%	0.003%
17	4.639	1011	1026	1075	rBV2	98511	330348	22.55%	2.863%
18	4.870	1094	1098	1102	rBV4	299	322	0.02%	0.003%
19	4.967	1124	1128	1132	rVB3	288	229	0.02%	0.002%
20	4.993	1132	1136	1141	rVB3	354	293	0.02%	0.003%
21	5.067	1141	1159	1184	rBV	266860	585451	39.96%	5.073%
22	5.279	1220	1225	1228	rBV2	315	312	0.02%	0.003%
23	5.729	1343	1365	1397	rBV2	544751	1465149	100.00%	12.697%
24	5.931	1425	1428	1432	rBV2	356	298	0.02%	0.003%
25	5.996	1443	1448	1452	rVB2	405	393	0.03%	0.003%
26	6.021	1452	1456	1459	rBV2	426	314	0.02%	0.003%
27	6.041	1459	1462	1465	rBV3	567	432	0.03%	0.004%
28	6.070	1469	1471	1481	rVB3	561	531	0.04%	0.005%
29	6.115	1481	1485	1487	rBV2	512	363	0.02%	0.003%
30	6.253	1513	1528	1556	rBV	416887	804912	54.94%	6.975%
31	6.420	1577	1580	1586	rVB4	328	280	0.02%	0.002%
32	6.468	1593	1595	1602	rVB3	446	435	0.03%	0.004%
33	6.513	1605	1609	1610	rBV	428	276	0.02%	0.002%
34	6.539	1610	1617	1618	rBV4	1023	1228	0.08%	0.011%
35	6.620	1637	1642	1646	rBV2	291	321	0.02%	0.003%
36	6.693	1648	1665	1689	rBV	329552	646058	44.10%	5.599%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040122\
 Data File : VU047785.D
 Acq On : 01 Apr 2022 13:32
 Operator : SY/MD
 Sample : N2179-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0R37

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.803	1695	1699	1712	rVB6	892	1621	0.11%	0.014%
38	6.886	1721	1725	1728	rBV3	414	284	0.02%	0.002%
39	6.967	1745	1750	1752	rBV2	352	300	0.02%	0.003%
40	7.025	1760	1768	1770	rBV2	417	477	0.03%	0.004%
41	7.044	1770	1774	1776	rBV2	618	444	0.03%	0.004%
42	7.189	1809	1819	1831	rVB5	1922	3377	0.23%	0.029%
43	7.359	1868	1872	1877	rVB3	299	243	0.02%	0.002%
44	7.568	1923	1937	1952	rBV	190871	336323	22.95%	2.915%
45	7.693	1968	1976	1982	rBV4	1335	1903	0.13%	0.016%
46	7.803	2000	2010	2020	rBV6	2277	4283	0.29%	0.037%
47	7.899	2026	2040	2056	rBV	706011	1219282	83.22%	10.566%
48	8.182	2113	2128	2145	rBV	133714	231203	15.78%	2.004%
49	8.475	2207	2219	2236	rBV2	21225	38362	2.62%	0.332%
50	8.639	2256	2270	2300	rBV	348218	692365	47.26%	6.000%
51	9.095	2407	2412	2415	rVB2	366	299	0.02%	0.003%
52	9.115	2415	2418	2423	rBV3	244	272	0.02%	0.002%
53	9.140	2423	2426	2429	rBV	384	308	0.02%	0.003%
54	9.172	2433	2436	2442	rVB2	268	276	0.02%	0.002%
55	9.211	2442	2448	2451	rBV3	392	508	0.03%	0.004%
56	9.420	2499	2513	2547	rBV	609075	1037082	70.78%	8.987%
57	9.555	2551	2555	2556	rBV3	318	226	0.02%	0.002%
58	9.697	2591	2599	2611	rBV6	1872	3203	0.22%	0.028%
59	9.918	2662	2668	2672	rVB3	478	445	0.03%	0.004%
60	10.108	2718	2727	2729	rBV5	1269	1307	0.09%	0.011%
61	10.166	2743	2745	2750	rVB	423	282	0.02%	0.002%
62	10.230	2760	2765	2769	rVB3	427	410	0.03%	0.004%
63	10.269	2775	2777	2781	rVB2	428	268	0.02%	0.002%
64	10.333	2792	2797	2801	rBV3	542	459	0.03%	0.004%
65	10.381	2809	2812	2815	rBV2	321	236	0.02%	0.002%
66	10.410	2816	2821	2824	rBV2	237	234	0.02%	0.002%
67	10.430	2824	2827	2830	rVB3	383	274	0.02%	0.002%
68	10.491	2842	2846	2848	rBV2	476	335	0.02%	0.003%
69	10.555	2864	2866	2872	rVB2	399	311	0.02%	0.003%
70	10.632	2886	2890	2896	rBV4	767	1074	0.07%	0.009%
71	10.671	2896	2902	2911	rVB7	4021	5570	0.38%	0.048%
72	10.758	2916	2929	2947	rBV	463949	746426	50.95%	6.468%
73	10.896	2958	2972	2984	rBV	30564	52281	3.57%	0.453%
74	10.996	2997	3003	3005	rBV5	383	370	0.03%	0.003%
75	11.050	3016	3020	3024	rBV3	294	244	0.02%	0.002%
76	11.089	3024	3032	3034	rBV3	1100	1171	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040122\
 Data File : VU047785.D
 Acq On : 01 Apr 2022 13:32
 Operator : SY/MD
 Sample : N2179-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0R37

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.417	3129	3134	3136	rBV2	926	751	0.05%	0.007%
78	11.462	3139	3148	3160	rVB7	4089	7376	0.50%	0.064%
79	11.578	3178	3184	3188	rBV4	749	919	0.06%	0.008%
80	11.635	3199	3202	3204	rBV2	411	290	0.02%	0.003%
81	11.697	3213	3221	3231	rVB5	1967	2817	0.19%	0.024%
82	11.748	3231	3237	3244	rBV3	1907	2513	0.17%	0.022%
83	11.812	3244	3257	3279	rBV	694119	1129766	77.11%	9.790%
84	11.938	3291	3296	3298	rBV4	1565	1373	0.09%	0.012%
85	12.195	3358	3376	3395	rBV	703714	1146285	78.24%	9.933%
86	12.333	3414	3419	3426	rVB6	1356	1567	0.11%	0.014%
87	12.397	3434	3439	3441	rBV4	662	594	0.04%	0.005%
88	12.549	3482	3486	3490	rBV	324	273	0.02%	0.002%
89	12.574	3490	3494	3497	rBV	382	314	0.02%	0.003%
90	12.632	3506	3512	3519	rBV6	867	1444	0.10%	0.013%
91	12.774	3548	3556	3569	rVB	7308	11832	0.81%	0.103%
92	12.835	3572	3575	3578	rBV2	313	256	0.02%	0.002%
93	13.150	3670	3673	3680	rVB4	408	484	0.03%	0.004%
94	13.224	3690	3696	3697	rBV2	755	721	0.05%	0.006%
95	13.446	3762	3765	3774	rBV5	731	822	0.06%	0.007%
96	13.844	3881	3889	3901	rVB6	3931	6471	0.44%	0.056%
97	14.092	3958	3966	3973	rBV	7539	11445	0.78%	0.099%
98	14.333	4034	4041	4049	rBV3	3761	5800	0.40%	0.050%
99	14.475	4083	4085	4089	rVB	508	263	0.02%	0.002%
100	14.751	4169	4171	4175	rBV2	449	351	0.02%	0.003%




Sum of corrected areas: 11539621

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040122\
Data File : VU047785.D
Acq On : 01 Apr 2022 13:32
Operator : SY/MD
Sample : N2179-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0R37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

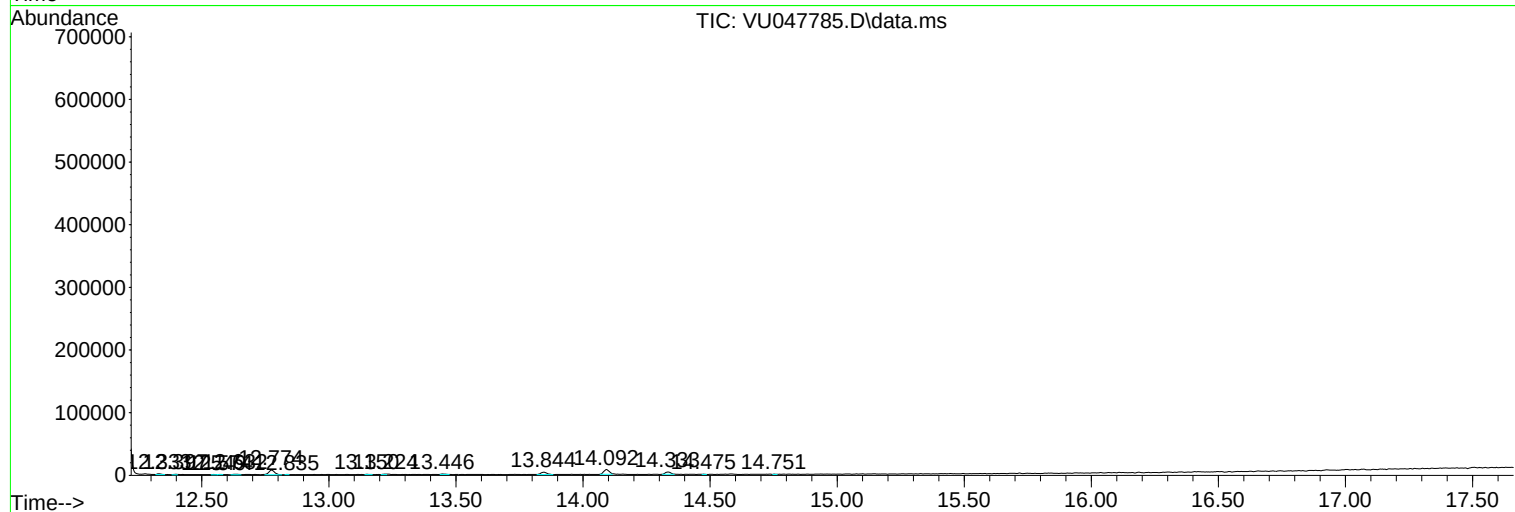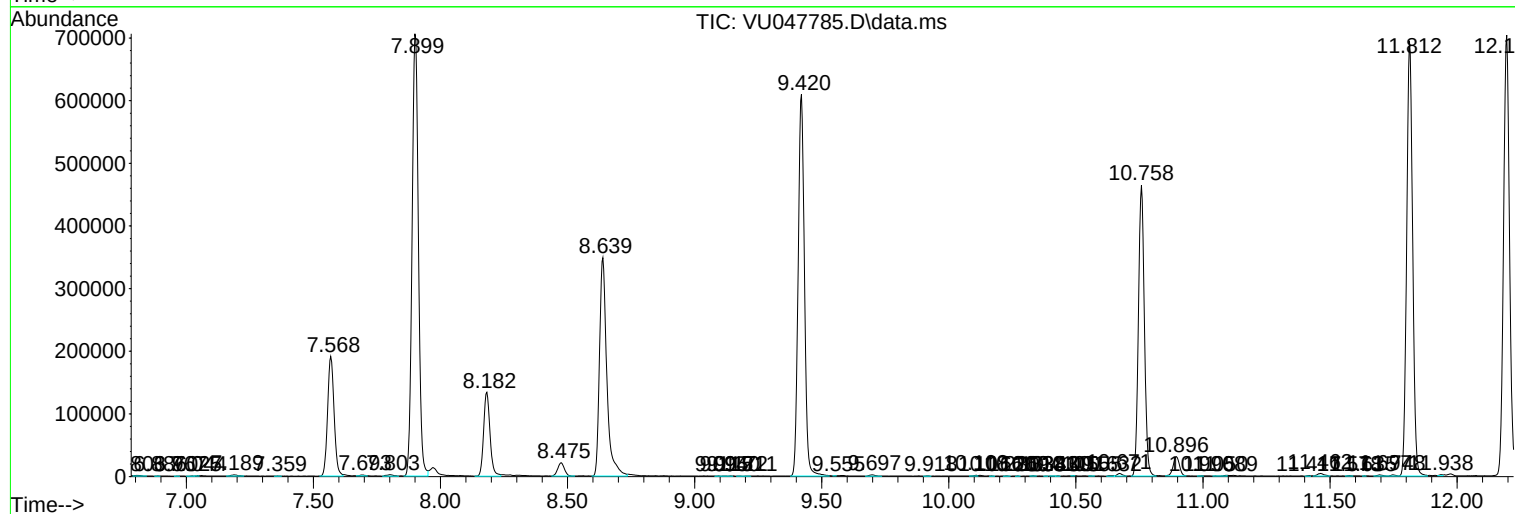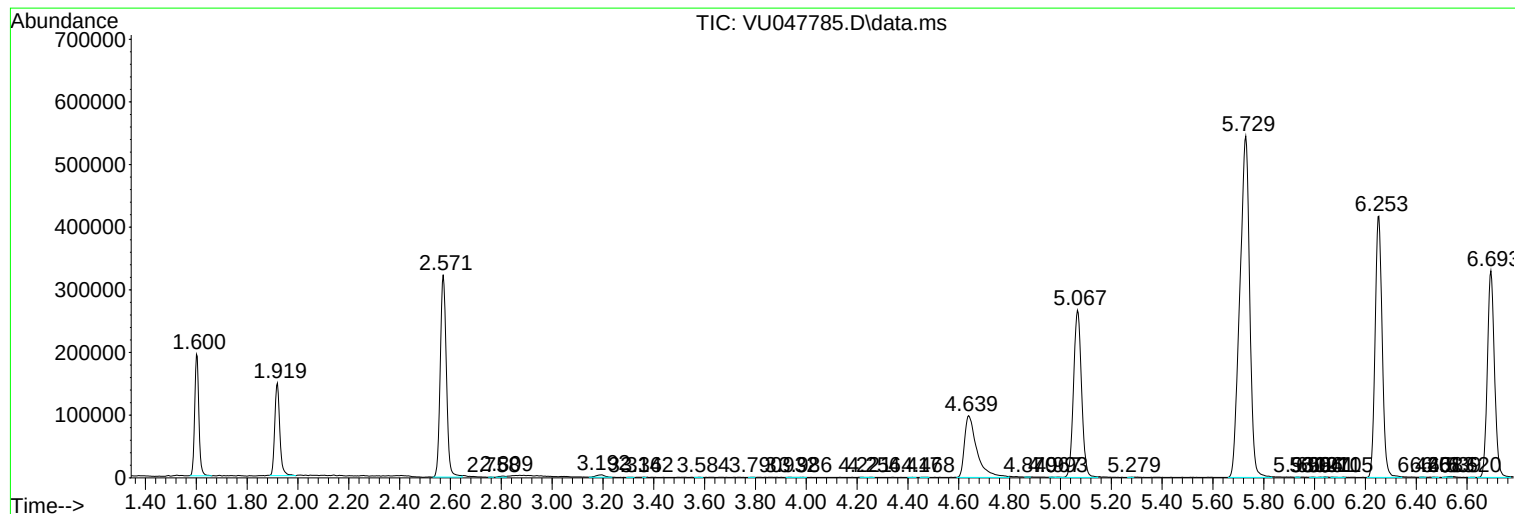

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040122\
Data File : VU047785.D
Acq On : 01 Apr 2022 13:32
Operator : SY/MD
Sample : N2179-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0R37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040122\
Data File : VU047785.D
Acq On : 01 Apr 2022 13:32
Operator : SY/MD
Sample : N2179-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0R37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc