

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040122\
 Data File : VU047787.D
 Acq On : 01 Apr 2022 16:02
 Operator : SY/MD
 Sample : N2179-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047787.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.401	17	19	34	rVB2	760	1196	0.09%	0.012%
2	1.526	53	58	60	rBV3	678	792	0.06%	0.008%
3	1.600	73	81	95	rBV	166331	192243	14.87%	1.889%
4	1.684	104	107	113	rBV5	896	891	0.07%	0.009%
5	1.732	116	122	124	rBV4	1010	969	0.07%	0.010%
6	1.764	125	132	139	rVV7	3400	4979	0.39%	0.049%
7	1.813	144	147	149	rVB	756	472	0.04%	0.005%
8	1.877	166	167	170	rBV3	405	266	0.02%	0.003%
9	1.916	170	179	200	rVV	126720	178286	13.79%	1.752%
10	2.118	240	242	244	rBV3	666	353	0.03%	0.003%
11	2.179	259	261	264	rBV3	604	329	0.03%	0.003%
12	2.198	264	267	272	rVV5	817	656	0.05%	0.006%
13	2.298	296	298	300	rBV3	356	147	0.01%	0.001%
14	2.353	313	315	316	rBV2	666	278	0.02%	0.003%
15	2.459	345	348	351	rBV2	170	136	0.01%	0.001%
16	2.478	351	354	360	rVB2	367	383	0.03%	0.004%
17	2.507	360	363	365	rBV2	157	112	0.01%	0.001%
18	2.520	365	367	370	rVB2	389	226	0.02%	0.002%
19	2.571	370	383	413	rBV	285224	468737	36.25%	4.605%
20	2.678	413	416	420	rVB2	192	158	0.01%	0.002%
21	2.710	422	426	428	rVB	205	140	0.01%	0.001%
22	2.803	440	455	460	rVB4	819	1547	0.12%	0.015%
23	2.832	460	464	465	rBV2	188	124	0.01%	0.001%
24	2.893	479	483	484	rBV2	323	218	0.02%	0.002%
25	2.948	498	500	502	rVV	230	135	0.01%	0.001%
26	2.964	502	505	516	rVB4	428	556	0.04%	0.005%
27	3.012	516	520	524	rBV2	146	146	0.01%	0.001%
28	3.057	524	534	545	rVB3	2867	5588	0.43%	0.055%
29	3.099	545	547	551	rVB2	254	157	0.01%	0.002%
30	3.121	551	554	556	rBV	189	110	0.01%	0.001%
31	3.189	566	575	584	rVB4	584	1184	0.09%	0.012%
32	3.227	584	587	591	rVB2	165	121	0.01%	0.001%
33	3.256	591	596	599	rBV2	258	232	0.02%	0.002%
34	3.295	603	608	610	rBV2	189	109	0.01%	0.001%
35	3.359	626	628	630	rVB2	229	118	0.01%	0.001%
36	3.378	631	634	635	rBV	287	133	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040122\
 Data File : VU047787.D
 Acq On : 01 Apr 2022 16:02
 Operator : SY/MD
 Sample : N2179-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	3.562	686	691	695	rVB2	324	255	0.02%	0.003%
38	3.697	730	733	738	rVB2	208	166	0.01%	0.002%
39	3.806	763	767	771	rBV	221	178	0.01%	0.002%
40	3.838	775	777	782	rVB2	217	178	0.01%	0.002%
41	3.870	782	787	790	rBV2	231	264	0.02%	0.003%
42	3.893	790	794	800	rVB2	173	189	0.01%	0.002%
43	3.977	811	820	824	rBV2	252	275	0.02%	0.003%
44	4.034	834	838	840	rVV	157	121	0.01%	0.001%
45	4.092	854	856	860	rVB	169	112	0.01%	0.001%
46	4.157	868	876	881	rBV2	346	433	0.03%	0.004%
47	4.218	893	895	898	rBV2	155	107	0.01%	0.001%
48	4.272	908	912	916	rBV2	151	134	0.01%	0.001%
49	4.311	920	924	930	rVB2	170	168	0.01%	0.002%
50	4.366	939	941	946	rVB2	217	140	0.01%	0.001%
51	4.404	951	953	958	rVV	243	195	0.02%	0.002%
52	4.430	958	961	965	rVB2	218	167	0.01%	0.002%
53	4.456	965	969	971	rBV	181	122	0.01%	0.001%
54	4.481	971	977	980	rVV2	127	113	0.01%	0.001%
55	4.523	987	990	992	rBV	255	129	0.01%	0.001%
56	4.623	1008	1021	1055	rBV	99383	241736	18.69%	2.375%
57	4.813	1078	1080	1086	rVB2	414	263	0.02%	0.003%
58	4.845	1086	1090	1094	rVB2	353	279	0.02%	0.003%
59	4.864	1094	1096	1104	rVB2	375	297	0.02%	0.003%
60	4.896	1104	1106	1109	rVB	274	112	0.01%	0.001%
61	4.912	1109	1111	1118	rVB4	382	375	0.03%	0.004%
62	4.951	1118	1123	1129	rBV3	248	329	0.03%	0.003%
63	5.067	1140	1159	1182	rVV	235977	516369	39.93%	5.073%
64	5.243	1212	1214	1217	rVB2	339	207	0.02%	0.002%
65	5.263	1217	1220	1224	rBV2	293	282	0.02%	0.003%
66	5.288	1224	1228	1234	rVB2	375	441	0.03%	0.004%
67	5.333	1240	1242	1248	rVB3	409	308	0.02%	0.003%
68	5.385	1254	1258	1263	rVB3	308	239	0.02%	0.002%
69	5.414	1263	1267	1269	rBV3	193	144	0.01%	0.001%
70	5.513	1292	1298	1300	rBV3	274	207	0.02%	0.002%
71	5.571	1309	1316	1320	rBV2	126	187	0.01%	0.002%
72	5.729	1343	1365	1397	rBV2	480993	1293155	100.00%	12.704%
73	5.864	1405	1407	1411	rVB2	223	123	0.01%	0.001%
74	5.902	1418	1419	1430	rVB3	399	618	0.05%	0.006%
75	5.954	1430	1435	1439	rVB2	121	113	0.01%	0.001%
76	5.986	1439	1445	1448	rBV4	296	379	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040122\
 Data File : VU047787.D
 Acq On : 01 Apr 2022 16:02
 Operator : SY/MD
 Sample : N2179-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	6.041	1455	1462	1468	rBV4	403	606	0.05%	0.006%
78	6.118	1484	1486	1491	rVB3	233	180	0.01%	0.002%
79	6.160	1495	1499	1501	rBV2	153	137	0.01%	0.001%
80	6.253	1513	1528	1557	rBV	409139	786137	60.79%	7.723%
81	6.382	1565	1568	1572	rVB2	280	177	0.01%	0.002%
82	6.439	1584	1586	1589	rVB2	307	174	0.01%	0.002%
83	6.459	1589	1592	1594	rBV2	328	189	0.01%	0.002%
84	6.533	1605	1615	1618	rBV4	1782	2433	0.19%	0.024%
85	6.581	1627	1630	1633	rBV2	207	191	0.01%	0.002%
86	6.607	1637	1638	1642	rBV2	308	193	0.01%	0.002%
87	6.693	1650	1665	1687	rBV	290007	573674	44.36%	5.636%
88	6.812	1698	1702	1709	rBV5	815	1078	0.08%	0.011%
89	7.568	1926	1937	1951	rBV	170395	299291	23.14%	2.940%
90	7.902	2028	2041	2055	rBV	598209	1043369	80.68%	10.250%
91	8.182	2119	2128	2142	rBV	118294	192551	14.89%	1.892%
92	8.636	2259	2269	2303	rVB	293703	569851	44.07%	5.598%
93	9.420	2501	2513	2538	rBV	592852	1007332	77.90%	9.896%
94	10.758	2918	2929	2953	rVB	413101	674154	52.13%	6.623%
95	11.815	3246	3258	3273	rBV	680177	1088910	84.21%	10.698%
96	12.195	3364	3376	3394	rVB	621744	1014589	78.46%	9.968%
97	15.548	4417	4419	4422	rVB3	675	349	0.03%	0.003%
98	15.564	4422	4424	4427	rBV3	456	253	0.02%	0.002%
99	15.648	4447	4450	4455	rBV4	925	748	0.06%	0.007%
100	15.909	4529	4531	4535	rVB4	899	530	0.04%	0.005%




Sum of corrected areas: 10178932

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040122\
Data File : VU047787.D
Acq On : 01 Apr 2022 16:02
Operator : SY/MD
Sample : N2179-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

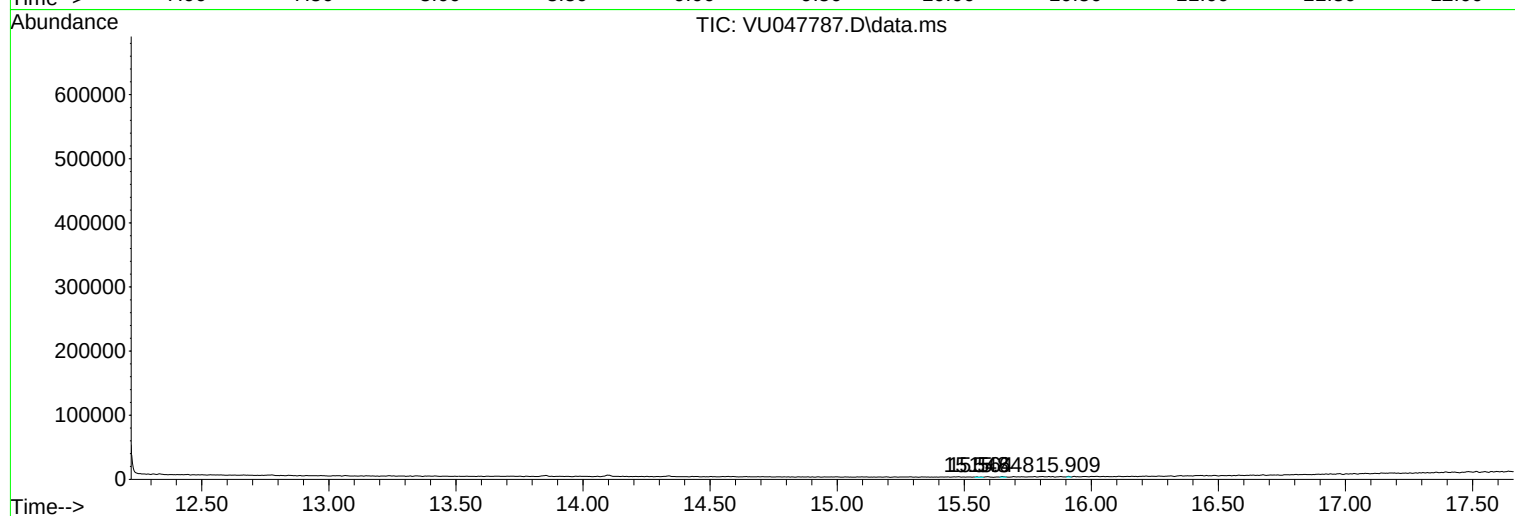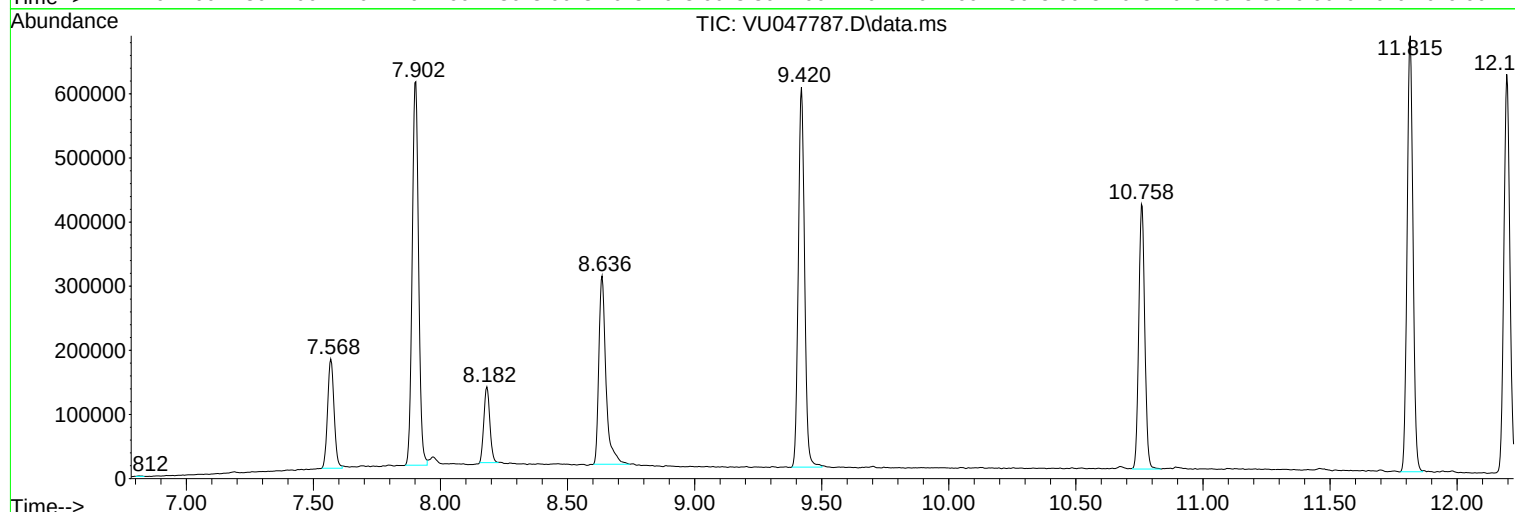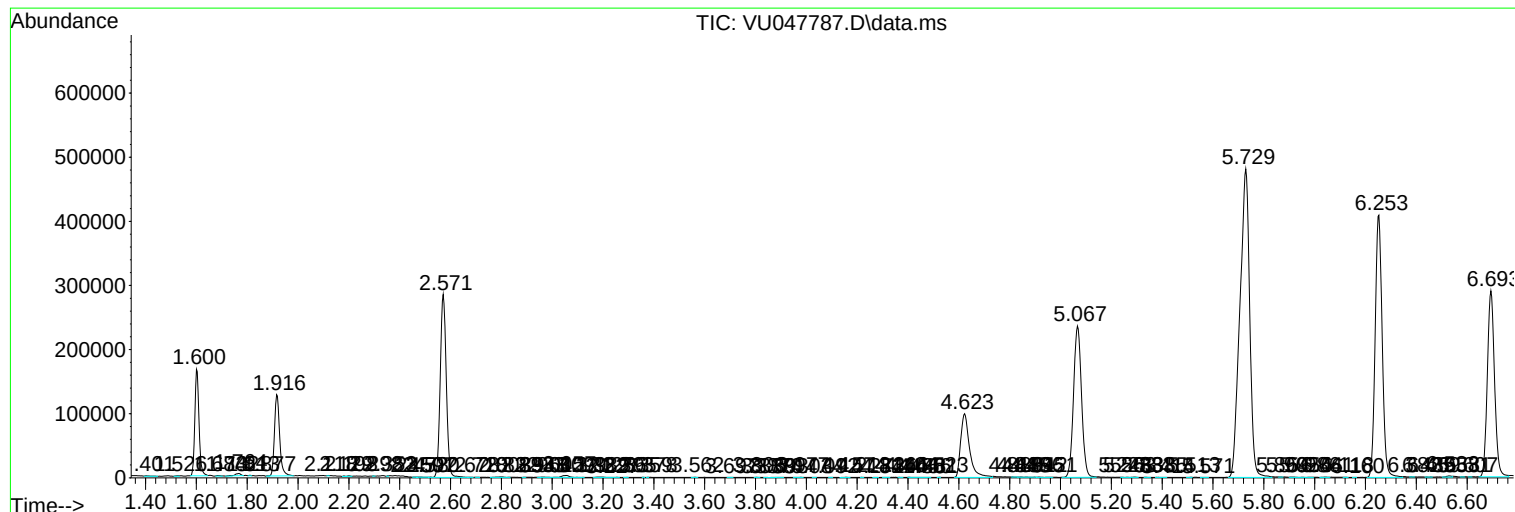

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040122\
Data File : VU047787.D
Acq On : 01 Apr 2022 16:02
Operator : SY/MD
Sample : N2179-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040122\
Data File : VU047787.D
Acq On : 01 Apr 2022 16:02
Operator : SY/MD
Sample : N2179-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc