


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040122\
Data File : VU047781.D
Acq On : 01 Apr 2022 08:56
Operator : SY/MD
Sample : BFB058
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB058

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Title : VOC Analysis
Last Update : Sat Apr 02 01:06:35 2022

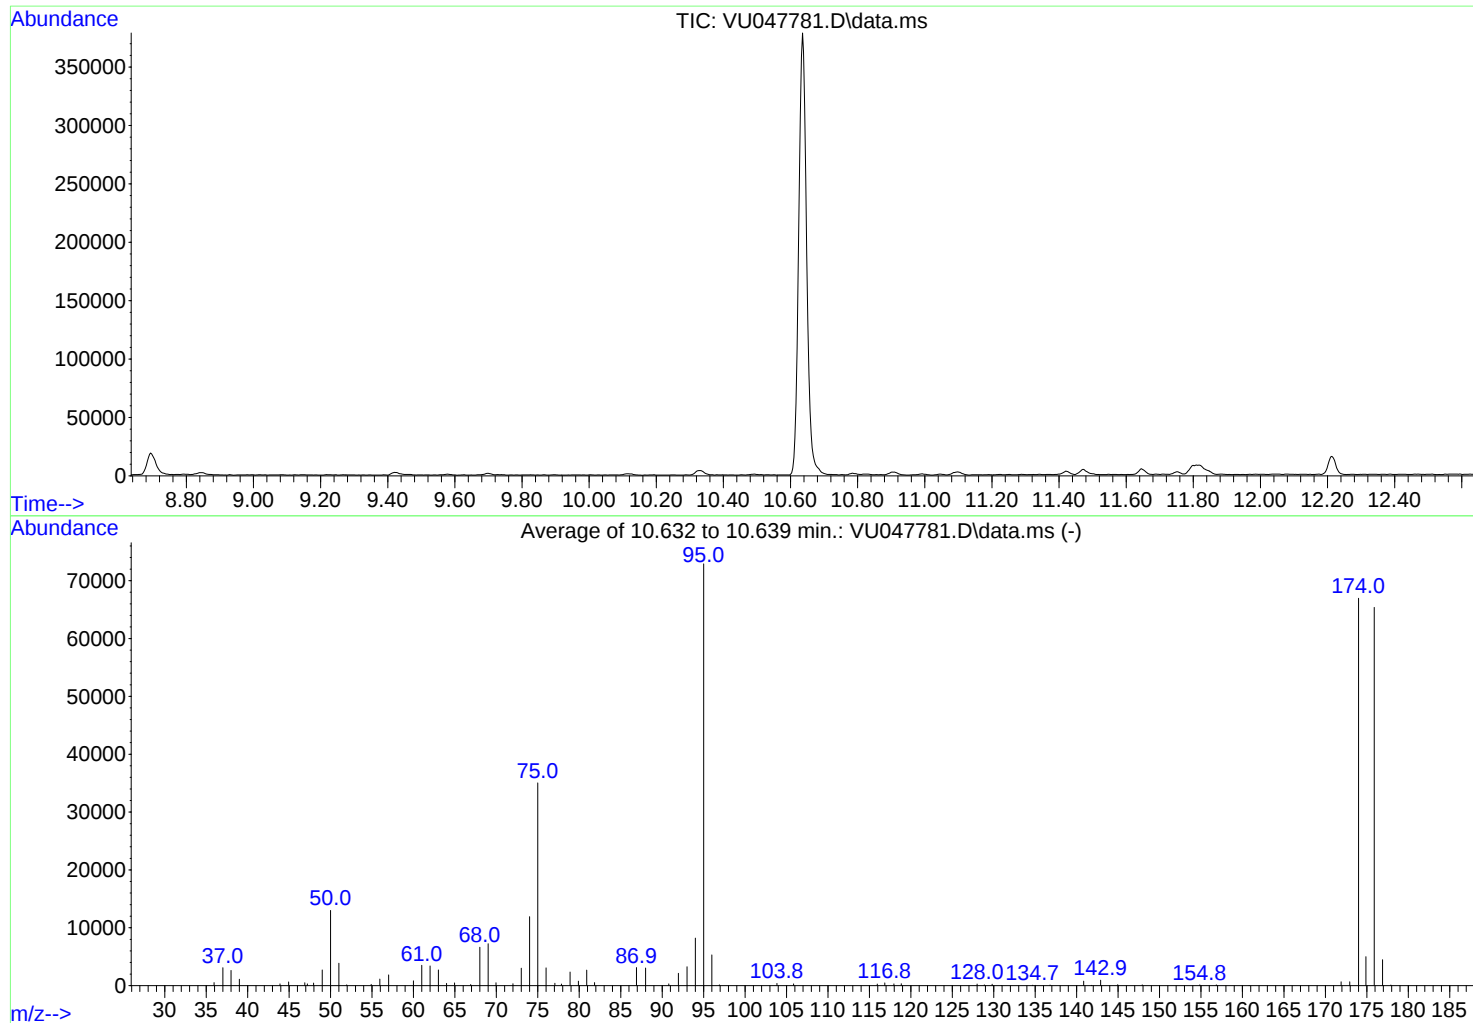

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	13012	PASS
75	95	30	80	48.1	35040	PASS
95	95	100	100	100.0	72909	PASS
96	95	5	9	7.3	5315	PASS
173	174	0.00	2	1.0	670	PASS
174	95	50	120	91.8	66963	PASS
175	174	5	9	7.5	5002	PASS
176	174	95	101	97.6	65381	PASS
177	176	5	9	6.9	4487	PASS

m/z	Abundance
35.90	526.0
37.00	3172.0
38.00	2691.0
39.00	1139.0
40.00	391.0
43.90	690.0
44.90	648.0
46.90	472.0
47.20	445.0
48.00	471.0
49.00	2810.0
50.00	13553.0
51.00	3966.0
51.90	140.0
54.90	231.0
56.00	1142.0
57.00	1903.0
60.00	911.0
61.00	3642.0
62.00	3480.0
63.00	2798.0
64.00	400.0
64.90	465.0
66.90	197.0
68.00	6865.0
69.00	7551.0
70.00	526.0
72.00	331.0
73.00	3137.0
74.00	12287.0
75.00	36184.0
76.00	3213.0
77.10	438.0
77.90	286.0
78.90	2452.0
79.90	808.0
80.90	2802.0
81.90	536.0
86.90	3272.0
88.00	3233.0
90.80	335.0
91.90	2222.0
93.00	3356.0
94.00	8424.0
95.00	75216.0
96.00	5459.0
96.90	138.0
103.90	421.0
105.80	314.0
116.00	302.0
116.90	483.0
118.00	317.0
118.80	341.0
128.00	285.0
128.80	144.0
129.80	256.0
134.70	128.0
136.80	121.0
140.90	775.0
141.80	101.0
142.90	975.0
145.00	176.0
147.90	151.0
154.90	147.0
156.80	135.0
171.90	690.0
173.00	692.0
174.00	69344.0
174.90	5192.0
175.90	67448.0
176.90	4662.0
177.90	166.0

Instrument :
MSVOA_U
ClientSampleId :
BFB058

m/z	Abundance
36.00	543.0
37.00	3069.0
38.00	2578.0
39.00	1064.0
40.00	463.0
44.00	661.0
44.90	615.0
46.90	487.0
47.20	487.0
48.00	407.0
49.00	2728.0
50.00	12546.0
51.00	3781.0
52.00	135.0
54.90	226.0
56.00	1093.0
57.00	1822.0
60.00	805.0
61.00	3132.0
62.00	3298.0
63.00	2586.0
64.00	360.0
64.90	504.0
66.90	214.0
68.00	6369.0
69.00	7110.0
69.90	474.0
72.00	334.0
73.00	2927.0
74.00	11542.0
75.00	33728.0
76.00	2829.0
77.10	370.0
77.90	285.0
78.90	2248.0
79.90	765.0
80.90	2513.0
81.80	545.0
86.90	3150.0
88.00	2994.0
90.80	298.0
92.00	2144.0
93.00	3347.0
94.00	7896.0
95.00	72384.0
96.00	5376.0
96.90	147.0
103.80	388.0
105.80	292.0
115.90	285.0
116.80	552.0
117.90	301.0
118.90	311.0
128.00	256.0
128.90	141.0
129.80	241.0
130.90	101.0
134.70	154.0
135.00	146.0
136.80	118.0
140.80	786.0
142.90	885.0
145.00	204.0
147.90	160.0
154.90	178.0
156.80	183.0
160.80	118.0
171.90	718.0
173.00	708.0
174.00	67360.0
174.90	4850.0
175.90	65736.0
176.90	4457.0

Instrument :
MSVOA_U
ClientSampleId :
BFB058

m/z	Abundance
39.80	428.0
43.90	374.0

Instrument :
MSVOA_U
ClientSampleId :
BFB058

m/z	Abundance
35.90	534.0
37.00	3076.0
38.00	2611.0
39.00	1157.0
39.90	387.0
43.90	696.0
45.00	623.0
46.90	521.0
47.90	497.0
49.00	2631.0
50.00	12938.0
51.00	3883.0
51.90	163.0
54.90	185.0
55.90	1160.0
57.00	1846.0
60.00	809.0
61.00	3739.0
62.00	3436.0
63.00	2732.0
64.00	411.0
65.00	414.0
66.90	146.0
68.00	6685.0
69.00	7059.0
70.00	540.0
72.00	338.0
73.00	2998.0
74.00	11968.0
75.00	35208.0
76.00	3213.0
77.00	449.0
77.80	252.0
78.90	2386.0
79.90	768.0
80.90	2751.0
81.90	548.0
86.90	2944.0
88.00	2869.0
90.80	313.0
91.90	2071.0
93.00	3072.0
94.00	8372.0
95.00	71128.0
96.00	5111.0
96.90	114.0
103.90	382.0
105.90	283.0
116.00	280.0
116.90	415.0
117.90	285.0
118.80	350.0
128.00	269.0
128.80	127.0
129.80	250.0
136.80	121.0
140.90	732.0
141.80	108.0
142.90	926.0
144.90	162.0
147.90	141.0
154.80	124.0
156.90	101.0
171.90	558.0
172.90	610.0
174.00	64184.0
174.90	4963.0
175.90	62960.0
176.90	4341.0
177.90	214.0

Instrument :
MSVOA_U
ClientSampleId :
BFB058