

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040124\
 Data File : VU058311.D
 Acq On : 01 Apr 2024 14:19
 Operator : MD/SY
 Sample : P1912-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCOD6

Quant Time: Apr 02 02:27:20 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032124WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Apr 02 02:24:47 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	74188	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	72548	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	32188	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	27055	4.315	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.400%
7) Chloroethane-d5	1.907	69	26230	5.126	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.600%
11) 1,1-Dichloroethene-d2	2.560	65	11904	4.573	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	91.400%
20) 2-Butanone-d5	4.621	46	56004	50.282	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.560%
24) Chloroform-d	5.052	84	53165	4.743	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.800%
26) 1,2-Dichloroethane-d4	5.692	65	26393	5.037	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.800%
32) Benzene-d6	5.721	84	110294	4.681	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.600%
36) 1,2-Dichloropropane-d6	6.682	67	34256	4.933	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.600%
41) Toluene-d8	7.891	98	92030	4.409	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.200%
43) trans-1,3-Dichloroprop...	8.174	79	9459	4.251	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.000%
46) 2-Hexanone-d5	8.627	63	42300	46.940	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.880%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	21262	4.700	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.000%
66) 1,2-Dichlorobenzene-d4	12.187	152	30573	5.101	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.000%
Target Compounds						
17) Methyl tert-butyl Ether	3.354	73	14524	1.455	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040124\
Data File : VU058311.D
Acq On : 01 Apr 2024 14:19
Operator : MD/SY
Sample : P1912-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCOD6


Quant Time: Apr 02 02:27:20 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032124WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Apr 02 02:24:47 2024
Response via : Initial Calibration

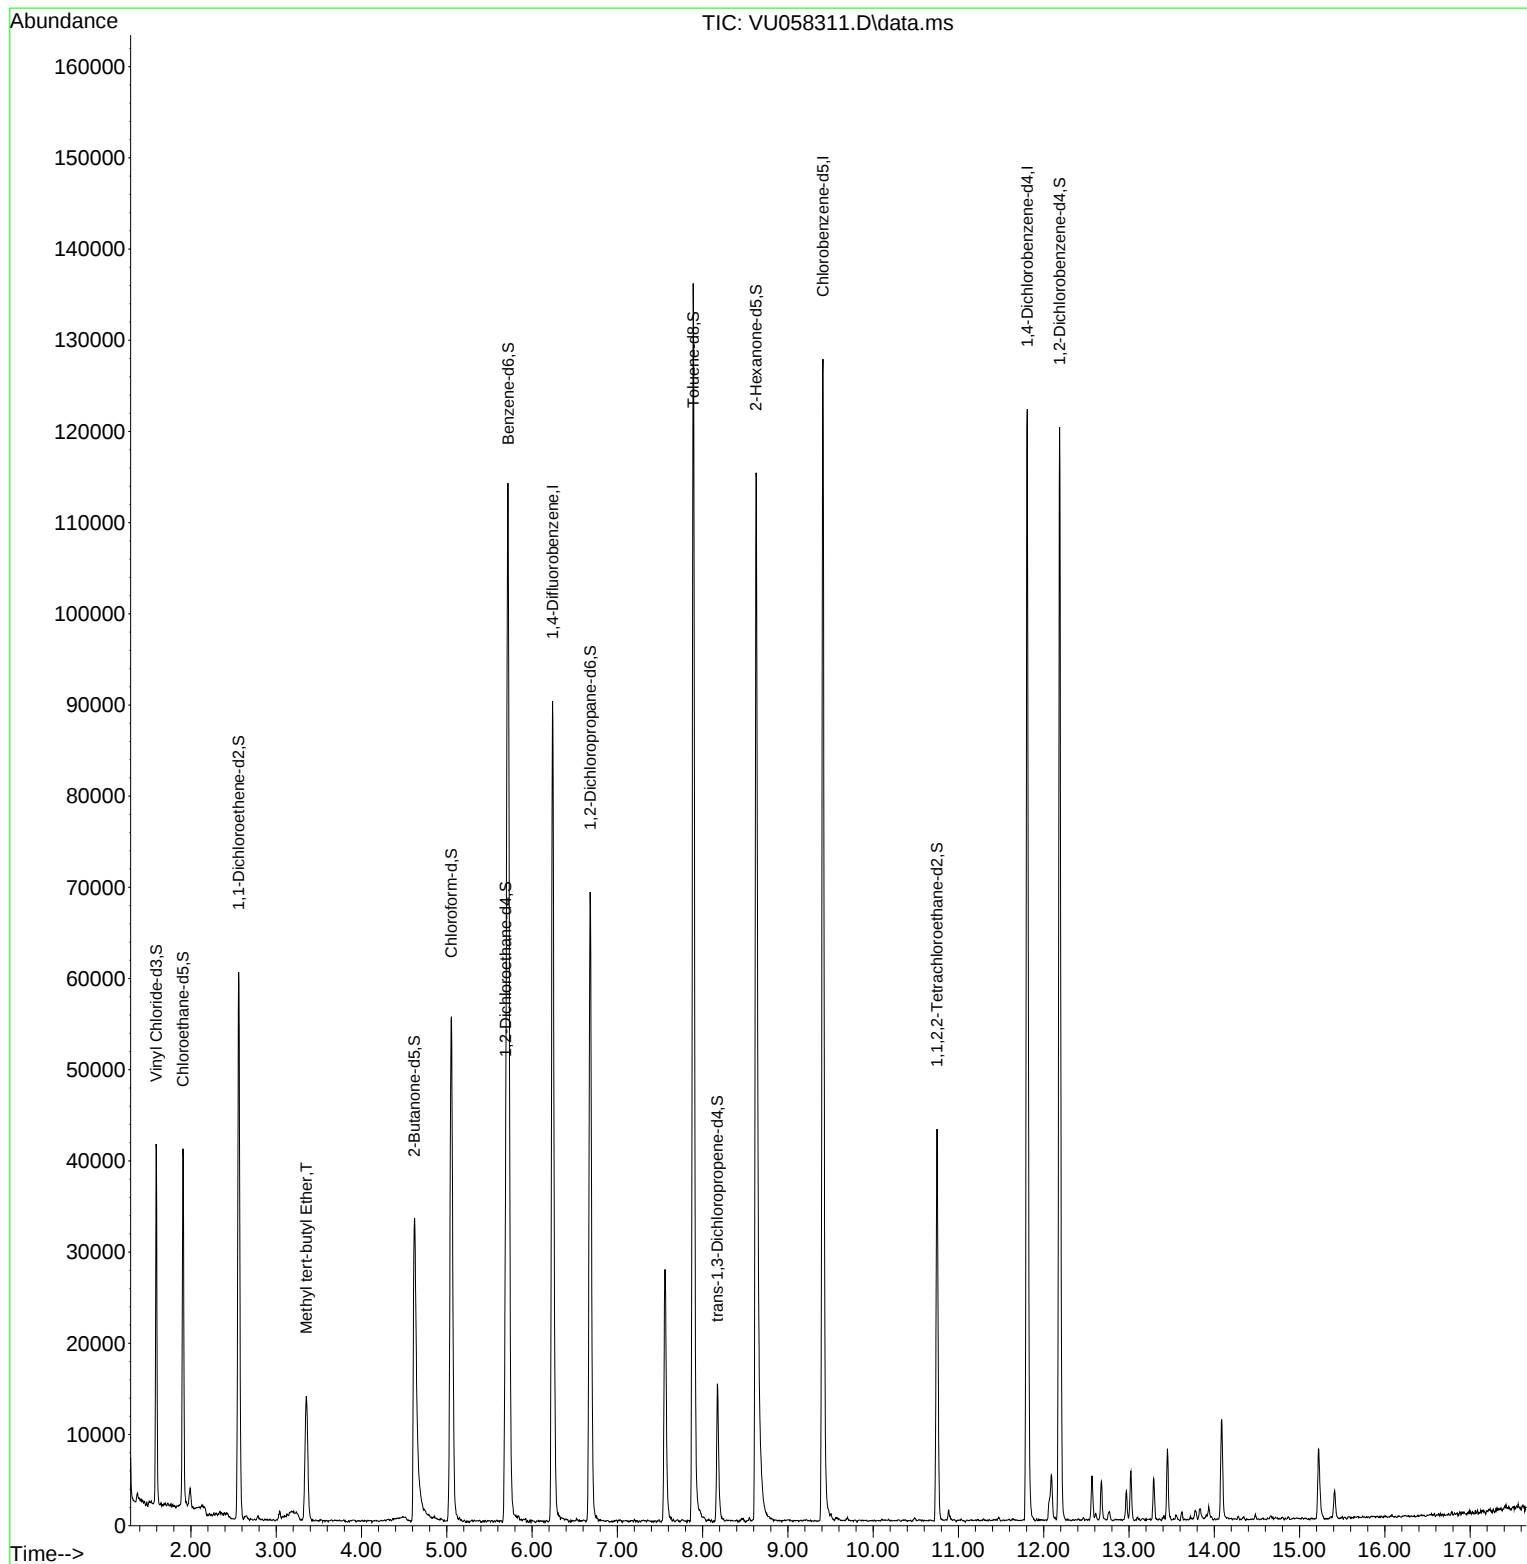

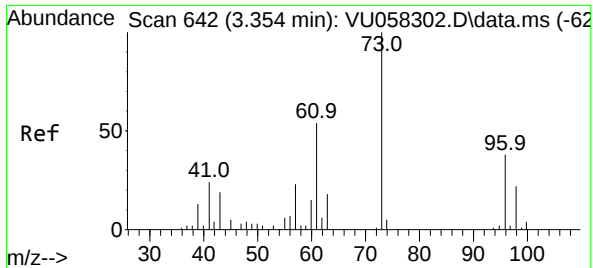

#17
Methyl tert-butyl Ether
Concen: 1.455 ug/L
RT: 3.354 min Scan# 64
Delta R.T. 0.000 min
Lab File: VU058311.D
Acq: 01 Apr 2024 14:19

Instrument :
MSVOA_U
ClientSampleId :
DCOD6

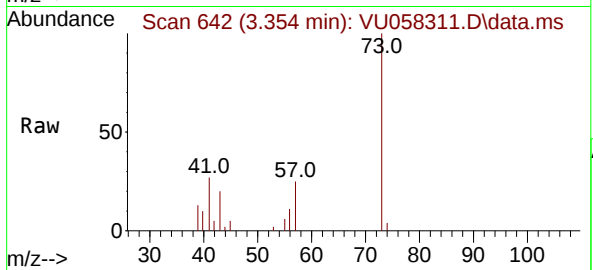

Tgt Ion:	73	Resp:	14524
Ion	Ratio	Lower	Upper
73	100		
43	19.6	15.5	23.3
57	26.6	18.0	27.0

