
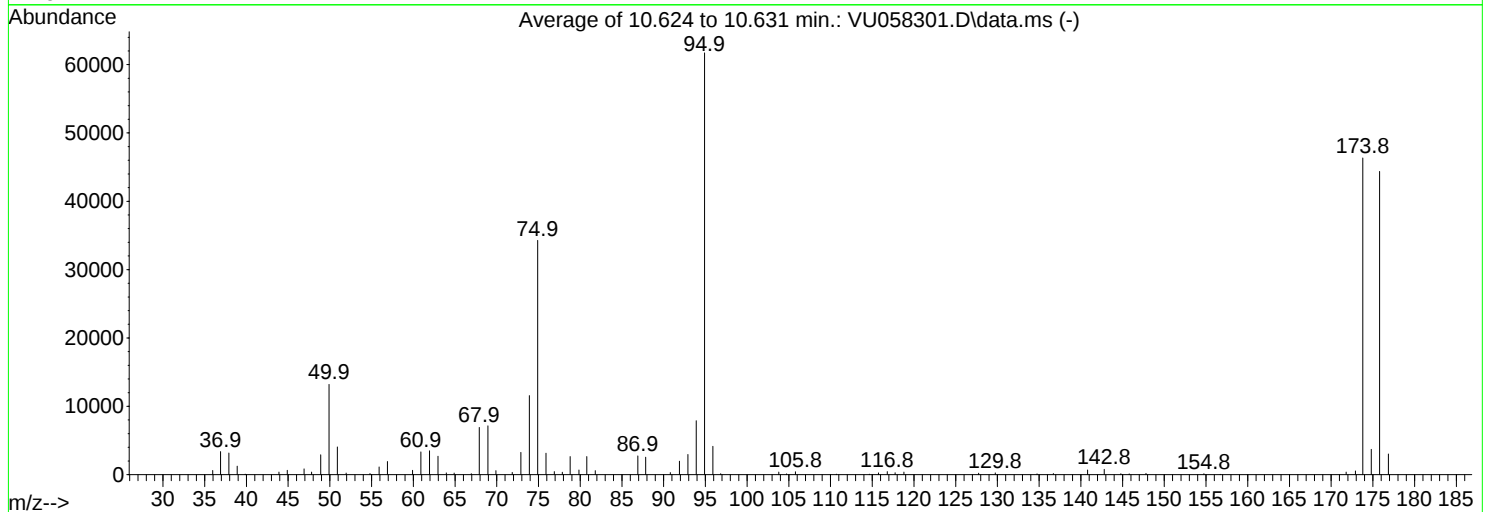


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040124\
Data File : VU058301.D
Acq On : 01 Apr 2024 09:01
Operator : MD/SY
Sample : BFB133
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB133

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032124WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Apr 02 02:24:47 2024

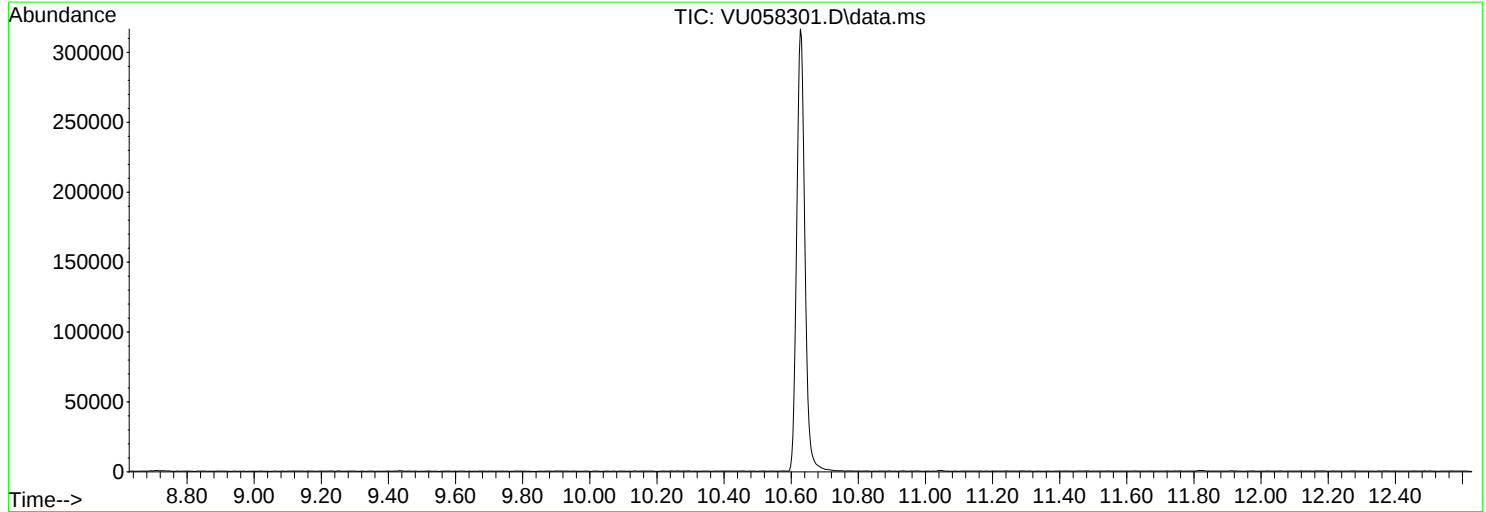

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	13210	PASS
75	95	30	80	55.5	34275	PASS
95	95	100	100	100.0	61723	PASS
96	95	5	9	6.7	4152	PASS
173	174	0.00	2	1.2	548	PASS
174	95	50	120	75.1	46331	PASS
175	174	5	9	8.0	3697	PASS
176	174	95	101	95.8	44381	PASS
177	176	5	9	6.8	3031	PASS

m/z	Abundance
39.80	409.0
43.80	121.0

Instrument :
MSVOA_U
ClientSampleId :
BFB133

m/z	Abundance
36.00	592.0
36.90	3301.0
37.90	3045.0
38.90	1205.0
39.90	531.0
43.90	486.0
44.90	613.0
46.90	810.0
47.80	376.0
48.90	2855.0
49.90	13134.0
50.90	4025.0
52.00	210.0
54.80	166.0
55.90	1143.0
56.90	1868.0
59.90	632.0
60.90	3389.0
62.00	3410.0
63.00	2685.0
64.00	251.0
64.90	276.0
66.90	147.0
67.90	6712.0
69.00	6976.0
69.90	540.0
71.80	346.0
72.90	3162.0
73.90	11322.0
74.90	33168.0
75.90	3043.0
76.90	384.0
77.80	322.0
78.80	2620.0
79.90	667.0
80.80	2596.0
81.80	575.0
86.90	2603.0
87.80	2451.0
90.80	301.0
91.90	1906.0
92.90	2956.0
93.90	7622.0
94.90	59488.0
95.90	3970.0
96.80	132.0
103.80	371.0
104.70	111.0
105.80	387.0
110.70	109.0
115.80	265.0
116.80	407.0
117.70	272.0
118.80	374.0
127.70	176.0
129.80	219.0
134.70	112.0
136.70	131.0
140.80	595.0
142.80	747.0
144.70	136.0
145.70	106.0
147.80	178.0
154.80	139.0
171.80	363.0
172.90	519.0
173.80	44224.0
174.80	3558.0
175.80	42256.0
176.90	2843.0

Instrument :
MSVOA_U
ClientSampleId :
BFB133

m/z	Abundance
36.00	619.0
36.90	3465.0
37.90	3241.0
38.90	1274.0
39.90	482.0
44.00	490.0
44.90	637.0
46.90	871.0
47.80	393.0
48.90	2977.0
49.90	13531.0
50.90	4167.0
52.00	242.0
54.80	176.0
55.90	1135.0
56.90	1978.0
59.90	653.0
60.90	3392.0
61.90	3553.0
63.00	2775.0
64.00	259.0
64.90	247.0
66.90	147.0
67.90	7100.0
68.90	7396.0
69.90	600.0
71.80	345.0
72.90	3333.0
73.90	11924.0
74.90	35264.0
75.90	3237.0
76.90	446.0
77.90	371.0
78.80	2746.0
79.80	682.0
80.80	2701.0
81.80	616.0
86.90	2782.0
87.90	2653.0
90.80	310.0
91.90	2022.0
92.90	3010.0
93.90	8176.0
94.90	63448.0
95.90	4305.0
96.80	147.0
103.80	384.0
104.80	132.0
105.80	452.0
110.70	116.0
114.60	108.0
115.70	271.0
116.80	443.0
117.80	287.0
118.80	403.0
127.80	218.0
129.70	260.0
134.80	114.0
136.70	166.0
140.80	678.0
142.80	808.0
144.80	138.0
145.80	110.0
147.80	195.0
154.70	139.0
171.80	395.0
172.90	554.0
173.80	47648.0
174.80	3826.0
175.80	45432.0
176.80	3117.0

Instrument :
MSVOA_U
ClientSampleId :
BFB133

m/z	Abundance
35.90	592.0
36.90	3364.0
37.90	3200.0
38.90	1259.0
39.90	464.0
43.90	517.0
44.90	625.0
46.90	828.0
47.80	352.0
48.90	2853.0
49.90	12966.0
50.90	3933.0
51.90	224.0
54.80	189.0
55.90	1083.0
56.90	1888.0
59.90	624.0
60.90	3175.0
61.90	3483.0
62.90	2644.0
63.90	268.0
64.90	211.0
67.00	143.0
67.90	6931.0
68.90	7062.0
69.90	624.0
71.90	301.0
72.90	3279.0
73.90	11446.0
74.90	34392.0
75.90	3164.0
76.90	488.0
77.80	363.0
78.80	2587.0
79.80	663.0
80.80	2620.0
81.80	601.0
86.90	2838.0
87.80	2540.0
90.80	289.0
91.90	1978.0
92.90	2878.0
93.90	7851.0
94.90	62232.0
95.90	4182.0
96.90	128.0
103.80	350.0
104.80	126.0
105.80	442.0
114.70	105.0
115.70	243.0
116.80	456.0
117.80	270.0
118.80	374.0
127.80	232.0
129.70	287.0
134.80	107.0
136.70	175.0
140.80	741.0
142.80	796.0
144.90	126.0
145.90	107.0
147.80	190.0
154.70	122.0
156.70	111.0
171.80	397.0
172.90	571.0
173.80	47120.0
174.80	3707.0
175.80	45456.0
176.80	3134.0

Instrument :
MSVOA_U
ClientSampleId :
BFB133