

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040219\
Data File : VU030613.D
Acq On : 02 Apr 2019 21:13
Operator : JC/SP
Sample : I.BLK
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK46

Quant Time: Apr 03 18:51:33 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\524U040219DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Wed Apr 03 02:39:21 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene	5.74	96	32717	1.00	ug/l	0.00

System Monitoring Compounds

57) 4-Bromofluorobenzene	10.31	95	10802	0.93	ug/l	0.00
Spiked Amount 1.000			Recovery	=	93.00%	
68) 1,2-Dichlorobenzene-d4	11.86	152	10761	0.97	ug/l	0.00
Spiked Amount 1.000			Recovery	=	97.00%	


Target Compounds	Ovalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU040219\
Data File : VU030613.D
Acq On : 02 Apr 2019 21:13
Operator : JC/SP
Sample : I.BLK
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK46

Quant Time: Apr 03 18:51:33 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U040219DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Wed Apr 03 02:39:21 2019
Response via : Initial Calibration

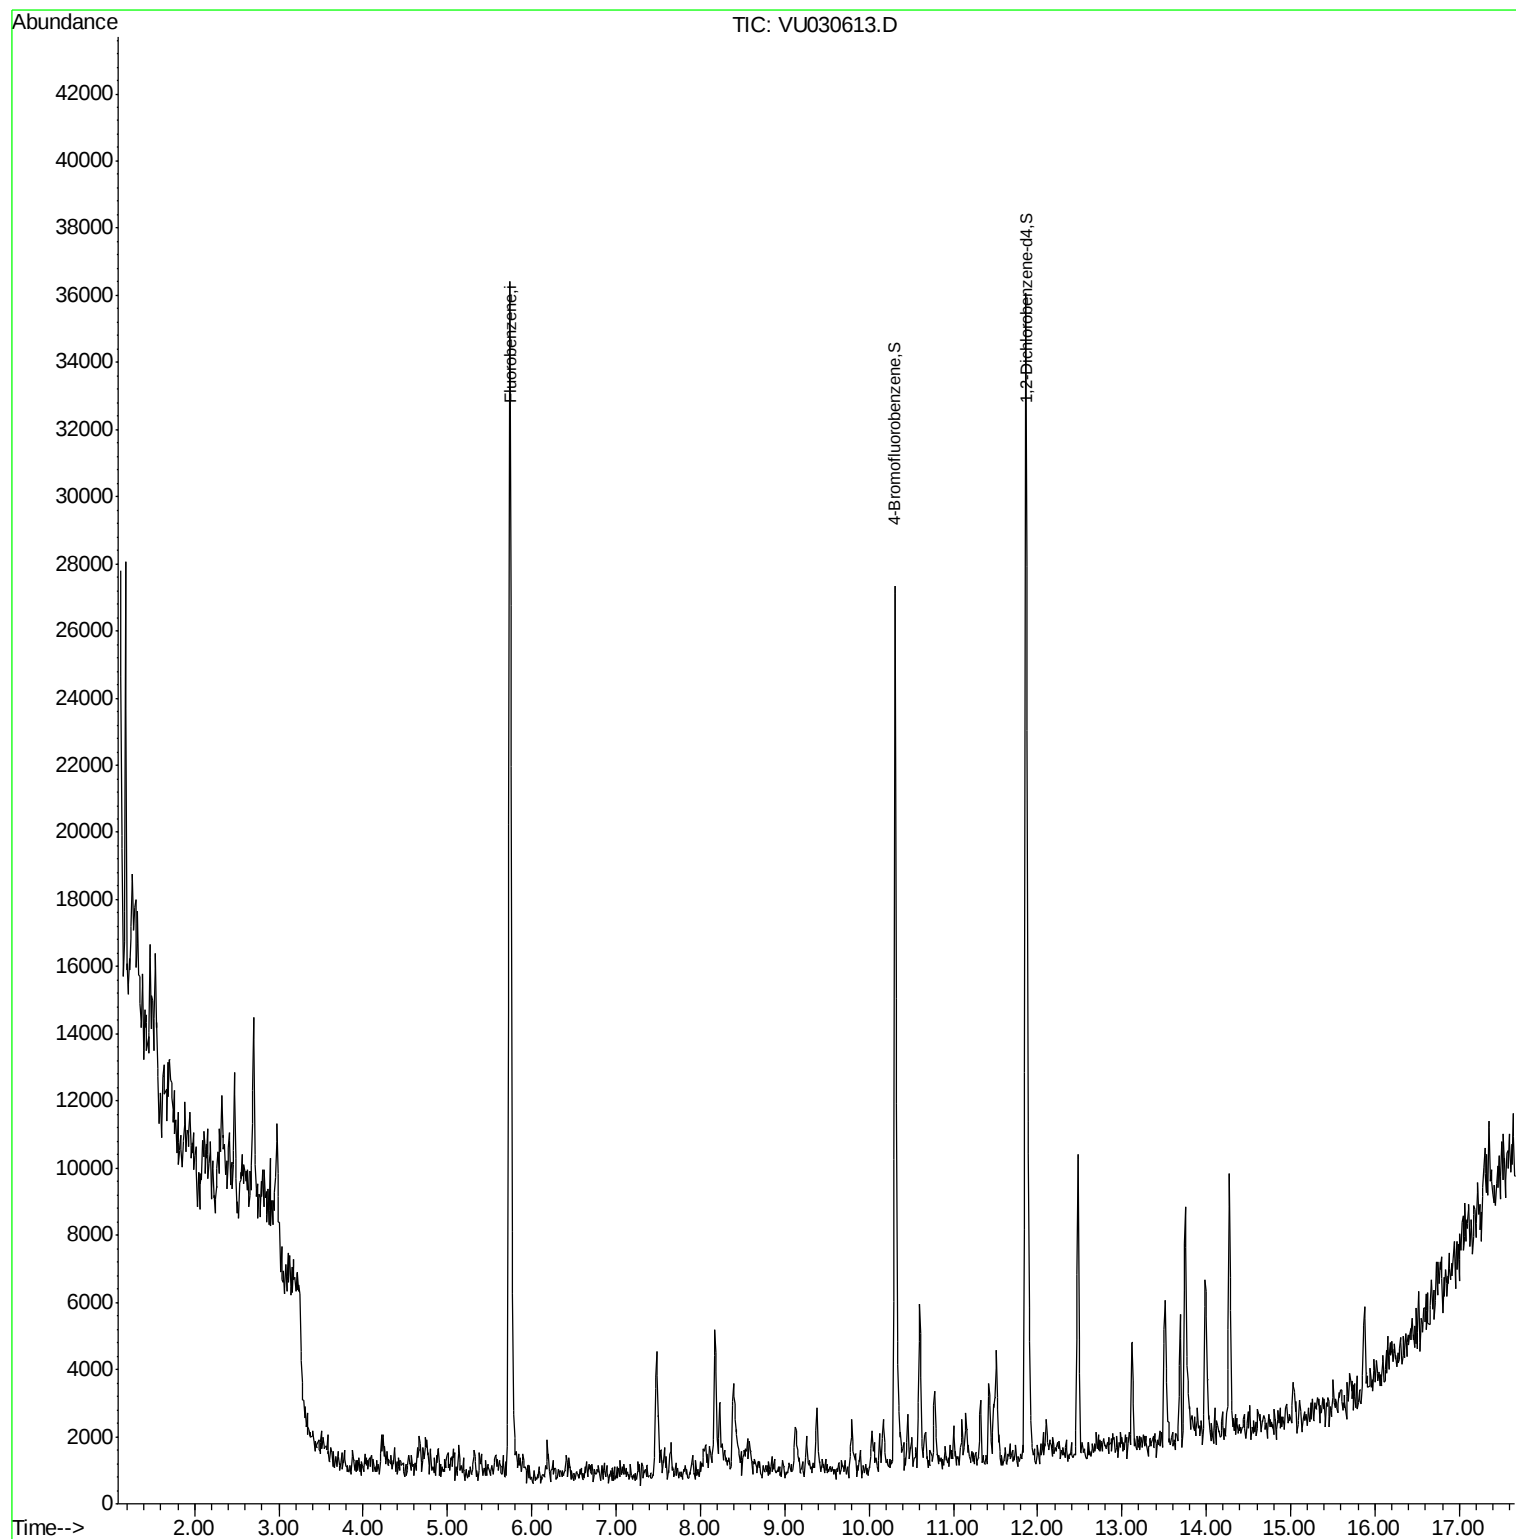

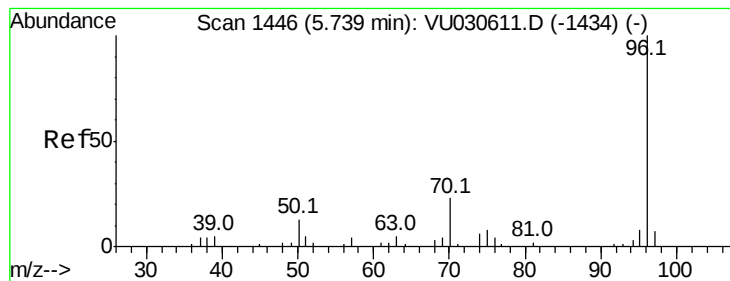

#1

Fluorobenzene

Concen: 1.000 ug/l

RT: 5.74 min Scan# 1447

Delta R.T. 0.00 min

Lab File: VU030613.D

Acq: 02 Apr 2019 21:13

Instrument :

MSVOA_U

ClientSampleId :

VBLK46

Tot Ion: 96 Resp: 32717


Ion Ratio Lower Upper

96 100

70 21.0 18.5 27.7

95 9.3 0.0 0.0#

97 6.9 0.0 0.0#



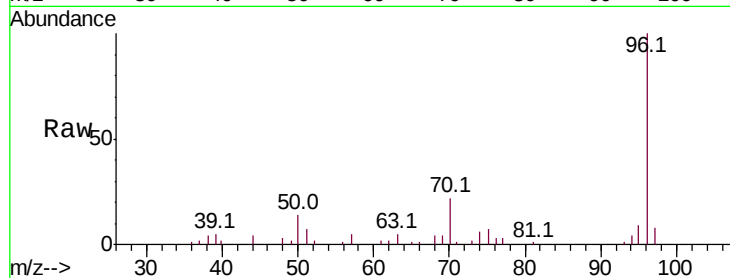


Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 70.00 (69.70 to 70.70): VU0

Ion 95.00 (94.70 to 95.70): VU0

Ion 97.00 (96.70 to 97.70): VU0

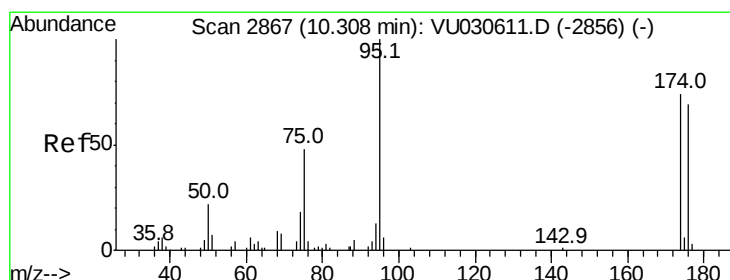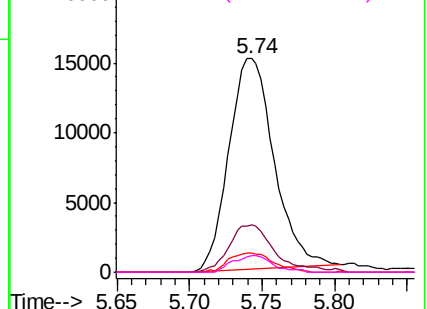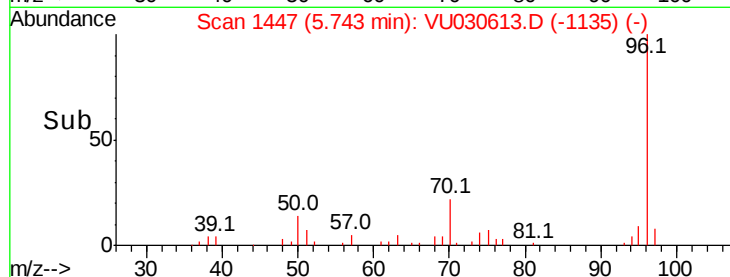

#57

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 10.31 min Scan# 2867

Delta R.T. 0.00 min

Lab File: VU030613.D

Acq: 02 Apr 2019 21:13


Tgt Ion: 95 Resp: 10802

Ion Ratio Lower Upper

95 100

174 75.9 59.1 88.7



176 65.8 55.7 83.5

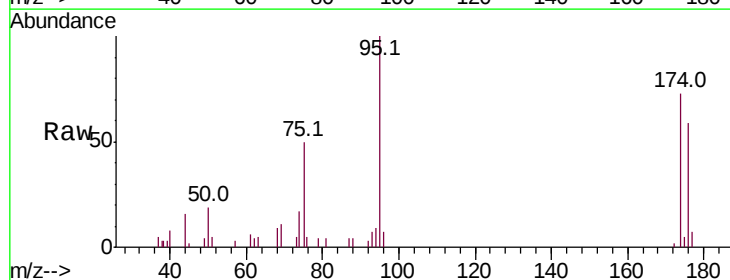


Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 174.00 (173.70 to 174.70): V

Ion 176.00 (175.70 to 176.70): V

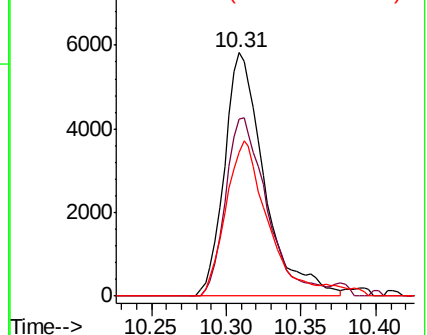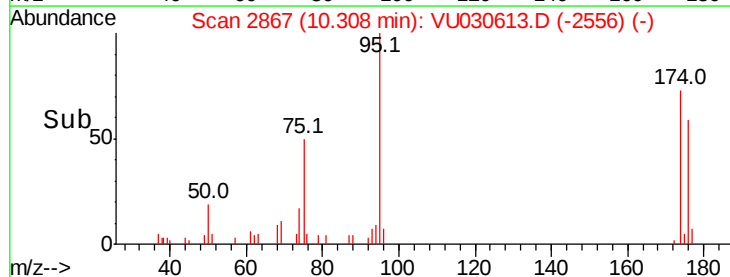


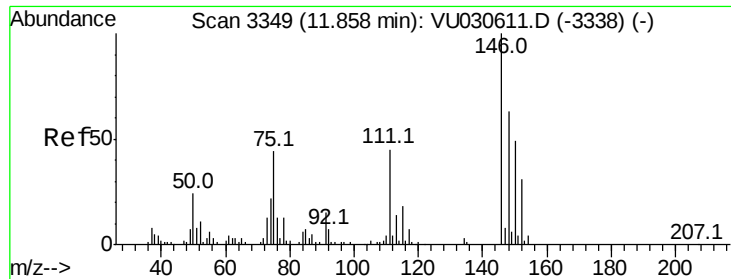

#68
 1,2-Dichlorobenzene-d4
 Concen: N.D. ug/l
 RT: 11.86 min Scan# 3351
 Delta R.T. 0.01 min
 Lab File: VU030613.D
 Acq: 02 Apr 2019 21:13

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK46

Tot Ion	Ratio	Lower	Upper
152	100		
115	62.3	0.0	122.4
150	150.2	0.0	595.2

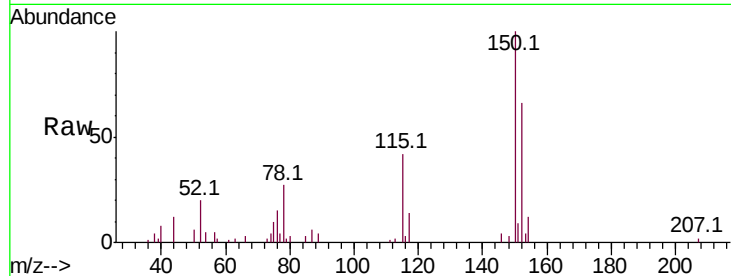

Abundance

Ion 152.00 (151.70 to 152.70): V

Ion 115.00 (114.70 to 115.70): V

Ion 150.00 (149.70 to 150.70): V

