


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040219\
 Data File : VU030606.D
 Acq On : 02 Apr 2019 17:32
 Operator : JC/SP
 Sample : BFB
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U040219DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Wed Apr 03 02:39:21 2019

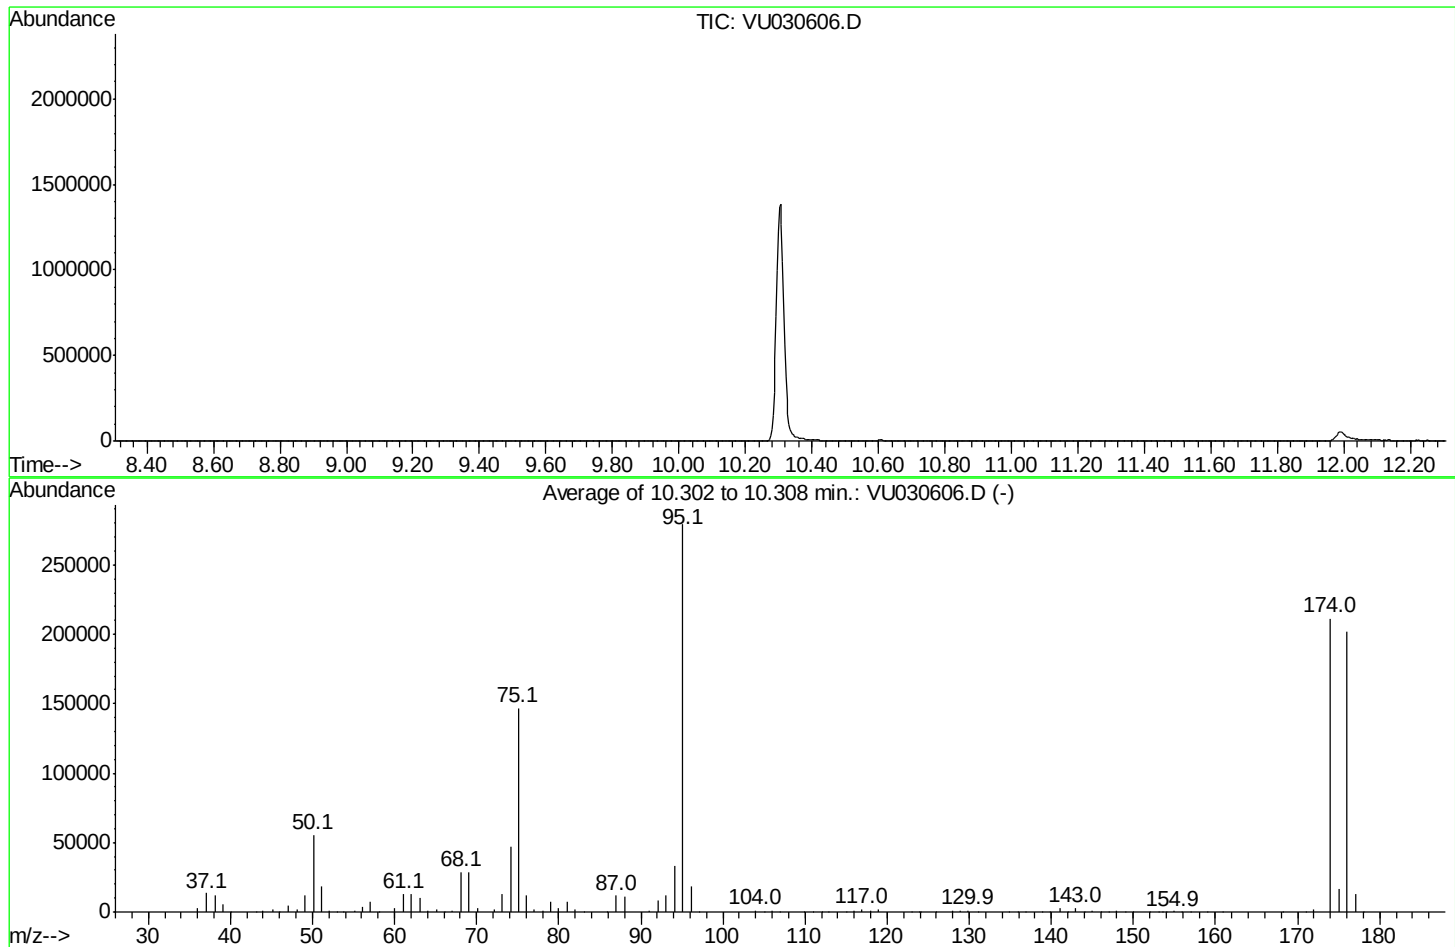

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2851

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	55805	PASS
75	95	30	60	52.6	146837	PASS
95	95	100	100	100.0	279210	PASS
96	95	5	9	6.6	18533	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	75.7	211285	PASS
175	174	5	9	7.9	16765	PASS
176	174	95	101	95.5	201792	PASS
177	176	5	9	6.6	13388	PASS