


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU040220\
 Data File : VU037545.D
 Acq On : 02 Apr 2020 08:55
 Operator : JC/MD
 Sample : BFB12
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB12

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR040120WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Apr 03 00:57:17 2020

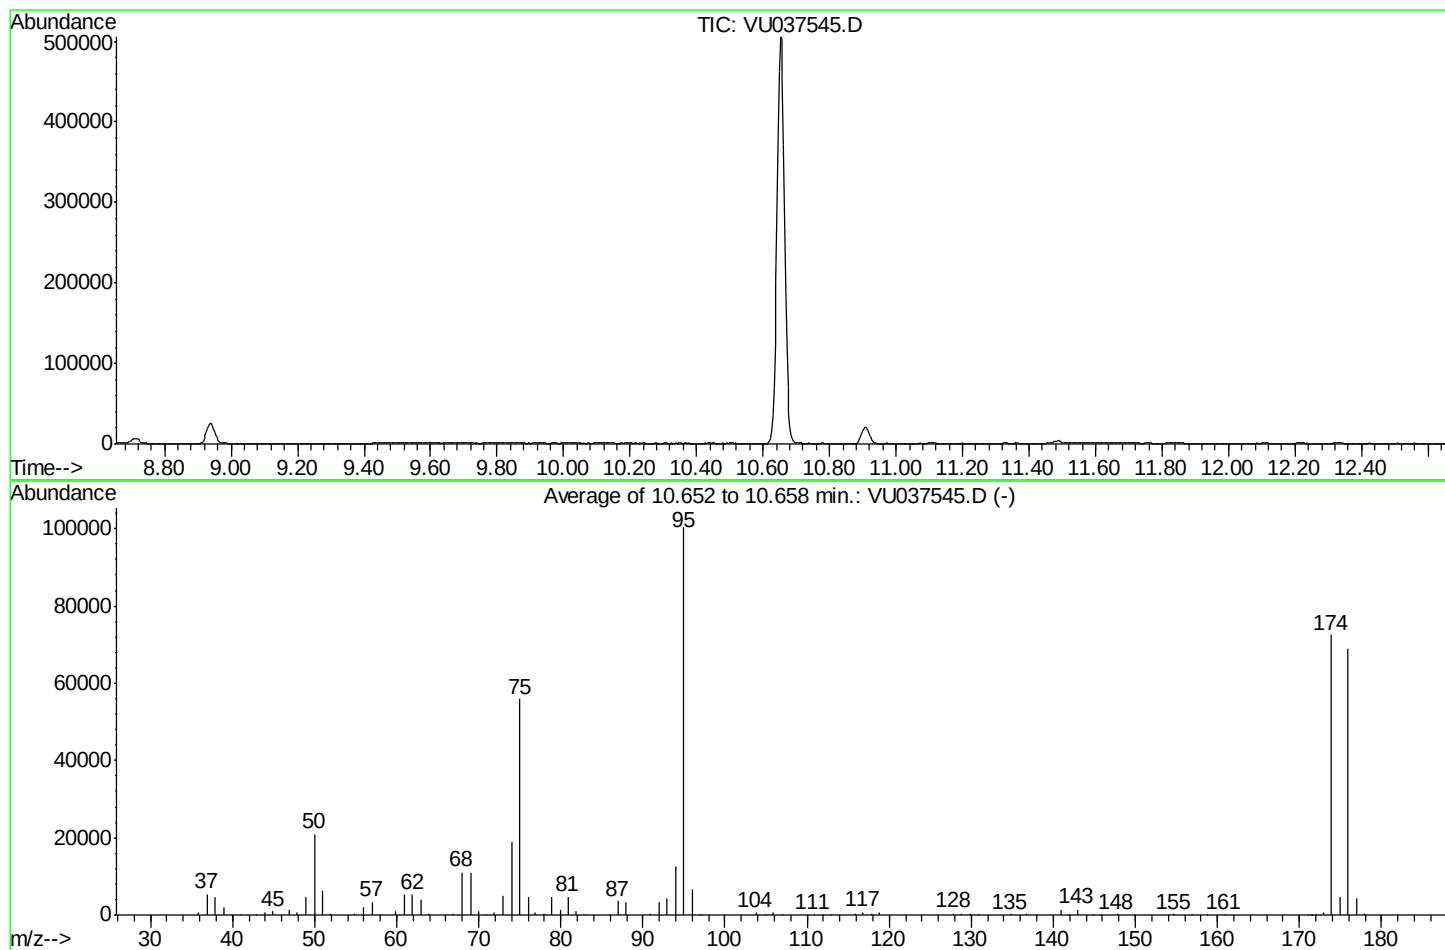

AutoFind: Scans 2896, 2897, 2898; Background Corrected with Scan 2882

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	20904	PASS
75	95	30	80	55.7	55906	PASS
95	95	100	100	100.0	100349	PASS
96	95	5	9	6.5	6567	PASS
173	174	0.00	2	0.9	619	PASS
174	95	50	120	72.3	72512	PASS
175	174	5	9	6.5	4709	PASS
176	174	95	101	95.1	68981	PASS
177	176	5	9	6.5	4450	PASS

m/z	Abundance
35.90	1267.0
36.90	5745.0
37.90	4958.0
39.00	1985.0
40.00	180.0
40.90	122.0
42.90	146.0
43.90	872.0
44.90	1004.0
46.90	1162.0
47.90	601.0
49.00	4839.0
50.00	22064.0
51.00	6575.0
52.00	205.0
54.90	254.0
56.00	1958.0
57.00	3804.0
57.90	180.0
59.90	1143.0
60.90	5475.0
61.90	5487.0
62.90	4222.0
63.90	467.0
66.80	245.0
67.90	11630.0
69.00	10971.0
69.90	905.0
70.90	145.0
71.90	810.0
72.90	5074.0
74.00	19800.0
75.00	58552.0
76.00	4915.0
76.80	647.0
78.00	497.0
78.90	4820.0
79.90	1266.0
80.90	4787.0
81.80	989.0
82.90	141.0
85.90	139.0
87.00	3675.0
87.90	3353.0
90.90	516.0
92.00	3325.0
92.90	4639.0
94.00	13744.0
95.00	103616.0
96.00	6898.0
97.10	183.0
103.80	610.0
104.90	148.0
105.80	597.0
106.90	108.0
110.90	116.0
112.00	114.0
112.90	156.0
115.90	426.0
116.80	740.0
117.80	406.0
118.80	562.0
127.90	467.0
128.80	181.0
129.90	380.0
130.90	139.0
134.80	308.0
136.70	197.0
140.90	1376.0
141.80	156.0
142.90	1511.0
145.80	144.0
147.80	291.0
149.80	176.0
154.70	203.0
156.80	147.0
171.10	146.0
172.00	233.0
172.90	640.0
173.90	74160.0
174.90	4887.0
175.90	69912.0
176.90	4791.0
177.90	219.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12

m/z	Abundance
35.90	1129.0
36.90	5540.0
37.90	4871.0
39.00	1953.0
39.90	174.0
42.90	140.0
43.90	864.0
44.90	995.0
46.90	1246.0
47.90	533.0
48.90	4755.0
50.00	21632.0
51.00	6465.0
52.00	192.0
54.80	273.0
56.00	2005.0
57.00	3520.0
57.90	132.0
59.90	1075.0
60.90	5279.0
61.90	5409.0
62.90	4074.0
63.90	451.0
66.90	231.0
67.90	11394.0
69.00	11129.0
70.00	922.0
71.90	677.0
73.00	5123.0
74.00	19384.0
75.00	57504.0
76.00	4716.0
76.80	529.0
77.90	516.0
78.90	4792.0
79.90	1275.0
80.90	4822.0
81.80	1000.0
82.80	127.0
85.90	142.0
87.00	3630.0
87.90	3566.0
90.90	445.0
91.90	3357.0
92.90	4453.0
94.00	13009.0
95.00	103656.0
96.00	6773.0
97.10	167.0
103.80	601.0
104.90	178.0
105.80	575.0
107.00	100.0
110.90	128.0
112.00	129.0
112.80	193.0
115.80	450.0
116.80	754.0
117.80	392.0
118.70	585.0
127.90	441.0
128.80	205.0
129.90	314.0
130.80	136.0
134.80	325.0
136.70	255.0
140.90	1298.0
141.90	130.0
142.90	1509.0
145.80	175.0
147.80	237.0
149.80	177.0
154.70	214.0
156.80	116.0
158.70	114.0
171.30	146.0
172.90	648.0
173.90	75064.0
174.90	4863.0
175.90	71128.0
176.90	4558.0
177.90	200.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12

m/z	Abundance
35.90	904.0
36.90	4805.0
37.90	4213.0
39.00	1698.0
39.90	157.0
42.90	127.0
43.90	785.0
44.90	833.0
46.90	1275.0
47.90	503.0
48.90	4278.0
50.00	19016.0
51.00	5898.0
51.90	201.0
54.80	261.0
56.00	1866.0
57.00	3033.0
57.90	115.0
59.90	939.0
61.00	4719.0
61.90	4897.0
62.90	3728.0
63.90	365.0
67.00	231.0
68.00	10290.0
69.00	10267.0
70.00	878.0
71.90	512.0
72.90	4516.0
74.00	17432.0
75.00	51664.0
76.00	4090.0
76.90	466.0
77.90	470.0
78.80	4424.0
79.90	1176.0
80.90	4394.0
81.80	956.0
82.80	107.0
86.90	3335.0
87.90	3367.0
90.80	373.0
91.90	3217.0
92.90	3764.0
94.00	10943.0
95.00	93776.0
96.00	6030.0
96.80	112.0
103.80	556.0
104.90	192.0
105.80	538.0
110.80	100.0
112.80	186.0
115.80	416.0
116.80	733.0
117.80	359.0
118.70	553.0
127.90	413.0
128.70	186.0
129.90	287.0
130.90	125.0
134.80	269.0
136.70	235.0
140.90	1055.0
142.90	1387.0
144.80	132.0
145.90	161.0
147.80	150.0
149.80	134.0
154.70	189.0
158.70	125.0
160.90	105.0
171.50	165.0
172.90	570.0
173.90	68312.0
174.90	4377.0
175.90	65904.0
176.90	4001.0
177.90	157.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12

Scan 2882 (10.607 min): VU037545.D
BFB12

m/z	Abundance
35.90	289.0
43.90	245.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12