
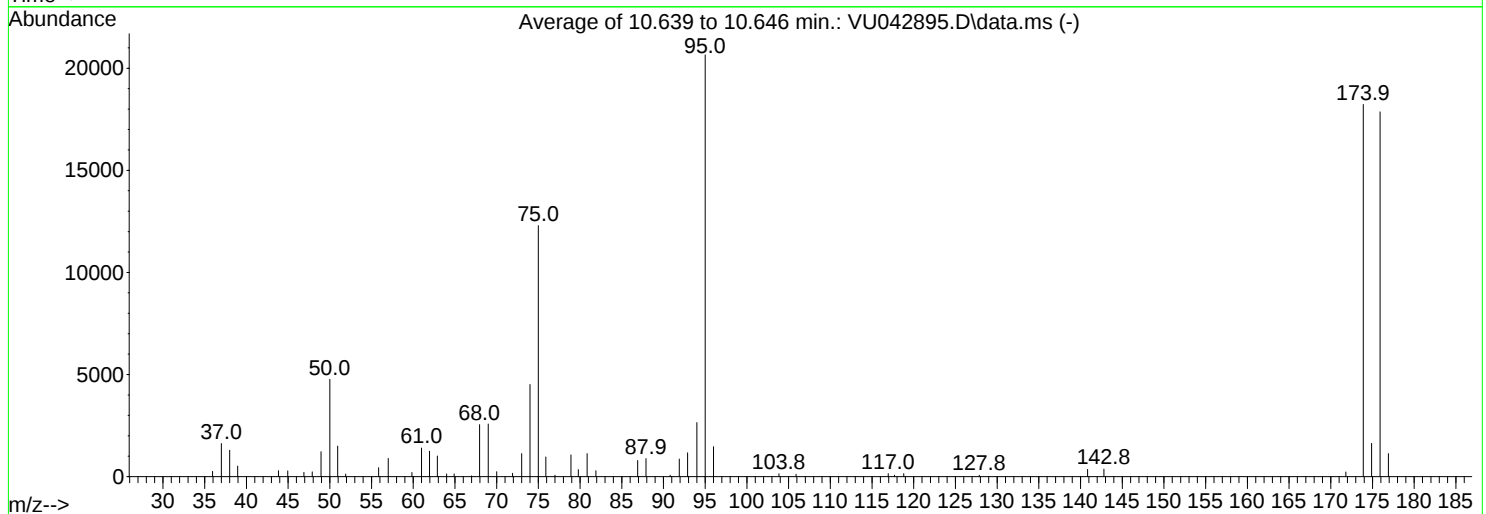


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040221\
Data File : VU042895.D
Acq On : 02 Apr 2021 14:05
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U032421W.M
Title : SW846 8260
Last Update : Thu Mar 25 05:42:00 2021

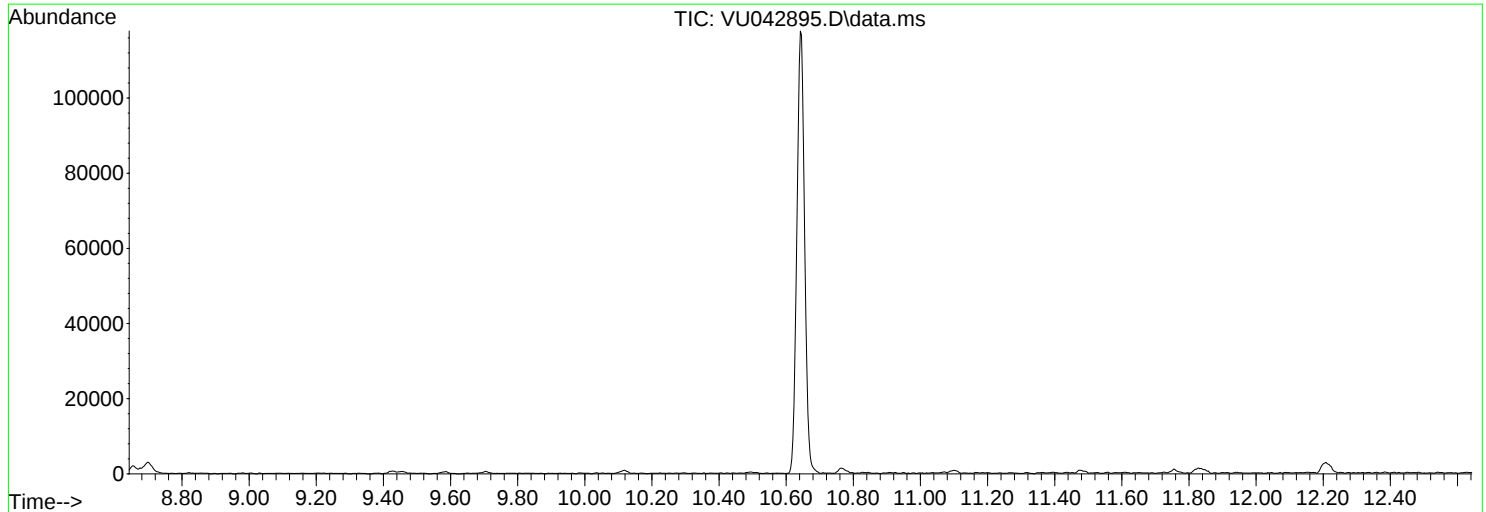

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2880

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.0	4761	PASS
75	95	30	60	59.5	12293	PASS
95	95	100	100	100.0	20656	PASS
96	95	5	9	7.1	1469	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	88.2	18224	PASS
175	174	5	9	8.9	1631	PASS
176	174	95	101	98.0	17867	PASS
177	176	5	9	6.3	1127	PASS