

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040222\
 Data File : VU047791.D
 Acq On : 02 Apr 2022 11:30
 Operator : SY/MD
 Sample : VU0402WBL03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0402WBL03

Quant Time: Apr 04 09:04:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U033122W.M
 Quant Title : SW846 8260
 QLast Update : Mon Apr 04 09:00:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.375	168	300167	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.253	114	449926	50.000	ug/l	0.00
63) Chlorobenzene-d5	9.420	117	433673	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.815	152	230523	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.703	65	181036	56.218	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 112.440%	
35) Dibromofluoromethane	5.292	113	161692	53.587	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 107.180%	
50) Toluene-d8	7.899	98	548690	50.475	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 100.940%	
62) 4-Bromofluorobenzene	10.635	95	194536	45.951	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 91.900%	
Target Compounds						
					Qvalue	
3) Chloromethane	1.520	50	771	0.206	ug/l	91
10) Methyl Iodide	2.726	142	46	1.969	ug/l #	43
11) Tert butyl alcohol	3.192	59	237	0.263	ug/l #	37
13) Acrolein	2.497	56	69	2.984	ug/l #	49
15) Acrylonitrile	3.337	53	462	0.213	ug/l #	61
16) Acetone	2.633	43	2125	0.905	ug/l	96
25) 2-Butanone	4.729	43	960	0.325	ug/l #	45
29) Tetrahydrofuran	5.060	42	879	0.480	ug/l #	88
31) Cyclohexane	5.375	56	5264	1.096	ug/l #	1
36) 1,1-Dichloropropene	5.375	75	20421	4.794	ug/l #	47
38) Carbon Tetrachloride	5.375	117	26391	5.809	ug/l #	16
49) 1,4-Dioxane	6.970	88	984	9.773	ug/l #	45
51) 4-Methyl-2-Pentanone	7.796	43	5487	1.041	ug/l	99
59) 2-Hexanone	8.687	43	8466	1.959	ug/l	88
74) N-amyl acetate	10.324	43	2506	0.470	ug/l	95
76) 1,2,3-Trichloropropane	10.635	75	94202	14.598	ug/l #	45
81) trans-1,4-Dichloro-2-b...	10.635	75	94202	51.959	ug/l #	15
84) 1,2,4-Trimethylbenzene	11.471	105	2268	0.201	ug/l	92
85) sec-Butylbenzene	11.645	105	3080	0.216	ug/l	98
86) p-Isopropyltoluene	11.796	119	2810	0.230	ug/l #	76
87) 1,3-Dichlorobenzene	11.748	146	2027	0.263	ug/l	88
88) 1,4-Dichlorobenzene	11.748	146	2027	0.257	ug/l	87
89) n-Butylbenzene	12.211	91	6490	0.568	ug/l	93
91) 1,2-Dichlorobenzene	12.217	146	2288	0.305	ug/l	88
92) 1,2-Dibromo-3-Chloropr...	13.002	75	721	0.514	ug/l	77
93) 1,2,4-Trichlorobenzene	13.844	180	5591	1.052	ug/l	97
94) Hexachlorobutadiene	14.021	225	1436	0.536	ug/l	90
95) Naphthalene	14.089	128	42449	2.680	ug/l	99
96) 1,2,3-Trichlorobenzene	14.333	180	6986	1.348	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040222\
Data File : VU047791.D
Acq On : 02 Apr 2022 11:30
Operator : SY/MD
Sample : VU0402WBL03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0402WBL03

Quant Time: Apr 04 09:04:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U033122W.M
Quant Title : SW846 8260
QLast Update : Mon Apr 04 09:00:10 2022
Response via : Initial Calibration




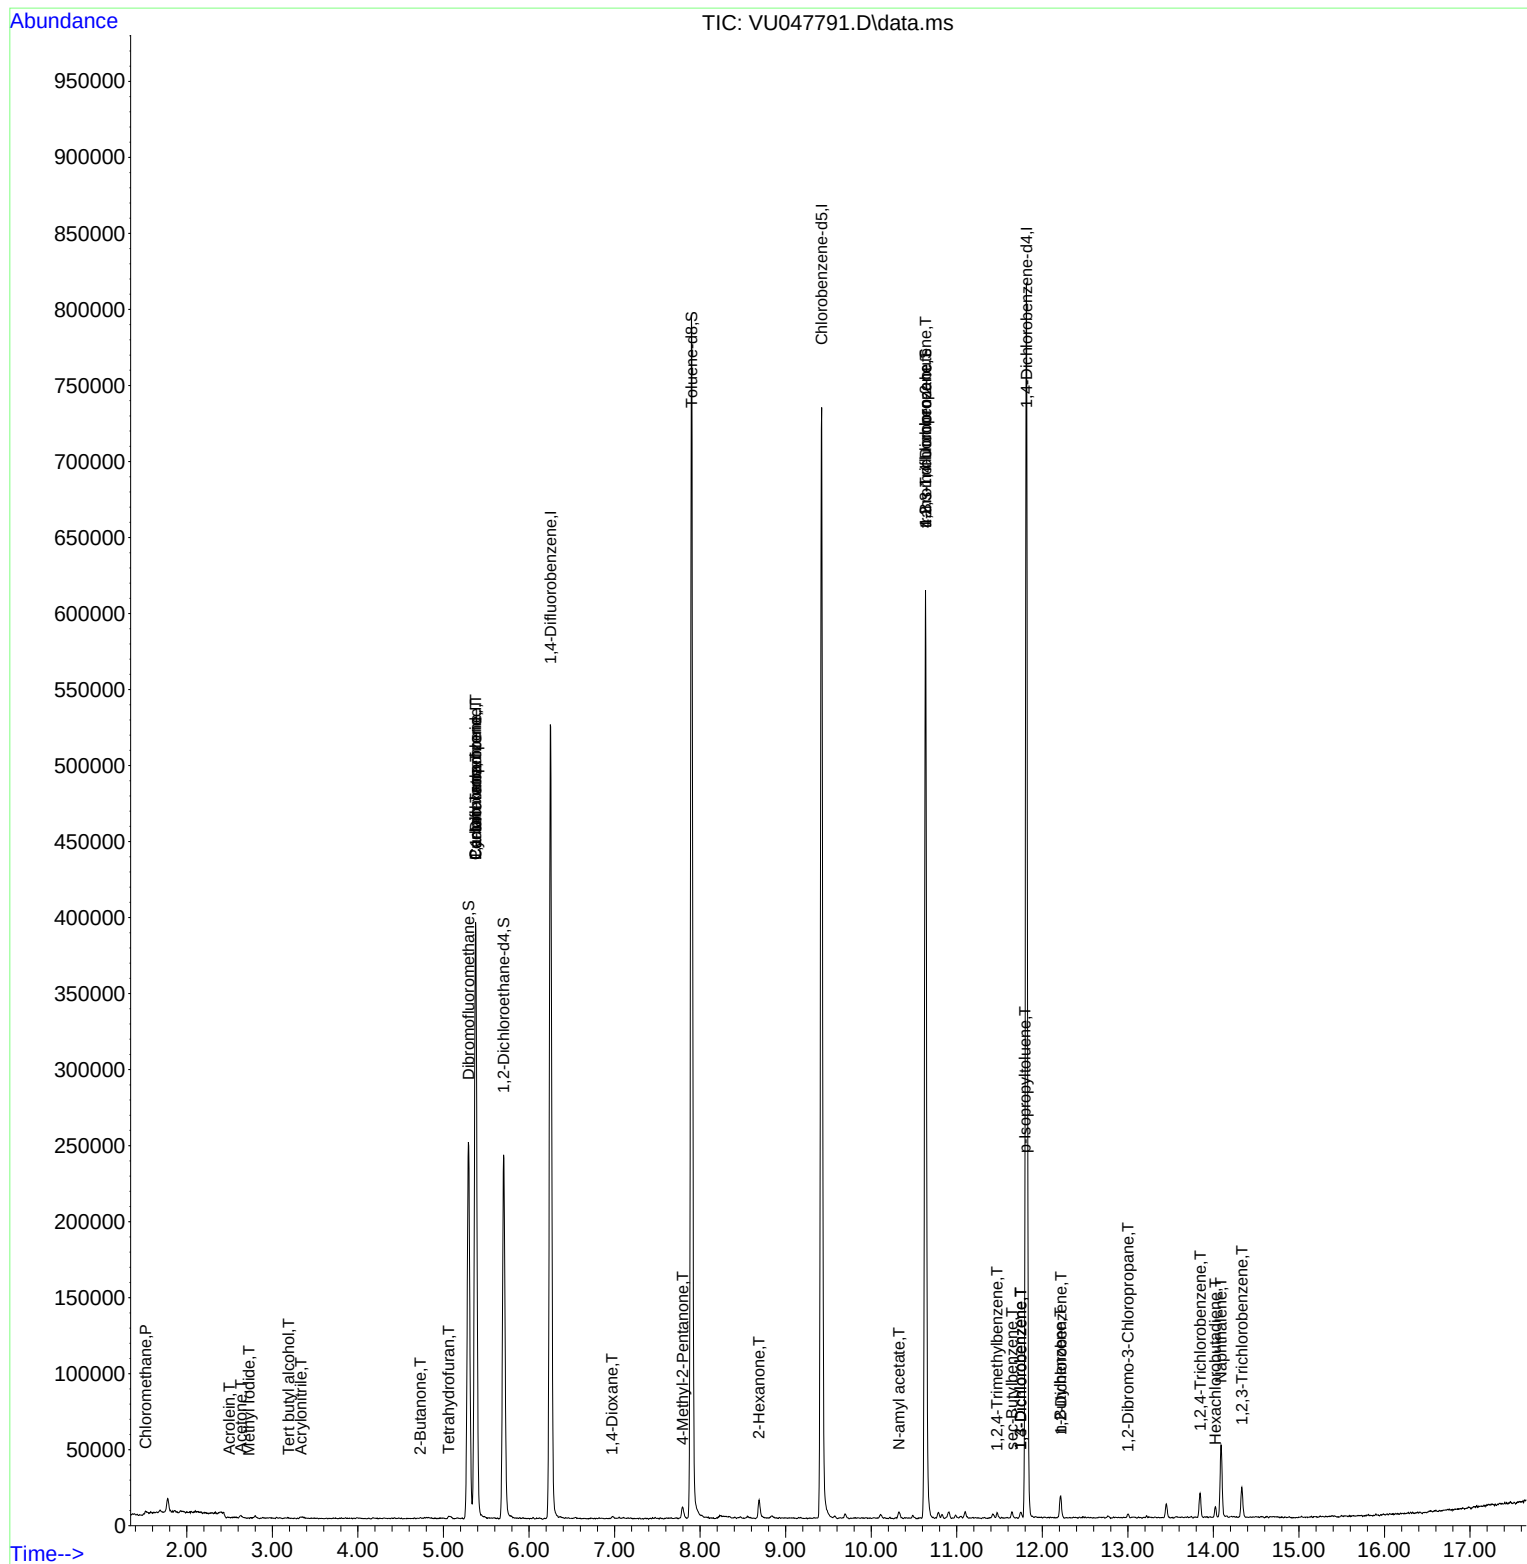




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.375 min Scan# 11
Delta R.T. 0.000 min
Lab File: VU047791.D
Acq: 02 Apr 2022 11:30




Instrument :
MSVOA_U
ClientSampleId :
VU0402WBL03


Tgt Ion:168 Resp: 300167
Ion Ratio Lower Upper
168 100
99 50.2 39.3 58.9

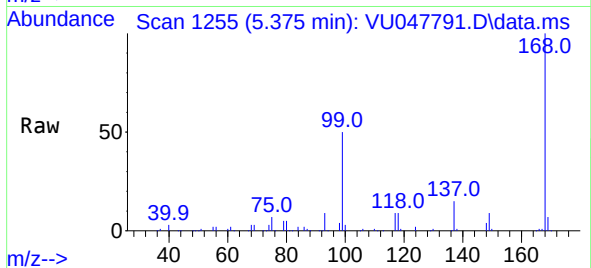

#3
Chloromethane
Concen: 0.206 ug/l
RT: 1.520 min Scan# 56
Delta R.T. -0.003 min
Lab File: VU047791.D
Acq: 02 Apr 2022 11:30


Tgt Ion: 50 Resp: 771
Ion Ratio Lower Upper
50 100
52 39.3 27.4 41.2

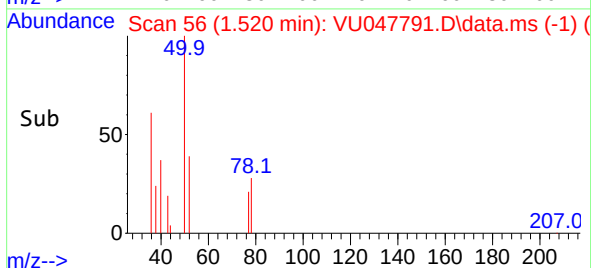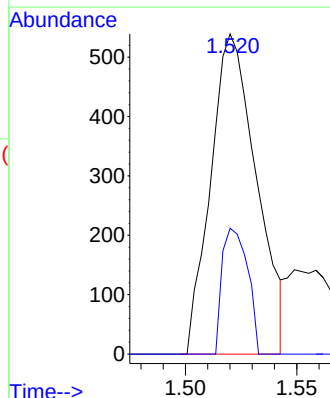






#10
Methyl Iodide
Concen: 1.969 ug/l
RT: 2.726 min Scan# 41
Delta R.T. -0.000 min
Lab File: VU047791.D
Acq: 02 Apr 2022 11:30

Instrument :
MSVOA_U
ClientSampleId :
VU0402WBL03



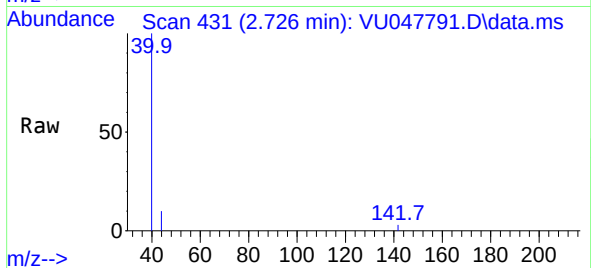



Tgt Ion:142 Resp: 46
Ion Ratio Lower Upper
142 100
127 0.0 32.5 48.7#
141 0.0 11.4 17.0#

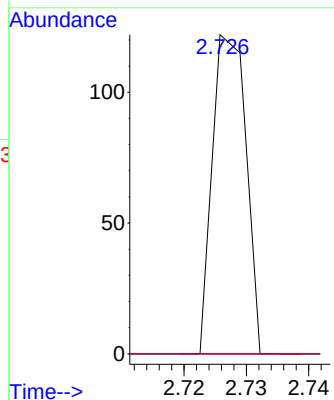

#11
Tert butyl alcohol
Concen: 0.263 ug/l
RT: 3.192 min Scan# 576
Delta R.T. -0.103 min
Lab File: VU047791.D
Acq: 02 Apr 2022 11:30


Tgt Ion: 59 Resp: 237
Ion Ratio Lower Upper
59 100
57 0.0 30.6 45.8#

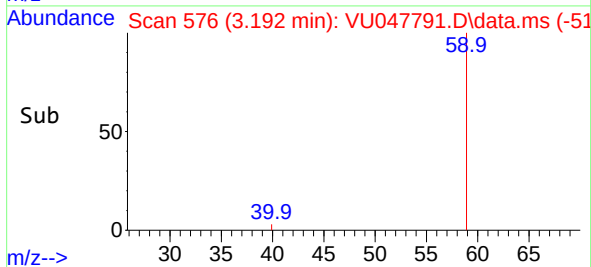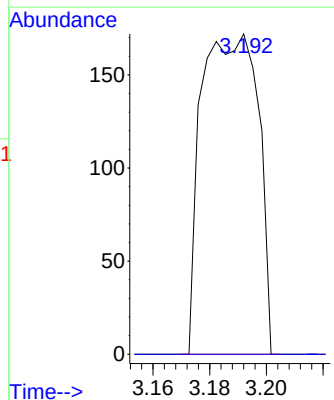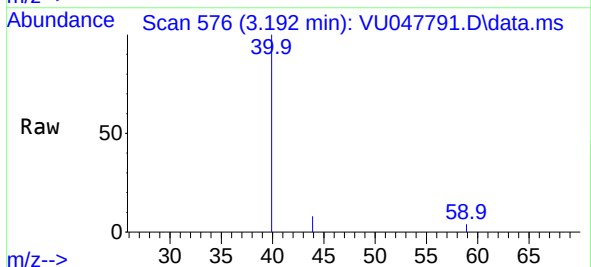






#13
Acrolein
Concen: 2.984 ug/l
RT: 2.497 min Scan# 30
Delta R.T. -0.001 min
Lab File: VU047791.D
Acq: 02 Apr 2022 11:30

Instrument :
MSVOA_U
ClientSampleId :
VU0402WBL03



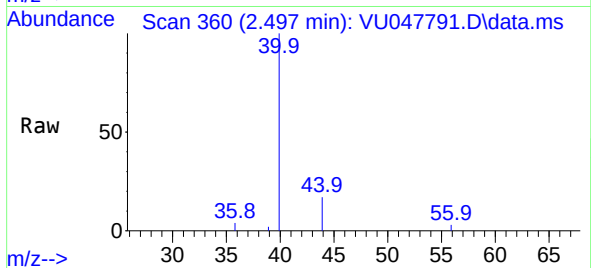



Tgt Ion: 56 Resp: 69
Ion Ratio Lower Upper
56 100
55 29.0 56.6 85.0#

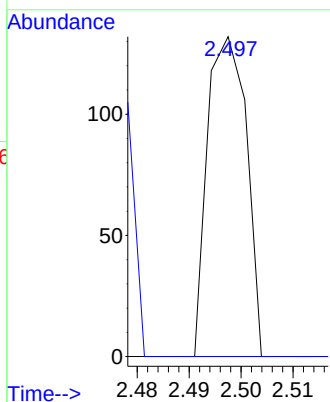

#15
Acrylonitrile
Concen: 0.213 ug/l
RT: 3.337 min Scan# 621
Delta R.T. 0.009 min
Lab File: VU047791.D
Acq: 02 Apr 2022 11:30

Tgt Ion: 53 Resp: 462
Ion Ratio Lower Upper
53 100
52 128.1 65.7 98.5#
51 40.3 28.2 42.4


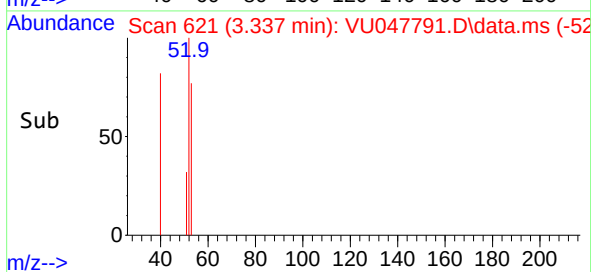






#16
Acetone
Concen: 0.905 ug/l
RT: 2.633 min Scan# 40
Delta R.T. -0.019 min
Lab File: VU047791.D
Acq: 02 Apr 2022 11:30




Instrument :
MSVOA_U
ClientSampleId :
VU0402WBL03


Tgt Ion: 43 Resp: 2125
Ion Ratio Lower Upper
43 100
58 32.3 27.5 41.3

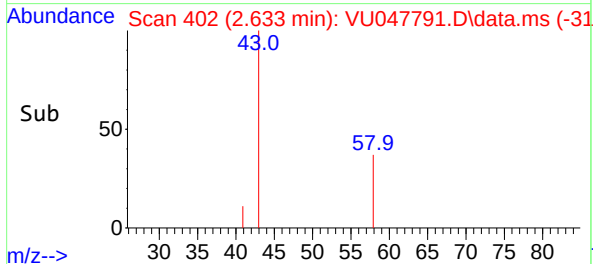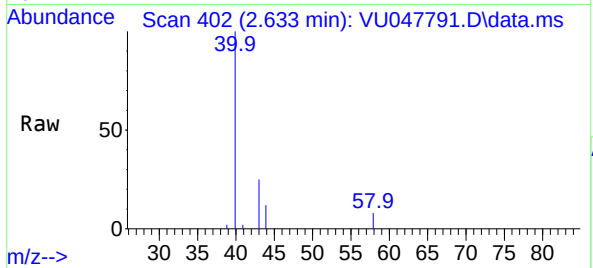

#25
2-Butanone
Concen: 0.325 ug/l
RT: 4.729 min Scan# 1054
Delta R.T. 0.013 min
Lab File: VU047791.D
Acq: 02 Apr 2022 11:30

Tgt Ion: 43 Resp: 960
Ion Ratio Lower Upper
43 100
72 0.0 23.8 35.6#


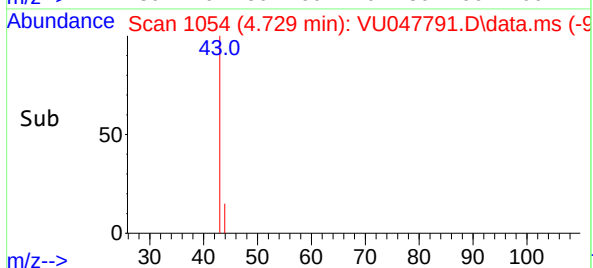
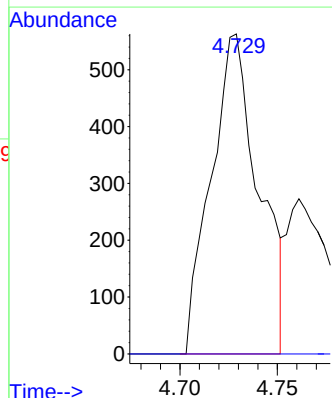
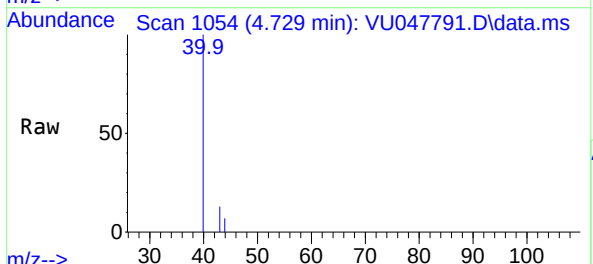




#29
Tetrahydrofuran
Concen: 0.480 ug/l
RT: 5.060 min Scan# 1158
Delta R.T. -0.003 min
Lab File: VU047791.D
Acq: 02 Apr 2022 11:30




Instrument :
MSVOA_U
ClientSampleId :
VU0402WBL03


Tgt Ion:	42	Resp:	879
Ion	Ratio	Lower	Upper
42	100		
72	52.4	42.6	63.8
71	34.1	40.3	60.5#

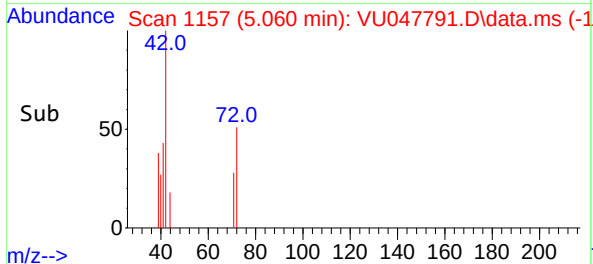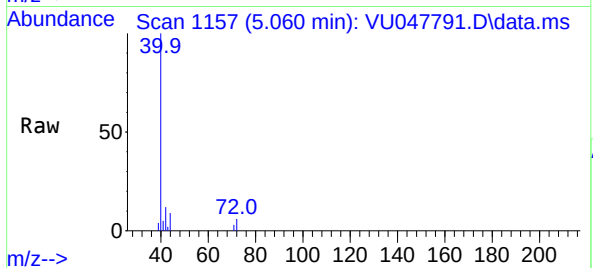

#31
Cyclohexane
Concen: 1.096 ug/l
RT: 5.375 min Scan# 1255
Delta R.T. -0.016 min
Lab File: VU047791.D
Acq: 02 Apr 2022 11:30

Tgt Ion:	56	Resp:	5264
Ion	Ratio	Lower	Upper
56	100		
69	188.7	27.8	41.8#
84	147.1	74.2	111.4#


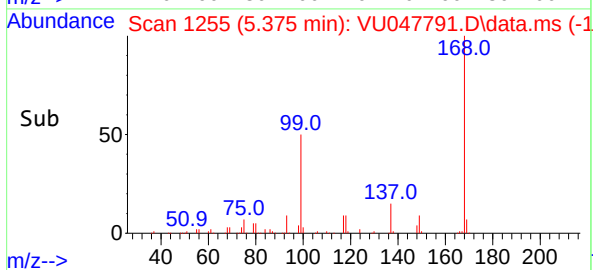

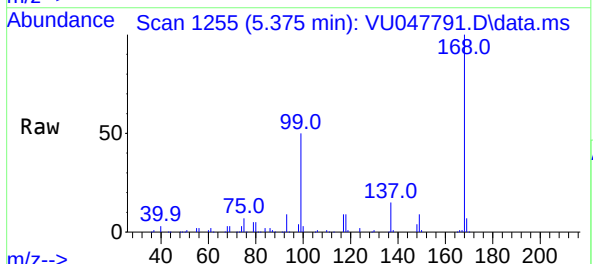




#33
1,2-Dichloroethane-d4
Concen: 56.218 ug/l
RT: 5.703 min Scan# 11
Delta R.T. -0.003 min
Lab File: VU047791.D
Acq: 02 Apr 2022 11:30




Instrument :
MSVOA_U
ClientSampleId :
VU0402WBL03


Tgt Ion: 65 Resp: 181036
Ion Ratio Lower Upper
65 100
67 53.1 0.0 108.0

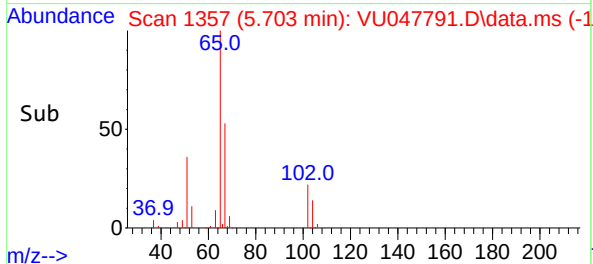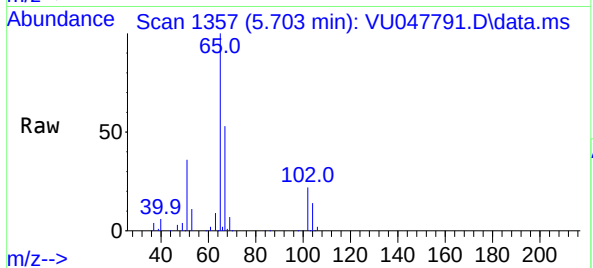

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.253 min Scan# 1528
Delta R.T. -0.000 min
Lab File: VU047791.D
Acq: 02 Apr 2022 11:30

Tgt Ion:114 Resp: 449926
Ion Ratio Lower Upper
114 100
63 19.1 0.0 37.8
88 15.3 0.0 29.2


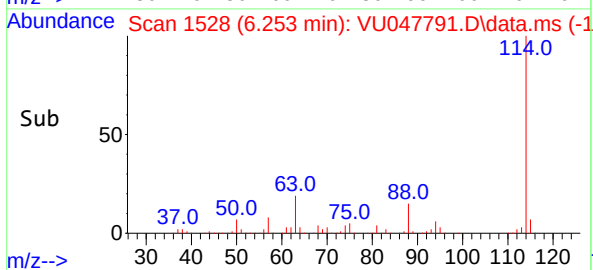

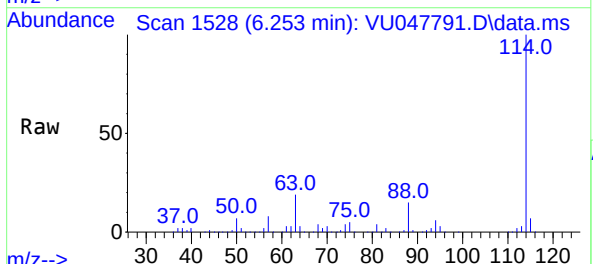


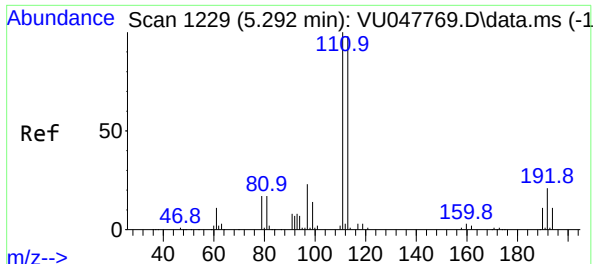

#35
Dibromofluoromethane
Concen: 53.587 ug/l
RT: 5.292 min Scan# 11
Delta R.T. -0.000 min
Lab File: VU047791.D
Acq: 02 Apr 2022 11:30




Instrument :
MSVOA_U
ClientSampleId :
VU0402WBL03


Tgt Ion:113 Resp: 161692
Ion Ratio Lower Upper
113 100
111 100.9 82.1 123.1
192 22.5 18.0 27.0

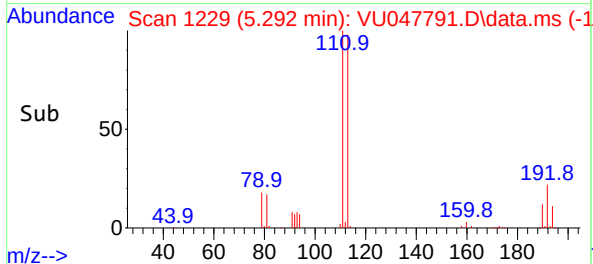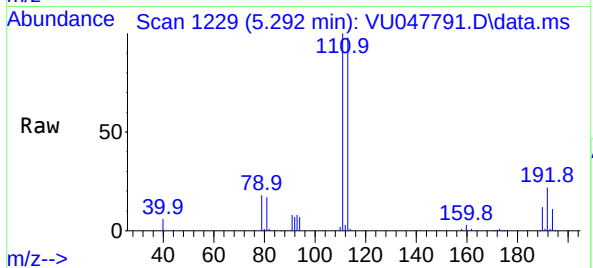

#36
1,1-Dichloropropene
Concen: 4.794 ug/l
RT: 5.375 min Scan# 1255
Delta R.T. -0.155 min
Lab File: VU047791.D
Acq: 02 Apr 2022 11:30


Tgt Ion: 75 Resp: 20421
Ion Ratio Lower Upper
75 100
110 7.2 18.4 55.2#
77 0.0 25.1 37.7#

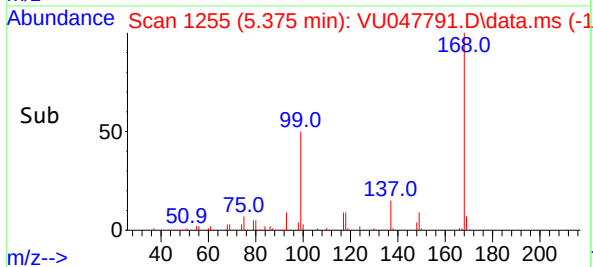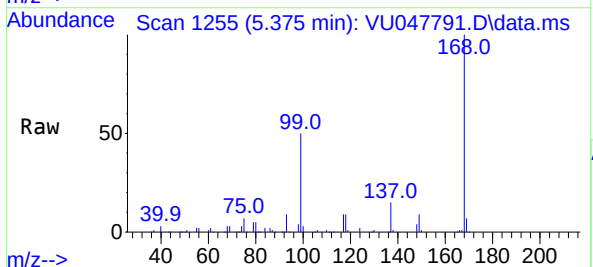






#38
Carbon Tetrachloride
Concen: 5.809 ug/l
RT: 5.375 min Scan# 11
Delta R.T. -0.155 min
Lab File: VU047791.D
Acq: 02 Apr 2022 11:30

Instrument :
MSVOA_U
ClientSampleId :
VU0402WBL03



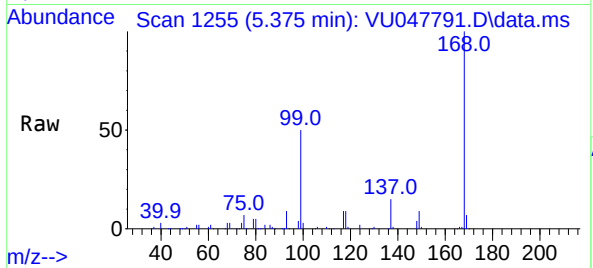



Tgt Ion:117 Resp: 26391
Ion Ratio Lower Upper
117 100
119 5.8 76.8 115.2#
121 0.0 24.7 37.1#

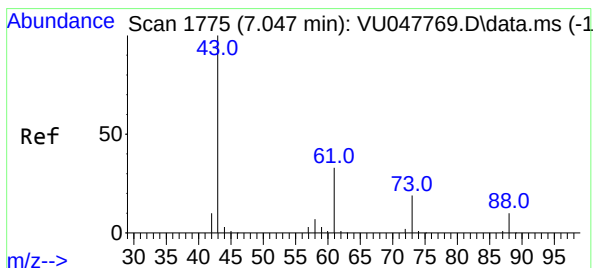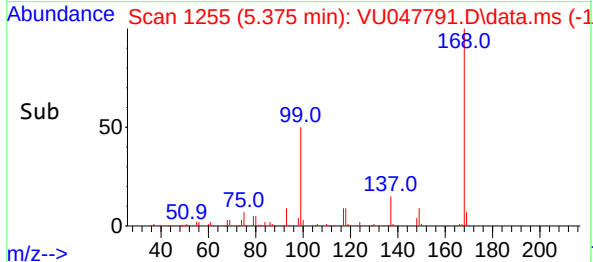

#49
1,4-Dioxane
Concen: 9.773 ug/l
RT: 6.970 min Scan# 1751
Delta R.T. -0.077 min
Lab File: VU047791.D
Acq: 02 Apr 2022 11:30

Tgt Ion: 88 Resp: 984
Ion Ratio Lower Upper
88 100
43 9.0 0.0 0.0#
58 44.0 15.4 23.0#


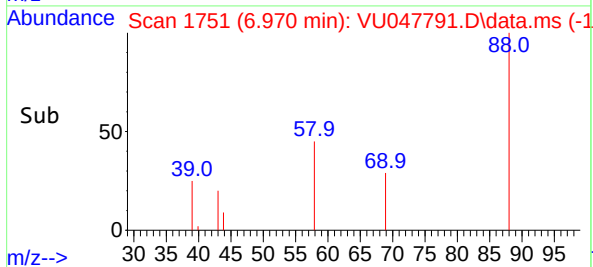

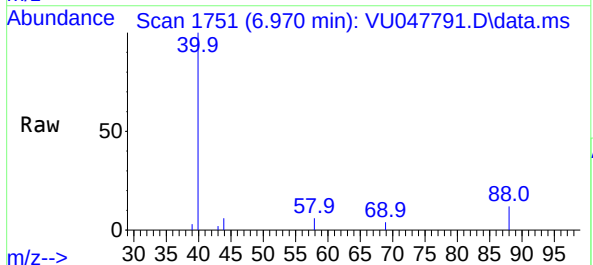




#50
Toluene-d8
Concen: 50.475 ug/l
RT: 7.899 min Scan# 2040
Delta R.T. -0.000 min
Lab File: VU047791.D
Acq: 02 Apr 2022 11:30




Instrument :
MSVOA_U
ClientSampleId :
VU0402WBL03


Tgt Ion: 98 Resp: 548690
Ion Ratio Lower Upper
98 100
100 63.9 51.7 77.5

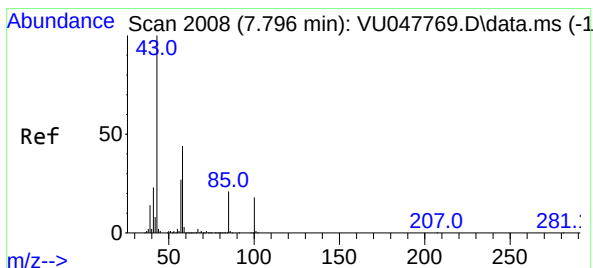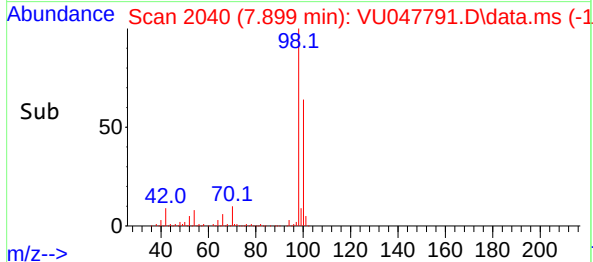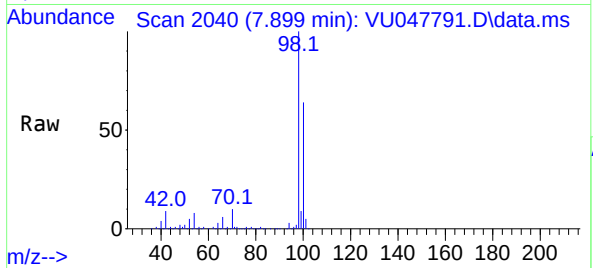

#51
4-Methyl-2-Pentanone
Concen: 1.041 ug/l
RT: 7.796 min Scan# 2008
Delta R.T. -0.000 min
Lab File: VU047791.D
Acq: 02 Apr 2022 11:30

Tgt Ion: 43 Resp: 5487
Ion Ratio Lower Upper
43 100
58 42.9 34.7 52.1

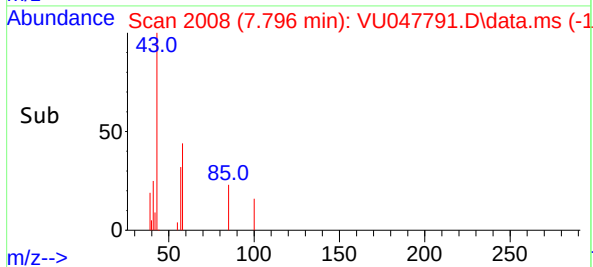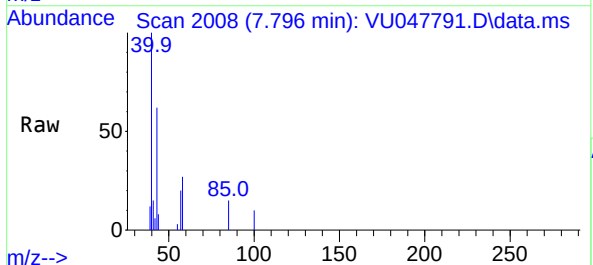



#59

2-Hexanone

Concen: 1.959 ug/l

RT: 8.687 min Scan# 21

Delta R.T. -0.000 min

Lab File: VU047791.D

Acq: 02 Apr 2022 11:30

Instrument :

MSVOA_U

ClientSampleId :





VU0402WBL03

Tgt Ion: 43 Resp: 8466

Ion Ratio Lower Upper

43 100

58 51.7 30.3 90.8

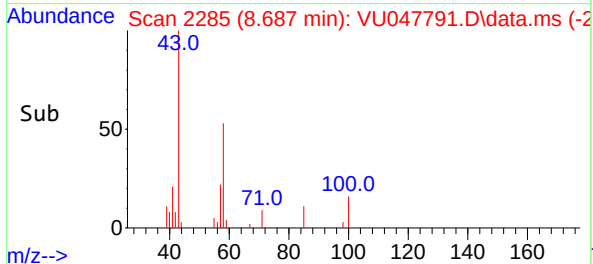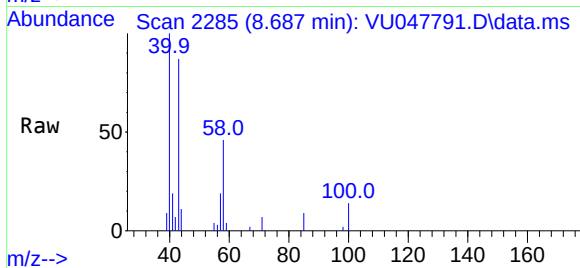

#62

4-Bromofluorobenzene

Concen: 45.951 ug/l

RT: 10.635 min Scan# 2891

Delta R.T. 0.003 min

Lab File: VU047791.D

Acq: 02 Apr 2022 11:30




Tgt Ion: 95 Resp: 194536


Ion Ratio Lower Upper

95 100

174 94.1 0.0 182.0

176 91.3 0.0 177.8


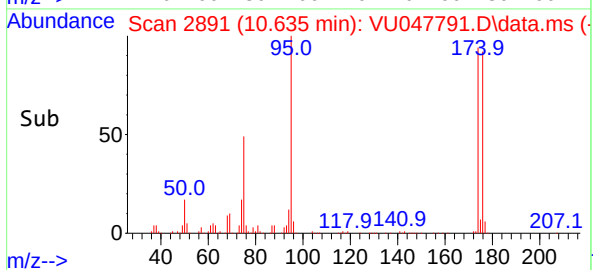

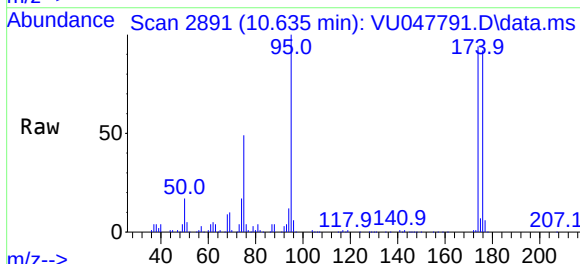




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.420 min Scan# 2513
Delta R.T. -0.000 min
Lab File: VU047791.D
Acq: 02 Apr 2022 11:30




Instrument :
MSVOA_U
ClientSampleId :
VU0402WBL03


Tgt Ion:117 Resp: 433673
Ion Ratio Lower Upper
117 100
82 51.9 41.7 62.5
119 32.2 25.7 38.5



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.815 min Scan# 3258
Delta R.T. 0.003 min
Lab File: VU047791.D
Acq: 02 Apr 2022 11:30

Tgt Ion:152 Resp: 230523
Ion Ratio Lower Upper
152 100
115 55.0 37.0 110.9
150 155.8 0.0 342.2


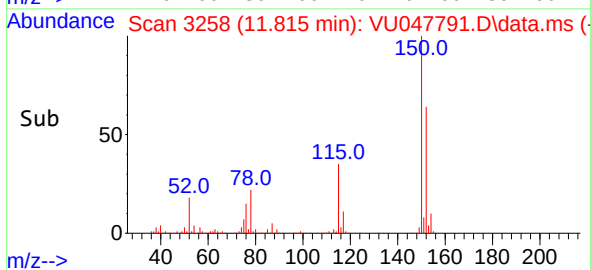






#74
N-amy1 acetate
Concen: 0.470 ug/l
RT: 10.324 min Scan# 2793
Delta R.T. 0.003 min
Lab File: VU047791.D
Acq: 02 Apr 2022 11:30




Instrument :
MSVOA_U
ClientSampleId :
VU0402WBL03


Tgt Ion: 43	Resp: 2506
Ion Ratio	Lower Upper
43	100
70	46.6 38.7 58.1
55	25.5 21.8 32.8
61	22.3 21.9 32.9

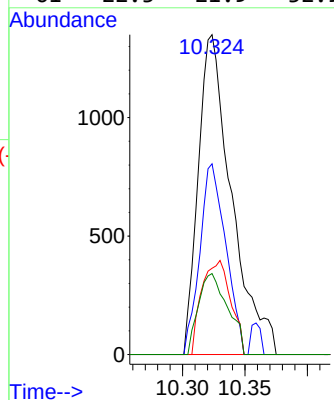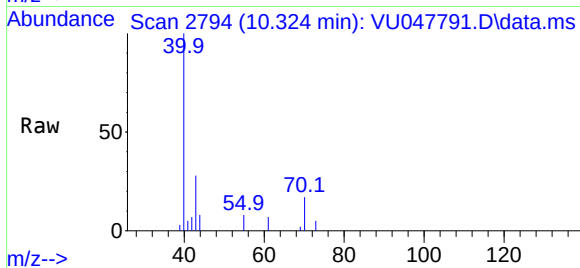

#76
1,2,3-Trichloropropane
Concen: 14.598 ug/l
RT: 10.635 min Scan# 2891
Delta R.T. -0.190 min
Lab File: VU047791.D
Acq: 02 Apr 2022 11:30

Tgt Ion: 75	Resp: 94202
Ion Ratio	Lower Upper
75	100
77	1.2 15.8 47.3#


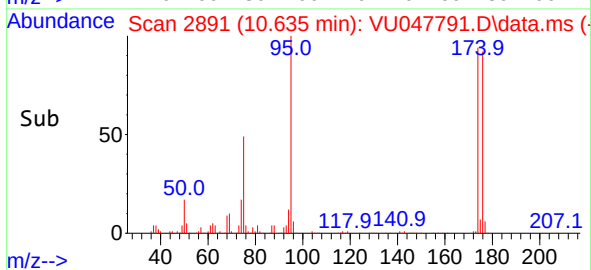
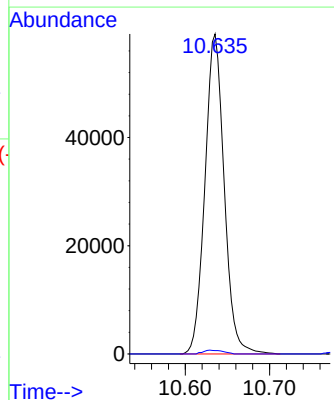





#81
trans-1,4-Dichloro-2-butene
Concen: 51.959 ug/l
RT: 10.635 min Scan# 2864
Delta R.T. 0.087 min
Lab File: VU047791.D
Acq: 02 Apr 2022 11:30




Instrument :
MSVOA_U
ClientSampleId :
VU0402WBL03


Tgt Ion: 75 Resp: 94202
Ion Ratio Lower Upper
75 100
53 0.0 69.2 103.8#
89 0.0 37.0 55.6#

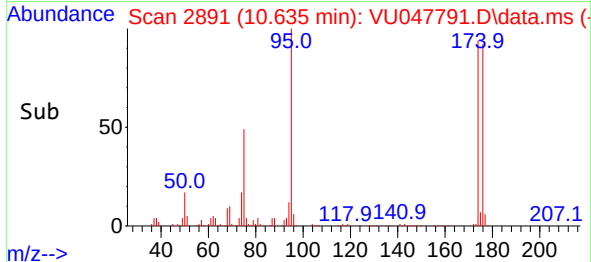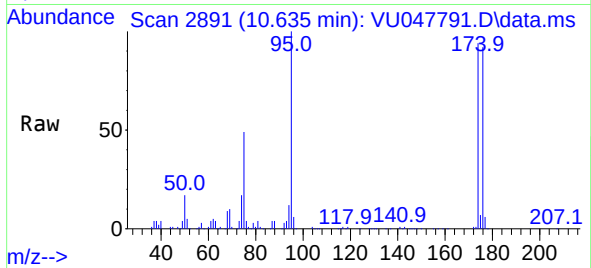

#84
1,2,4-Trimethylbenzene
Concen: 0.201 ug/l
RT: 11.471 min Scan# 3151
Delta R.T. 0.003 min
Lab File: VU047791.D
Acq: 02 Apr 2022 11:30

Tgt Ion: 105 Resp: 2268
Ion Ratio Lower Upper
105 100
120 41.3 23.4 70.3


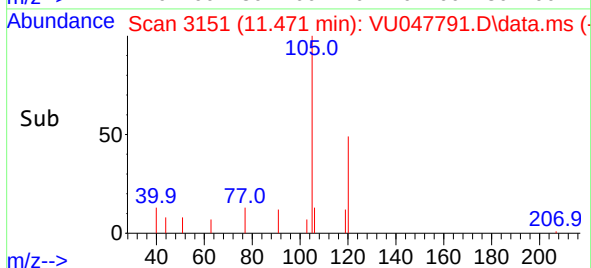
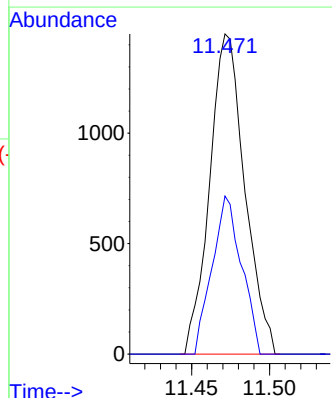





#85
 sec-Butylbenzene
 Concen: 0.216 ug/l
 RT: 11.645 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: VU047791.D
 Acq: 02 Apr 2022 11:30




Instrument :
 MSVOA_U
 ClientSampleId :
 VU0402WBL03


Tgt Ion:105 Resp: 3080
 Ion Ratio Lower Upper
 105 100
 134 19.7 10.4 31.1

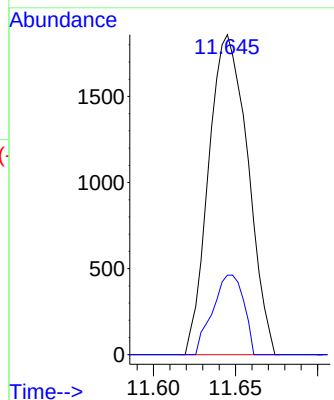

#86
 p-Isopropyltoluene
 Concen: 0.230 ug/l
 RT: 11.796 min Scan# 3252
 Delta R.T. 0.003 min
 Lab File: VU047791.D
 Acq: 02 Apr 2022 11:30

Tgt Ion:119 Resp: 2810
 Ion Ratio Lower Upper
 119 100
 134 30.8 13.5 40.4
 91 42.8 11.2 33.5#

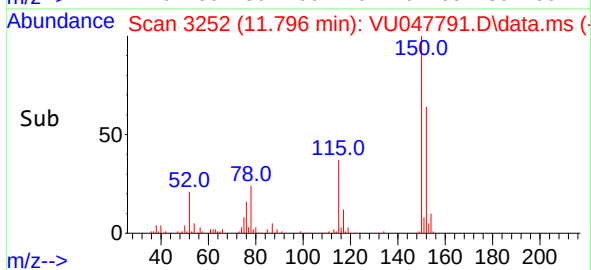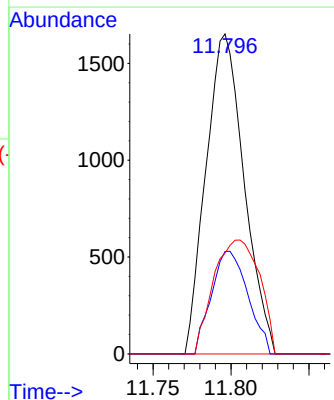

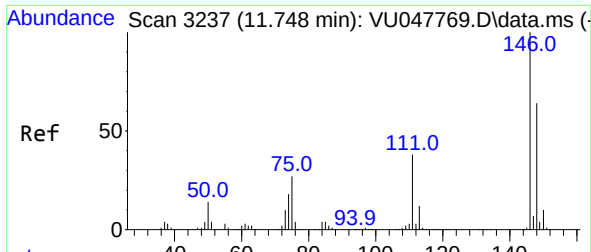

#87

1,3-Dichlorobenzene

Concen: 0.263 ug/l

RT: 11.748 min Scan# 3237

Delta R.T. -0.000 min

Lab File: VU047791.D

Acq: 02 Apr 2022 11:30

Instrument :

MSVOA_U

ClientSampleId :

VU0402WBL03





Tgt Ion:146 Resp: 2027

Ion Ratio Lower Upper

146 100

111 39.8 18.9 56.5

148 77.5 31.9 95.9

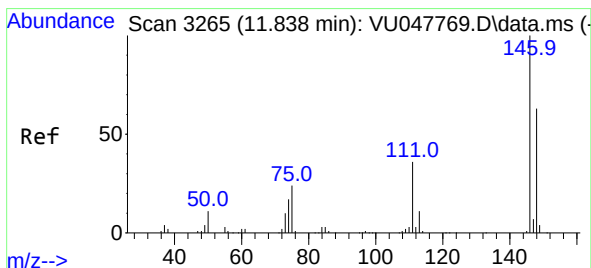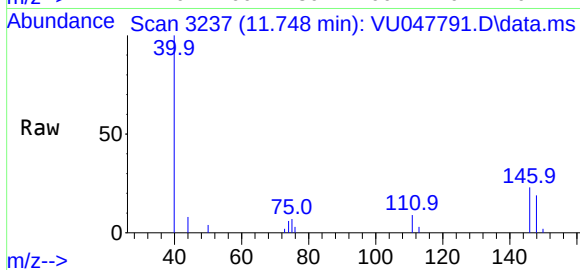

#88

1,4-Dichlorobenzene

Concen: 0.257 ug/l

RT: 11.748 min Scan# 3237

Delta R.T. -0.090 min

Lab File: VU047791.D

Acq: 02 Apr 2022 11:30




Tgt Ion:146 Resp: 2027


Ion Ratio Lower Upper

146 100

111 39.8 18.5 55.5

148 77.5 31.9 95.7


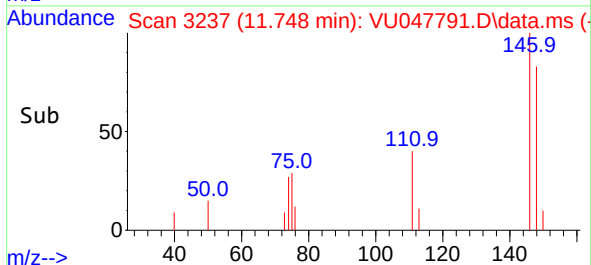
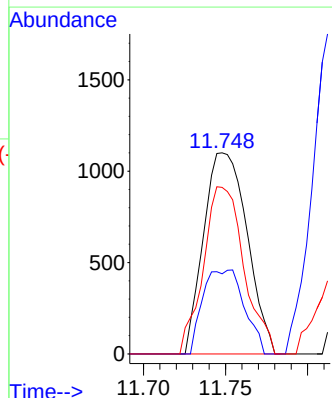
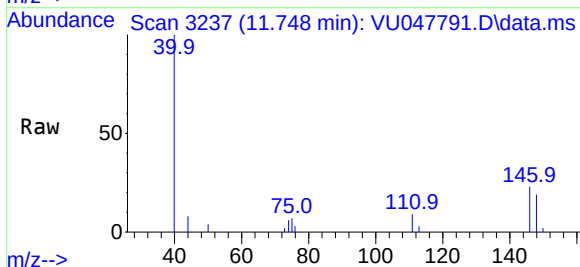




#89
n-Butylbenzene
Concen: 0.568 ug/l
RT: 12.211 min Scan# 3381
Delta R.T. 0.003 min
Lab File: VU047791.D
Acq: 02 Apr 2022 11:30




Instrument :
MSVOA_U
ClientSampleId :
VU0402WBL03


Tgt Ion: 91 Resp: 6490
Ion Ratio Lower Upper
91 100
92 46.4 26.2 78.6
134 25.0 13.5 40.4



#91
1,2-Dichlorobenzene
Concen: 0.305 ug/l
RT: 12.217 min Scan# 3383
Delta R.T. 0.003 min
Lab File: VU047791.D
Acq: 02 Apr 2022 11:30

Tgt Ion: 146 Resp: 2288
Ion Ratio Lower Upper
146 100
111 32.9 19.9 59.6
148 74.6 32.1 96.5


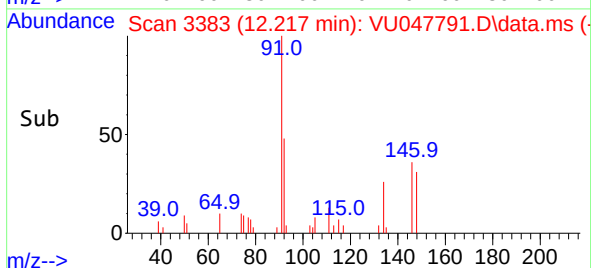
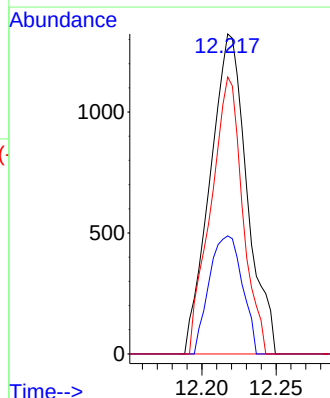





#92
 1,2-Dibromo-3-Chloropropane
 Concen: 0.514 ug/l
 RT: 13.002 min Scan# 3627
 Delta R.T. 0.006 min
 Lab File: VU047791.D
 Acq: 02 Apr 2022 11:30




Instrument :
 MSVOA_U
 ClientSampleId :
 VU0402WBL03


Tgt Ion: 75 Resp: 721
 Ion Ratio Lower Upper
 75 100
 155 74.3 47.8 143.4
 157 97.4 62.2 186.5



#93
 1,2,4-Trichlorobenzene
 Concen: 1.052 ug/l
 RT: 13.844 min Scan# 3889
 Delta R.T. 0.003 min
 Lab File: VU047791.D
 Acq: 02 Apr 2022 11:30

Tgt Ion: 180 Resp: 5591
 Ion Ratio Lower Upper
 180 100
 182 98.5 47.9 143.6
 145 30.4 14.0 41.9


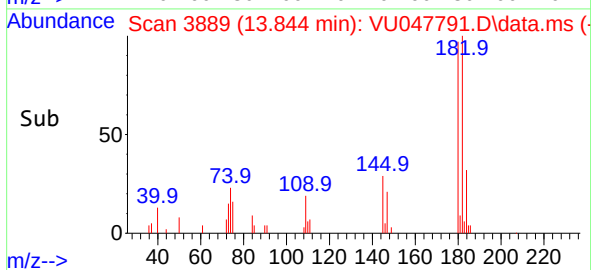






#94
Hexachlorobutadiene
Concen: 0.536 ug/l
RT: 14.021 min Scan# 3944
Delta R.T. -0.000 min
Lab File: VU047791.D
Acq: 02 Apr 2022 11:30




Instrument :
MSVOA_U
ClientSampleId :
VU0402WBL03


Tgt Ion:	225	Resp:	1436
Ion	Ratio	Lower	Upper
225	100		
223	55.1	31.3	93.9
227	72.1	32.0	96.2

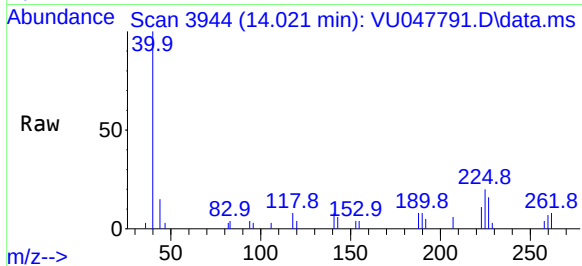

#95
Naphthalene
Concen: 2.680 ug/l
RT: 14.089 min Scan# 3965
Delta R.T. 0.003 min
Lab File: VU047791.D
Acq: 02 Apr 2022 11:30

Tgt Ion:	128	Resp:	42449
Ion	Ratio	Lower	Upper
128	100		
127	13.2	10.3	15.5
129	10.2	8.6	13.0

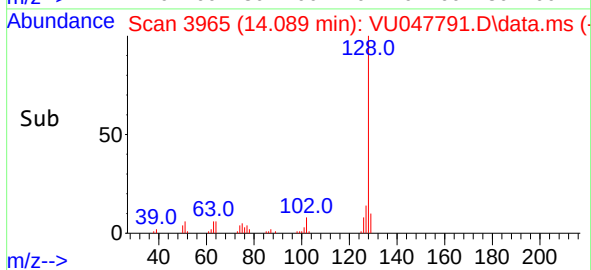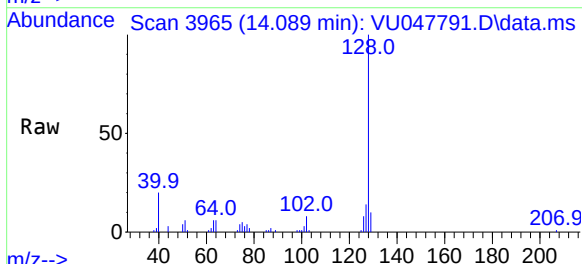



#96

1,2,3-Trichlorobenzene

Concen: 1.348 ug/l

RT: 14.333 min Scan# 4040

Delta R.T. 0.003 min

Lab File: VU047791.D


Acq: 02 Apr 2022 11:30

Instrument :

MSVOA_U

ClientSampleId :

VU0402WBL03

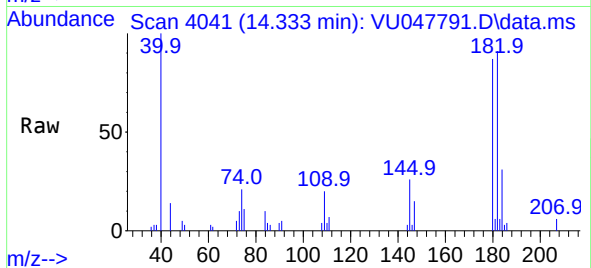

Tgt Ion:180 Resp: 6986

Ion Ratio Lower Upper

180 100

182 99.7 48.4 145.0

145 29.1 14.8 44.4

