


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040222\
 Data File : VU047789.D
 Acq On : 02 Apr 2022 10:28
 Operator : SY/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U033122W.M
 Title : SW846 8260
 Last Update : Thu Mar 31 13:50:29 2022

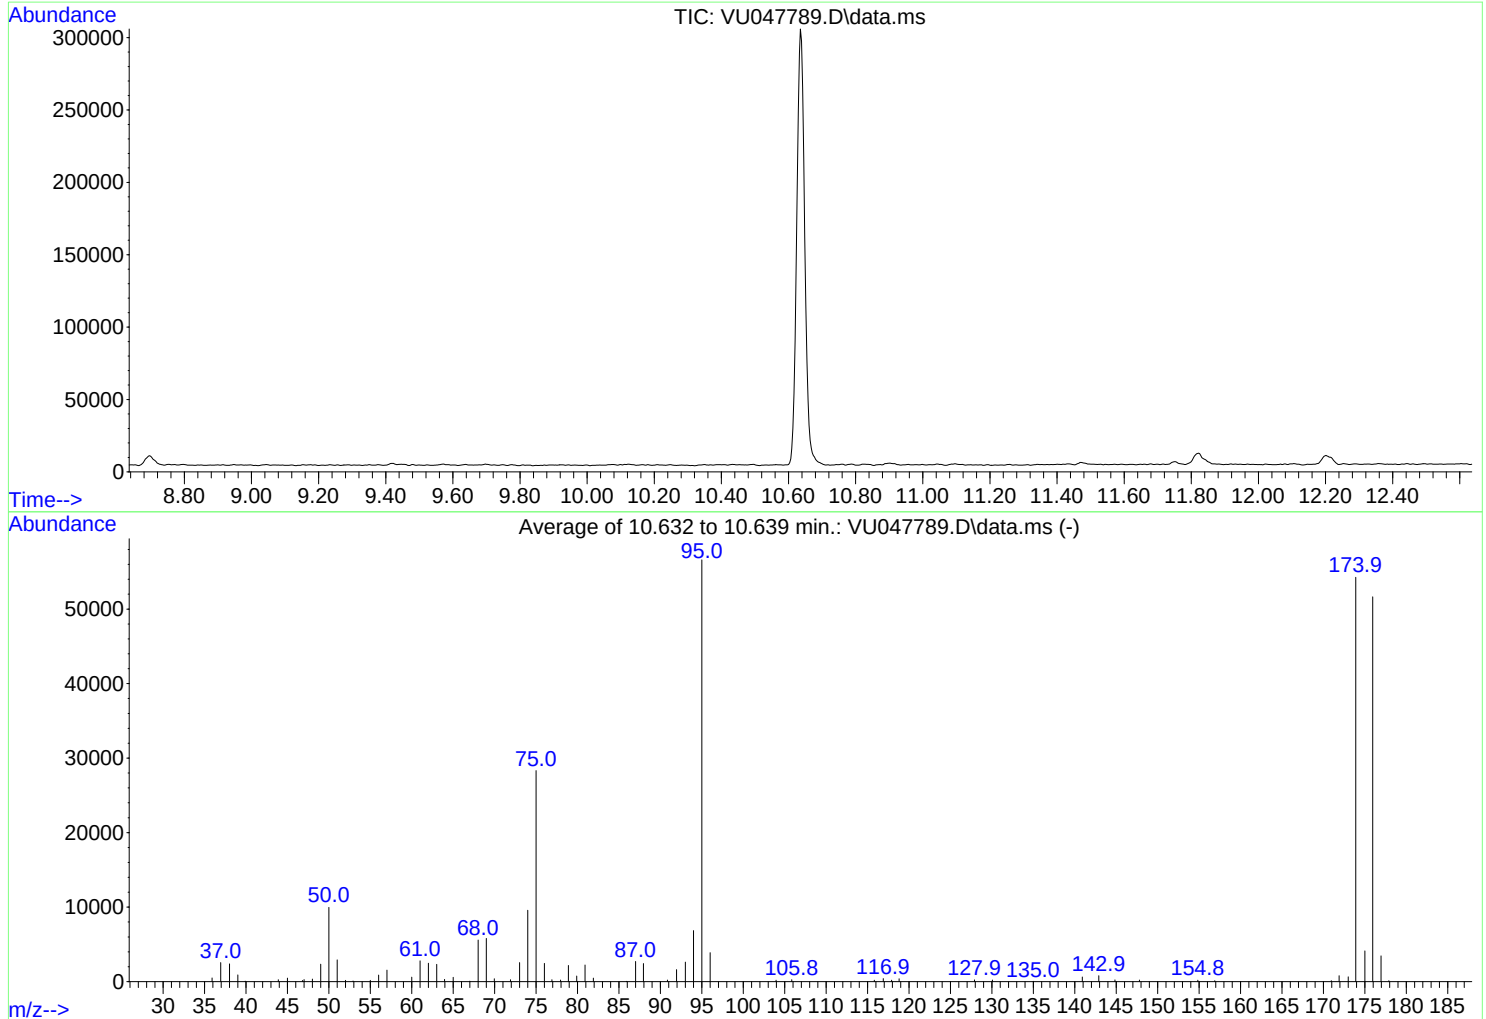

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	9969	PASS
75	95	30	60	50.0	28315	PASS
95	95	100	100	100.0	56608	PASS
96	95	5	9	6.9	3887	PASS
173	174	0.00	2	1.2	653	PASS
174	95	50	100	95.9	54267	PASS
175	174	5	9	7.6	4120	PASS
176	174	95	101	95.2	51651	PASS
177	176	5	9	6.7	3450	PASS