

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040320\
 Data File : VU037564.D
 Acq On : 03 Apr 2020 12:03
 Operator : JC/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	79	85	93	rVB	100706	102887	15.52%	2.081%
2	2.884	478	480	483	rVB	363	193	0.03%	0.004%
3	2.900	483	485	486	rBV	239	84	0.01%	0.002%
4	3.218	572	584	594	rBV3	2565	5471	0.83%	0.111%
5	3.385	630	636	637	rBV	1196	1238	0.19%	0.025%
6	3.472	662	663	664	rBV	304	82	0.01%	0.002%
7	3.504	669	673	676	rBV3	445	278	0.04%	0.006%
8	3.562	686	691	694	rBV	409	304	0.05%	0.006%
9	3.765	751	754	757	rBV	291	197	0.03%	0.004%
10	3.826	771	773	775	rBV2	372	204	0.03%	0.004%
11	3.900	795	796	798	rVB	349	94	0.01%	0.002%
12	3.938	805	808	810	rBV	275	125	0.02%	0.003%
13	3.990	821	824	826	rBV2	374	199	0.03%	0.004%
14	4.137	869	870	871	rBV2	107	24	0.00%	0.000%
15	4.292	916	918	920	rBV	276	95	0.01%	0.002%
16	4.321	925	927	929	rBV	191	106	0.02%	0.002%
17	4.379	941	945	947	rBV2	221	163	0.02%	0.003%
18	4.462	969	971	976	rVB	427	190	0.03%	0.004%
19	4.491	976	980	985	rBV	251	244	0.04%	0.005%
20	4.555	998	1000	1006	rBV	255	187	0.03%	0.004%
21	4.588	1007	1010	1013	rBV	240	125	0.02%	0.003%
22	4.932	1115	1117	1118	rBV	162	74	0.01%	0.001%
23	5.025	1145	1146	1148	rBV	234	70	0.01%	0.001%
24	5.044	1149	1152	1154	rBV	211	131	0.02%	0.003%
25	5.102	1154	1170	1191	rVV	119162	259146	39.09%	5.241%
26	5.202	1198	1201	1202	rBV	213	138	0.02%	0.003%
27	5.244	1211	1214	1217	rBV	260	171	0.03%	0.003%
28	5.285	1225	1227	1228	rBV	182	85	0.01%	0.002%
29	5.327	1236	1240	1242	rBV	428	428	0.06%	0.009%
30	5.427	1259	1271	1272	rBV6	1228	1951	0.29%	0.039%
31	5.465	1280	1283	1284	rBV6	150	67	0.01%	0.001%
32	5.527	1298	1302	1304	rBV	265	188	0.03%	0.004%
33	5.600	1322	1325	1330	rBV2	287	271	0.04%	0.005%
34	5.645	1336	1339	1342	rBV2	223	153	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040320\
 Data File : VU037564.D
 Acq On : 03 Apr 2020 12:03
 Operator : JC/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
 Title : VOC Analysis

35	5.761	1355	1375	1394	rBV2	252047	662983	100.00%	13.408%
36	5.877	1409	1411	1414	rBV2	207	148	0.02%	0.003%
37	5.919	1421	1424	1426	rBV	259	160	0.02%	0.003%
38	5.989	1443	1446	1450	rBV	224	172	0.03%	0.003%
39	6.044	1459	1463	1465	rBV2	242	222	0.03%	0.004%
40	6.089	1473	1477	1478	rBV	314	205	0.03%	0.004%
41	6.147	1491	1495	1498	rBV2	590	439	0.07%	0.009%
42	6.205	1510	1513	1519	rBV2	322	278	0.04%	0.006%
43	6.282	1524	1537	1551	rVB	226406	419416	63.26%	8.482%
44	6.465	1592	1594	1599	rVB2	281	192	0.03%	0.004%
45	6.494	1600	1603	1605	rBV	324	183	0.03%	0.004%
46	6.523	1610	1612	1614	rBV	236	120	0.02%	0.002%
47	6.536	1614	1616	1618	rBV	301	151	0.02%	0.003%
48	6.604	1635	1637	1640	rBV	205	87	0.01%	0.002%
49	6.620	1641	1642	1647	rVB	300	231	0.03%	0.005%
50	6.723	1660	1674	1690	rBV	158157	304497	45.93%	6.158%
51	6.887	1722	1725	1726	rVB	148	70	0.01%	0.001%
52	6.896	1726	1728	1730	rBV	336	181	0.03%	0.004%
53	7.105	1791	1793	1795	rBV	182	78	0.01%	0.002%
54	7.170	1809	1813	1818	rVB	249	204	0.03%	0.004%
55	7.202	1819	1823	1826	rVB2	320	273	0.04%	0.006%
56	7.491	1910	1913	1916	rBV	241	179	0.03%	0.004%
57	7.591	1933	1944	1960	rBV	101555	174265	26.28%	3.524%
58	7.732	1986	1988	1993	rBV	242	121	0.02%	0.002%
59	7.922	2034	2047	2063	rBV2	320149	547570	82.59%	11.074%
60	8.083	2095	2097	2098	rBV	143	53	0.01%	0.001%
61	8.118	2106	2108	2109	rBV	176	81	0.01%	0.002%
62	8.202	2123	2134	2150	rVB2	72592	122690	18.51%	2.481%
63	8.311	2163	2168	2170	rBV2	357	276	0.04%	0.006%
64	8.385	2188	2191	2195	rVB	221	136	0.02%	0.003%
65	8.655	2263	2275	2302	rBV	225182	398654	60.13%	8.062%
66	8.806	2320	2322	2324	rBV	297	144	0.02%	0.003%
67	9.160	2430	2432	2435	rBV	166	52	0.01%	0.001%
68	9.436	2505	2518	2536	rBV	322290	528287	79.68%	10.684%
69	9.645	2577	2583	2584	rBV	332	306	0.05%	0.006%
70	9.755	2616	2617	2619	rBV	150	52	0.01%	0.001%
71	9.829	2639	2640	2642	rVB	135	29	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040320\
 Data File : VU037564.D
 Acq On : 03 Apr 2020 12:03
 Operator : JC/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
 Title : VOC Analysis

72	9.973	2683	2685	2689	rVB	285	132	0.02%	0.003%
73	10.038	2704	2705	2709	rBV	224	143	0.02%	0.003%
74	10.076	2715	2717	2718	rBV	132	63	0.01%	0.001%
75	10.128	2723	2733	2741	rVV6	3801	6488	0.98%	0.131%
76	10.774	2921	2934	2948	rBV	212077	339335	51.18%	6.863%
77	10.919	2977	2979	2982	rBV	242	169	0.03%	0.003%
78	10.938	2982	2985	2988	rBV3	385	274	0.04%	0.006%
79	11.536	3169	3171	3175	rVB2	574	364	0.05%	0.007%
80	11.825	3249	3261	3277	rBV	331878	526714	79.45%	10.652%
81	12.205	3368	3379	3395	rVB	304340	496993	74.96%	10.051%
82	13.240	3693	3701	3709	rBV3	7713	10450	1.58%	0.211%
83	13.369	3739	3741	3746	rBV2	425	333	0.05%	0.007%
84	14.359	4040	4049	4062	rBV3	16219	24758	3.73%	0.501%


Sum of corrected areas: 4944764

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU040320\
Data File : VU037564.D
Acq On : 03 Apr 2020 12:03
Operator : JC/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

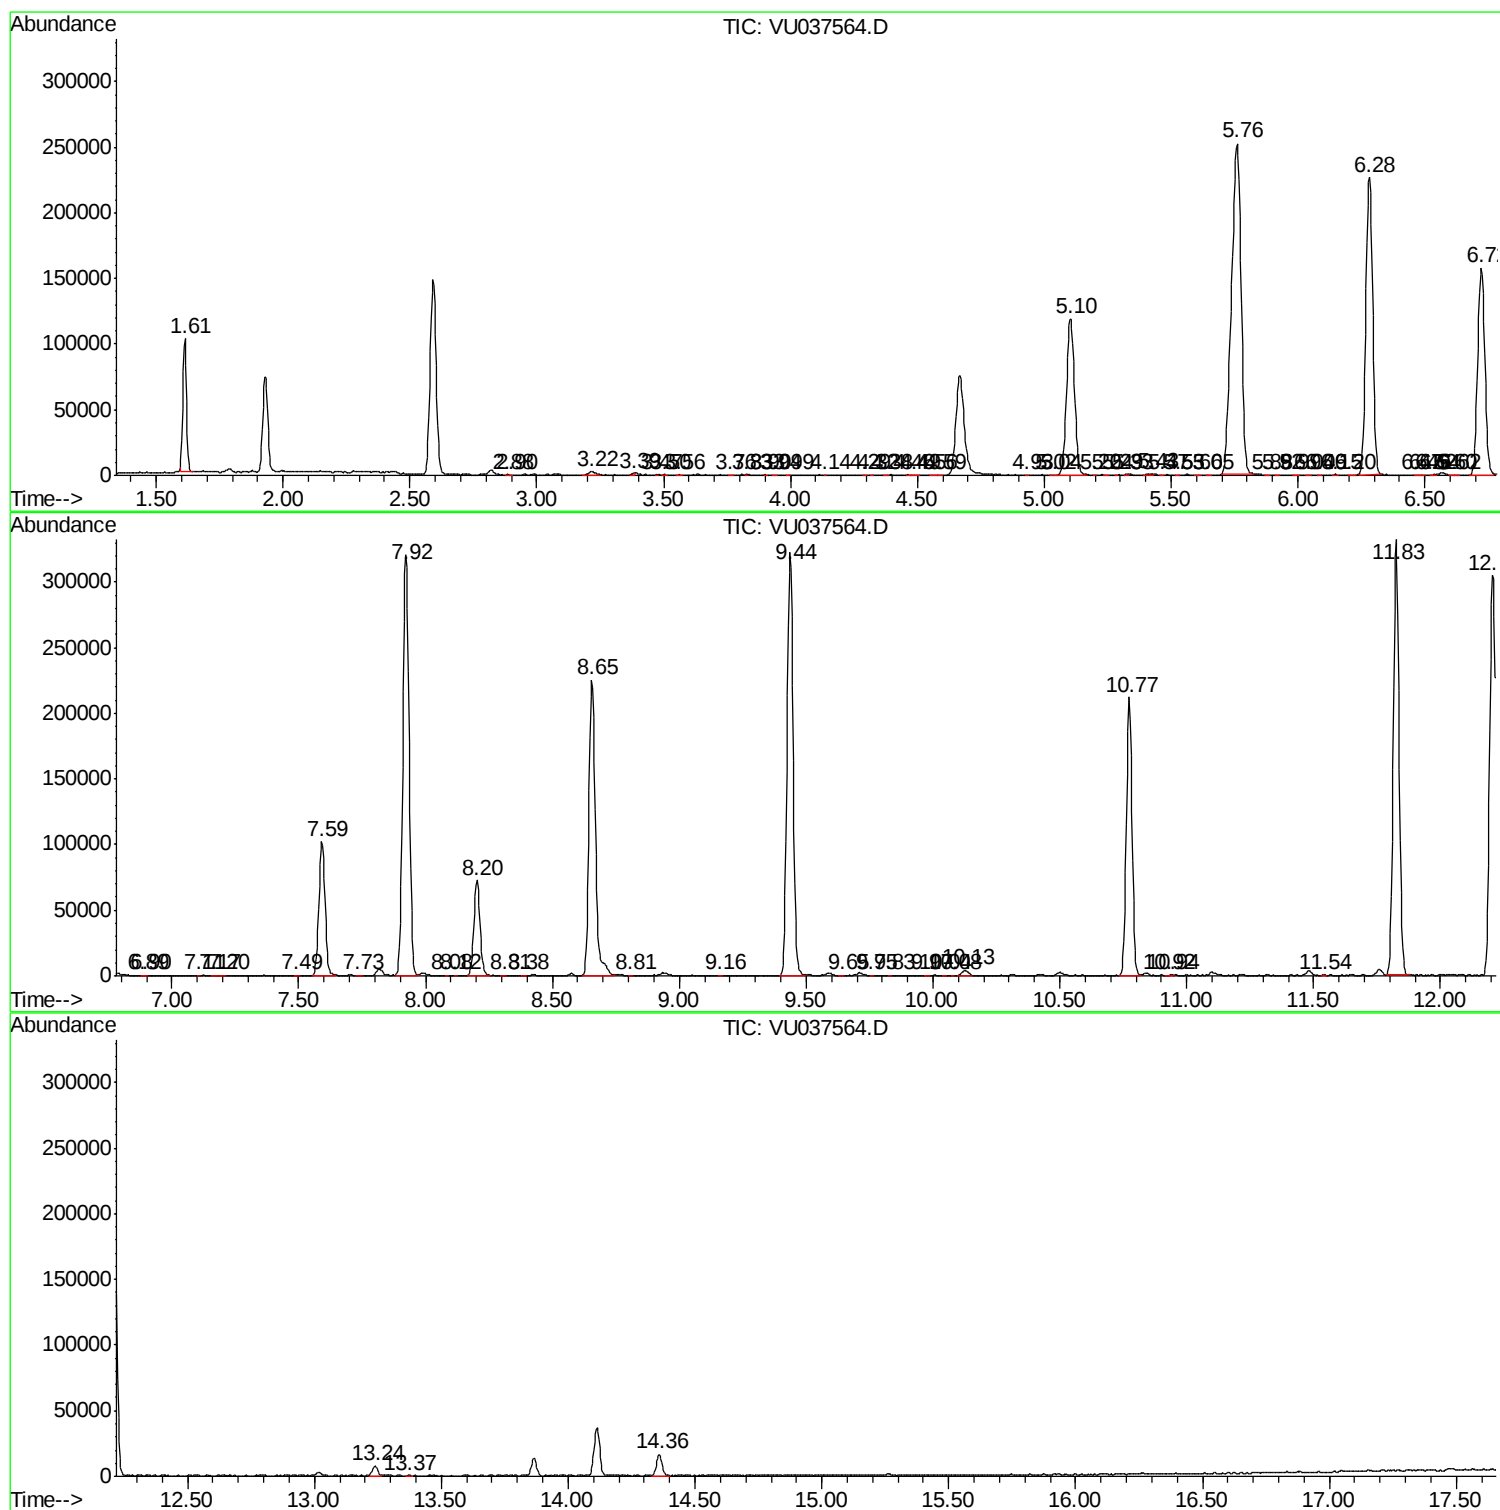

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040320\
Data File : VU037564.D
Acq On : 03 Apr 2020 12:03
Operator : JC/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040320\
Data File : VU037564.D
Acq On : 03 Apr 2020 12:03
Operator : JC/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc
