

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040320\
 Data File : VU037577.D
 Acq On : 03 Apr 2020 19:25
 Operator : JC/MD
 Sample : L2158-06 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0F03

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	79	85	99	rVB	93327	100663	15.45%	1.944%
2	2.591	379	389	406	rVB	141309	232836	35.74%	4.497%
3	2.999	513	516	518	rBV	439	250	0.04%	0.005%
4	3.047	529	531	533	rBV	294	164	0.03%	0.003%
5	3.224	573	586	597	rBV2	5541	12748	1.96%	0.246%
6	3.398	639	640	641	rVB2	208	40	0.01%	0.001%
7	3.417	643	646	647	rBV	257	161	0.02%	0.003%
8	3.517	674	677	682	rBV2	328	294	0.05%	0.006%
9	3.562	689	691	694	rVB2	472	236	0.04%	0.005%
10	3.649	715	718	722	rVB	280	207	0.03%	0.004%
11	3.674	724	726	728	rVB	131	35	0.01%	0.001%
12	3.684	728	729	730	rBV	109	27	0.00%	0.001%
13	3.790	759	762	766	rBV2	293	189	0.03%	0.004%
14	3.806	766	767	768	rBV2	124	28	0.00%	0.001%
15	3.854	778	782	784	rBV	120	109	0.02%	0.002%
16	3.912	798	800	802	rVB	258	104	0.02%	0.002%
17	3.973	816	819	821	rBV	202	114	0.02%	0.002%
18	4.002	824	828	834	rBV	308	251	0.04%	0.005%
19	4.038	838	839	840	rBV	166	52	0.01%	0.001%
20	4.067	846	848	854	rBV	202	186	0.03%	0.004%
21	4.221	893	896	897	rBV	136	57	0.01%	0.001%
22	4.256	903	907	909	rBV	170	113	0.02%	0.002%
23	4.276	910	913	917	rVB2	213	150	0.02%	0.003%
24	4.327	926	929	930	rBV	199	125	0.02%	0.002%
25	4.372	940	943	947	rBV	314	234	0.04%	0.005%
26	4.542	994	996	1000	rVB	196	96	0.01%	0.002%
27	4.558	1000	1001	1002	rBV	145	43	0.01%	0.001%
28	4.668	1022	1035	1056	rBV2	81390	189345	29.06%	3.657%
29	4.906	1105	1109	1113	rVB2	418	256	0.04%	0.005%
30	5.105	1155	1171	1192	rVB	116893	254271	39.03%	4.911%
31	5.185	1192	1196	1197	rBV	183	143	0.02%	0.003%
32	5.214	1204	1205	1208	rBV	229	77	0.01%	0.001%
33	5.266	1218	1221	1223	rBV	168	77	0.01%	0.001%
34	5.327	1235	1240	1243	rBV2	389	360	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040320\
 Data File : VU037577.D
 Acq On : 03 Apr 2020 19:25
 Operator : JC/MD
 Sample : L2158-06 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0F03

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
 Title : VOC Analysis

35	5.372	1250	1254	1259	rBV	200	187	0.03%	0.004%
36	5.401	1259	1263	1269	rVB3	347	362	0.06%	0.007%
37	5.456	1278	1280	1281	rBV3	119	51	0.01%	0.001%
38	5.542	1305	1307	1310	rVB	136	38	0.01%	0.001%
39	5.594	1321	1323	1325	rBV	242	52	0.01%	0.001%
40	5.671	1343	1347	1349	rBV	363	232	0.04%	0.004%
41	5.761	1355	1375	1394	rVB2	251046	651528	100.00%	12.584%
42	5.922	1423	1425	1428	rVB	325	158	0.02%	0.003%
43	6.073	1471	1472	1474	rBV	122	30	0.00%	0.001%
44	6.153	1494	1497	1498	rBV	251	123	0.02%	0.002%
45	6.192	1507	1509	1514	rBV3	277	200	0.03%	0.004%
46	6.282	1521	1537	1554	rBV	221014	407049	62.48%	7.862%
47	6.375	1562	1566	1571	rBV2	392	393	0.06%	0.008%
48	6.449	1587	1589	1594	rBV	173	123	0.02%	0.002%
49	6.475	1595	1597	1599	rVB	127	51	0.01%	0.001%
50	6.488	1599	1601	1602	rBV	224	73	0.01%	0.001%
51	6.574	1616	1628	1640	rVB3	39006	71522	10.98%	1.381%
52	6.674	1657	1659	1660	rBV	373	154	0.02%	0.003%
53	6.722	1661	1674	1692	rVB	156670	302451	46.42%	5.842%
54	6.809	1699	1701	1703	rBV	156	75	0.01%	0.001%
55	6.877	1720	1722	1724	rBV	202	62	0.01%	0.001%
56	6.928	1735	1738	1744	rBV	267	241	0.04%	0.005%
57	6.957	1744	1747	1750	rBV2	193	151	0.02%	0.003%
58	7.037	1770	1772	1777	rBV	201	116	0.02%	0.002%
59	7.066	1777	1781	1782	rBV	203	133	0.02%	0.003%
60	7.095	1788	1790	1792	rVB	151	61	0.01%	0.001%
61	7.111	1792	1795	1799	rBV	277	192	0.03%	0.004%
62	7.205	1823	1824	1827	rBV	322	166	0.03%	0.003%
63	7.253	1837	1839	1841	rVB	231	98	0.02%	0.002%
64	7.327	1860	1862	1864	rBV	301	113	0.02%	0.002%
65	7.378	1876	1878	1881	rBV	205	80	0.01%	0.002%
66	7.394	1881	1883	1884	rBV	257	102	0.02%	0.002%
67	7.523	1921	1923	1926	rVB	194	64	0.01%	0.001%
68	7.594	1931	1945	1961	rVV	99332	171151	26.27%	3.306%
69	7.713	1976	1982	1991	rBV3	508	750	0.12%	0.014%
70	7.809	2009	2012	2013	rBV	359	189	0.03%	0.004%
71	7.922	2034	2047	2063	rBV	313704	533721	81.92%	10.308%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU040320\
 Data File : VU037577.D
 Acq On : 03 Apr 2020 19:25
 Operator : JC/MD
 Sample : L2158-06 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0F03

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
 Title : VOC Analysis

72	8.050	2084	2087	2088	rBV	183	104	0.02%	0.002%
73	8.121	2107	2109	2111	rBV	264	122	0.02%	0.002%
74	8.420	2200	2202	2204	rBV	183	73	0.01%	0.001%
75	8.462	2212	2215	2218	rBV2	200	121	0.02%	0.002%
76	8.481	2218	2221	2222	rBV2	290	124	0.02%	0.002%
77	8.574	2243	2250	2257	rVB6	1926	2418	0.37%	0.047%
78	8.607	2257	2260	2262	rVB2	219	113	0.02%	0.002%
79	8.655	2262	2275	2301	rBV	231594	398638	61.19%	7.699%
80	8.854	2334	2337	2338	rBV	237	98	0.02%	0.002%
81	8.906	2351	2353	2356	rVB	143	68	0.01%	0.001%
82	8.922	2356	2358	2360	rVB	159	44	0.01%	0.001%
83	8.938	2360	2363	2364	rBV	181	81	0.01%	0.002%
84	9.115	2416	2418	2420	rBV	154	51	0.01%	0.001%
85	9.365	2493	2496	2497	rBV	237	115	0.02%	0.002%
86	9.436	2506	2518	2536	rBV	314661	511492	78.51%	9.879%
87	9.536	2547	2549	2551	rBV	161	68	0.01%	0.001%
88	9.934	2671	2673	2674	rBV	175	57	0.01%	0.001%
89	9.999	2691	2693	2695	rBV	160	63	0.01%	0.001%
90	10.066	2710	2714	2716	rBV	196	117	0.02%	0.002%
91	10.105	2722	2726	2729	rBV2	213	137	0.02%	0.003%
92	10.491	2844	2846	2848	rBV	171	70	0.01%	0.001%
93	10.774	2921	2934	2950	rBV	213640	341709	52.45%	6.600%
94	11.298	3094	3097	3098	rBV	261	137	0.02%	0.003%
95	11.414	3128	3133	3137	rBV	286	301	0.05%	0.006%
96	11.478	3146	3153	3156	rBV3	423	504	0.08%	0.010%
97	11.523	3164	3167	3173	rBV4	475	430	0.07%	0.008%
98	11.825	3249	3261	3279	rVB	318453	499936	76.73%	9.656%
99	12.134	3355	3357	3362	rBV2	349	247	0.04%	0.005%
100	12.208	3367	3380	3394	rBV	301735	483769	74.25%	9.344%


Sum of corrected areas: 5177490

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU040320\
Data File : VU037577.D
Acq On : 03 Apr 2020 19:25
Operator : JC/MD
Sample : L2158-06 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0F03

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

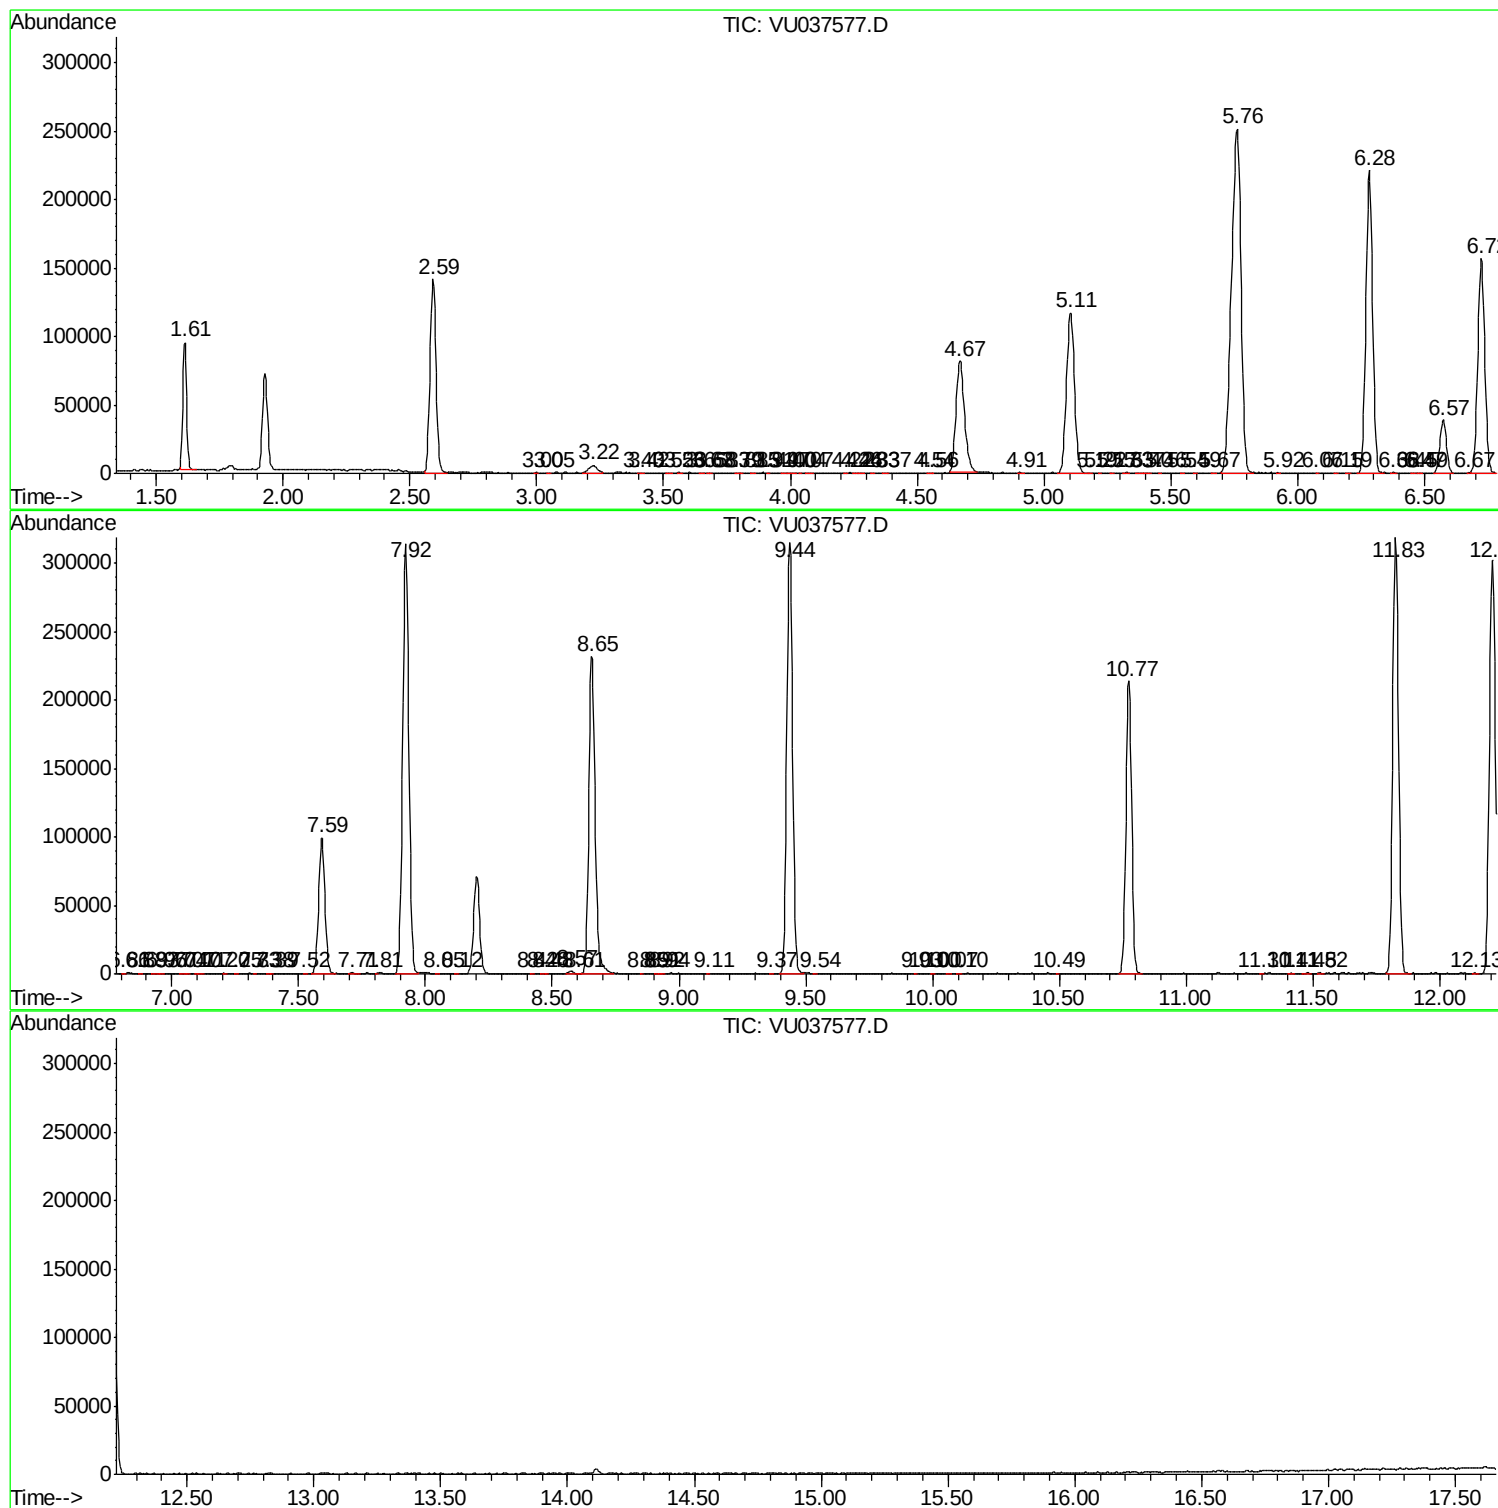

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040320\
Data File : VU037577.D
Acq On : 03 Apr 2020 19:25
Operator : JC/MD
Sample : L2158-06 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0F03

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU040320\
Data File : VU037577.D
Acq On : 03 Apr 2020 19:25
Operator : JC/MD
Sample : L2158-06 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0F03

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc