

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
 Data File : VU053512.D
 Acq On : 03 Apr 2023 12:06
 Operator : JC/MD
 Sample : VU0403WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK064

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053512.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rVB	148670	165717	17.65%	2.192%
2	1.909	169	177	192	rVB	111488	146565	15.61%	1.939%
3	2.565	368	381	397	rBV	207880	342985	36.52%	4.537%
4	2.858	470	472	477	rBV	286	137	0.01%	0.002%
5	3.044	521	530	540	rVB3	2815	4909	0.52%	0.065%
6	3.356	624	627	632	rVB4	527	385	0.04%	0.005%
7	3.501	667	672	674	rVB	279	219	0.02%	0.003%
8	3.604	702	704	706	rBV	153	92	0.01%	0.001%
9	3.787	759	761	763	rBV	173	78	0.01%	0.001%
10	4.031	831	837	841	rBV2	298	349	0.04%	0.005%
11	4.144	869	872	874	rBV	216	125	0.01%	0.002%
12	4.166	878	879	881	rBV	132	34	0.00%	0.000%
13	4.469	970	973	979	rBV	166	163	0.02%	0.002%
14	4.616	1007	1019	1051	rBV	73953	183774	19.57%	2.431%
15	5.002	1135	1139	1141	rBV	389	293	0.03%	0.004%
16	5.057	1141	1156	1181	rVV	175247	385914	41.09%	5.105%
17	5.385	1257	1258	1260	rBV	186	87	0.01%	0.001%
18	5.510	1295	1297	1301	rVB	139	57	0.01%	0.001%
19	5.536	1303	1305	1307	rBV2	188	98	0.01%	0.001%
20	5.719	1340	1362	1384	rBV2	344347	939095	100.00%	12.424%
21	6.034	1458	1460	1461	rBV	235	64	0.01%	0.001%
22	6.108	1480	1483	1489	rVB3	332	261	0.03%	0.003%
23	6.243	1511	1525	1543	rBV	304854	577242	61.47%	7.637%
24	6.481	1594	1599	1600	rBV3	377	275	0.03%	0.004%
25	6.530	1604	1614	1625	rVB7	5727	10867	1.16%	0.144%
26	6.684	1649	1662	1685	rBV	211844	417739	44.48%	5.526%
27	6.870	1718	1720	1723	rVB	155	69	0.01%	0.001%
28	7.121	1796	1798	1800	rBV2	160	93	0.01%	0.001%
29	7.189	1814	1819	1823	rBV3	421	413	0.04%	0.005%
30	7.423	1891	1892	1896	rVB2	190	129	0.01%	0.002%
31	7.446	1896	1899	1902	rBV	243	167	0.02%	0.002%
32	7.562	1923	1935	1960	rBV	125400	221949	23.63%	2.936%
33	7.793	2001	2007	2014	rBV2	289	429	0.05%	0.006%
34	7.893	2024	2038	2069	rBV	447544	783556	83.44%	10.366%
35	8.105	2102	2104	2109	rVB2	374	257	0.03%	0.003%
36	8.173	2114	2125	2141	rBV	89198	149429	15.91%	1.977%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
 Data File : VU053512.D
 Acq On : 03 Apr 2023 12:06
 Operator : JC/MD
 Sample : VU0403WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK064

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	8.340	2175	2177	2183	rVB	242	187	0.02%	0.002%
38	8.411	2196	2199	2204	rVB	312	197	0.02%	0.003%
39	8.468	2214	2217	2222	rBV2	337	279	0.03%	0.004%
40	8.549	2238	2242	2248	rVB3	858	757	0.08%	0.010%
41	8.571	2248	2249	2253	rVB	222	79	0.01%	0.001%
42	8.626	2254	2266	2291	rBV2	224680	416098	44.31%	5.505%
43	8.983	2375	2377	2384	rBV2	238	264	0.03%	0.003%
44	9.047	2393	2397	2401	rVB2	350	269	0.03%	0.004%
45	9.073	2402	2405	2407	rBV2	274	155	0.02%	0.002%
46	9.095	2409	2412	2414	rBV	223	139	0.01%	0.002%
47	9.131	2422	2423	2427	rVB	153	56	0.01%	0.001%
48	9.153	2427	2430	2433	rBV2	393	298	0.03%	0.004%
49	9.182	2437	2439	2441	rBV	209	113	0.01%	0.001%
50	9.247	2457	2459	2463	rBV	175	78	0.01%	0.001%
51	9.414	2498	2511	2533	rBV	436741	724262	77.12%	9.582%
52	9.693	2595	2598	2599	rBV	507	266	0.03%	0.004%
53	9.890	2656	2659	2661	rBV	223	138	0.01%	0.002%
54	9.973	2683	2685	2688	rBB2	175	96	0.01%	0.001%
55	10.201	2753	2756	2758	rBV	232	168	0.02%	0.002%
56	10.301	2782	2787	2789	rBV2	354	357	0.04%	0.005%
57	10.475	2838	2841	2842	rBV	370	164	0.02%	0.002%
58	10.636	2885	2891	2896	rBV3	1023	1289	0.14%	0.017%
59	10.751	2915	2927	2943	rBV	316622	506123	53.89%	6.696%
60	11.031	3012	3014	3019	rVB	249	152	0.02%	0.002%
61	11.182	3058	3061	3064	rBV	308	233	0.02%	0.003%
62	11.256	3082	3084	3086	rBV	234	86	0.01%	0.001%
63	11.407	3130	3131	3134	rBV2	220	111	0.01%	0.001%
64	11.459	3144	3147	3149	rBV	718	550	0.06%	0.007%
65	11.545	3169	3174	3177	rBV	387	321	0.03%	0.004%
66	11.623	3196	3198	3202	rBV	196	107	0.01%	0.001%
67	11.745	3229	3236	3243	rBV3	1271	1611	0.17%	0.021%
68	11.806	3243	3255	3275	rBV	476208	768232	81.81%	10.163%
69	12.015	3318	3320	3322	rBV	186	64	0.01%	0.001%
70	12.121	3350	3353	3355	rBV	324	189	0.02%	0.003%
71	12.189	3361	3374	3396	rBV	479805	785764	83.67%	10.395%
72	13.127	3663	3666	3671	rVB2	444	391	0.04%	0.005%
73	13.160	3673	3676	3677	rBV2	386	176	0.02%	0.002%
74	13.224	3691	3696	3708	rVB7	1432	2293	0.24%	0.030%
75	13.407	3750	3753	3754	rBV7	306	133	0.01%	0.002%
76	13.844	3882	3889	3899	rBV3	2603	3847	0.41%	0.051%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053512.D
Acq On : 03 Apr 2023 12:06
Operator : JC/MD
Sample : VU0403WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK064

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Title : VOC Analysis

77	14.089	3957	3965	3978	rBV2	4174	8329	0.89%	0.110%
78	14.285	4023	4026	4029	rBV	537	468	0.05%	0.006%




Sum of corrected areas: 7558904

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053512.D
Acq On : 03 Apr 2023 12:06
Operator : JC/MD
Sample : VU0403WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK064

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

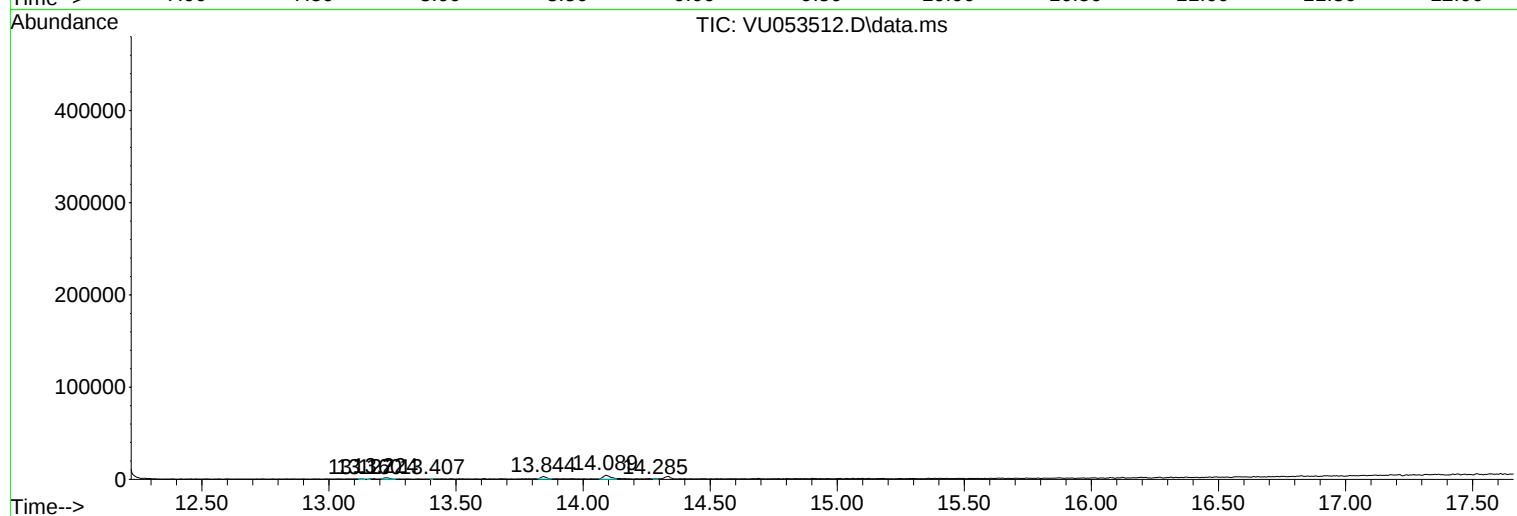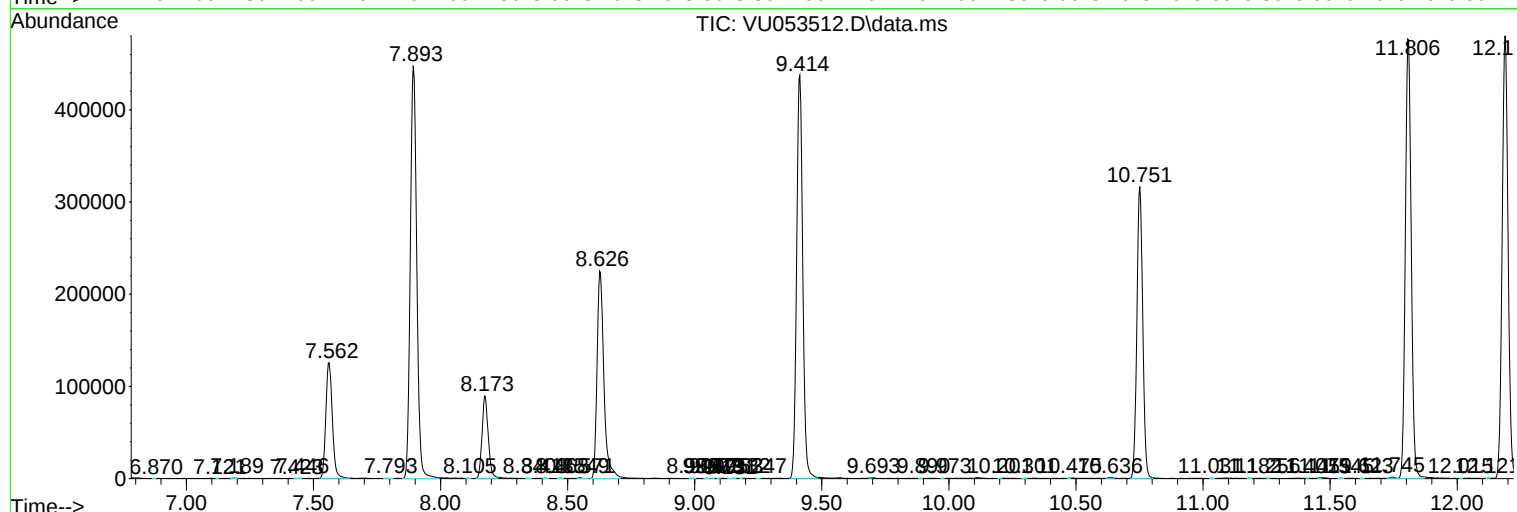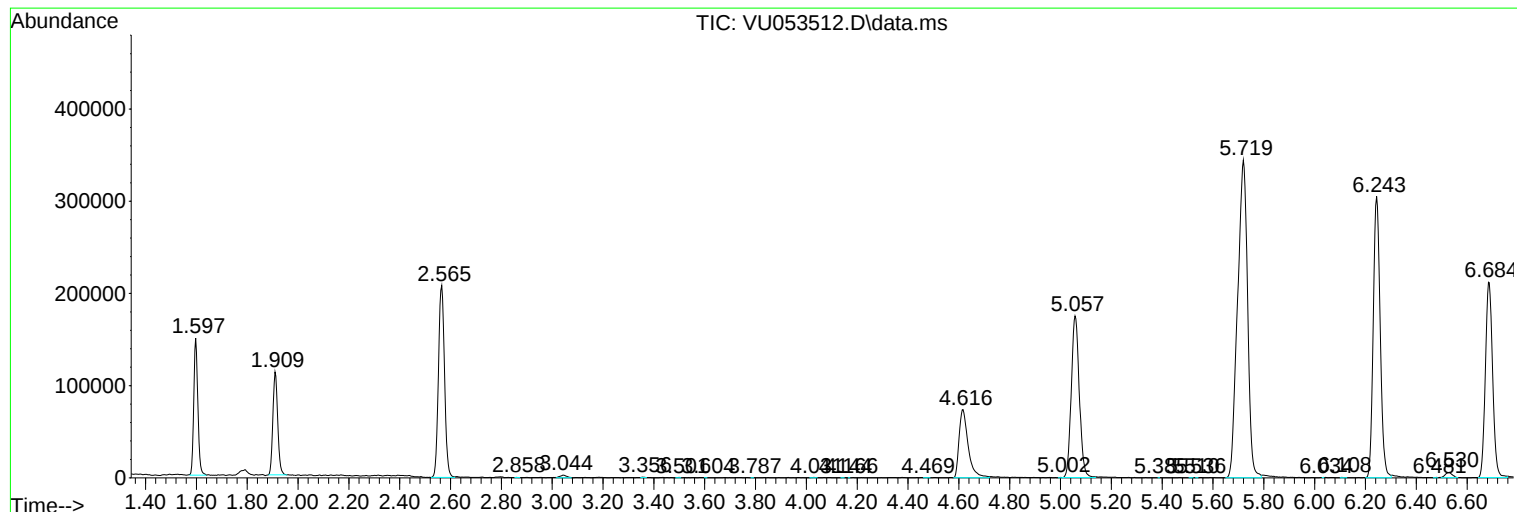

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053512.D
Acq On : 03 Apr 2023 12:06
Operator : JC/MD
Sample : VU0403WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK064

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053512.D
Acq On : 03 Apr 2023 12:06
Operator : JC/MD
Sample : VU0403WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK064

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------