

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
 Data File : VU053519.D
 Acq On : 03 Apr 2023 14:52
 Operator : JC/MD
 Sample : 02158-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TB(20230328)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M

Title : VOC Analysis

Signal : TIC: VU053519.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	94	rVB	144003	158129	16.83%	2.073%
2	1.909	169	177	193	rVB	109723	147570	15.70%	1.934%
3	2.562	369	380	397	rBV	204447	336803	35.84%	4.414%
4	2.887	478	481	486	rBV3	435	341	0.04%	0.004%
5	3.038	523	528	532	rBV3	1197	1488	0.16%	0.020%
6	3.076	538	540	543	rVB	217	90	0.01%	0.001%
7	3.093	543	545	551	rBV	209	133	0.01%	0.002%
8	3.340	620	622	625	rVB	175	93	0.01%	0.001%
9	3.395	637	639	643	rVB	264	118	0.01%	0.002%
10	3.623	709	710	711	rBV	119	24	0.00%	0.000%
11	3.816	767	770	772	rBV2	238	146	0.02%	0.002%
12	3.867	784	786	788	rBV2	193	107	0.01%	0.001%
13	3.935	804	807	810	rVB2	193	105	0.01%	0.001%
14	3.977	818	820	823	rBV	262	147	0.02%	0.002%
15	4.137	867	870	872	rBV2	268	162	0.02%	0.002%
16	4.179	881	883	886	rBV2	183	148	0.02%	0.002%
17	4.343	932	934	938	rVB	182	74	0.01%	0.001%
18	4.366	938	941	942	rBV	155	75	0.01%	0.001%
19	4.433	959	962	964	rBV	187	95	0.01%	0.001%
20	4.514	985	987	990	rVB	287	149	0.02%	0.002%
21	4.613	1006	1018	1048	rBV	75045	180357	19.19%	2.364%
22	4.967	1125	1128	1132	rBV	185	127	0.01%	0.002%
23	4.990	1132	1135	1137	rBV2	170	120	0.01%	0.002%
24	5.057	1141	1156	1181	rVV	173590	380177	40.46%	4.983%
25	5.285	1223	1227	1229	rBV3	530	334	0.04%	0.004%
26	5.317	1235	1237	1238	rBV3	121	34	0.00%	0.000%
27	5.330	1238	1241	1244	rVB2	360	208	0.02%	0.003%
28	5.398	1258	1262	1264	rBV2	193	176	0.02%	0.002%
29	5.491	1287	1291	1292	rBV	232	158	0.02%	0.002%
30	5.600	1321	1325	1328	rBV	243	246	0.03%	0.003%
31	5.620	1328	1331	1337	rBV	194	174	0.02%	0.002%
32	5.719	1340	1362	1384	rBV2	342899	939692	100.00%	12.316%
33	5.990	1443	1446	1447	rBV	306	159	0.02%	0.002%
34	6.054	1463	1466	1468	rVB2	203	109	0.01%	0.001%
35	6.244	1511	1525	1545	rBV	318532	600987	63.96%	7.877%
36	6.485	1598	1600	1604	rVB	314	135	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
 Data File : VU053519.D
 Acq On : 03 Apr 2023 14:52
 Operator : JC/MD
 Sample : 02158-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TB(20230328)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	6.533	1604	1615	1628	rBV9	8296	17271	1.84%	0.226%
38	6.684	1648	1662	1683	rBV	220572	434068	46.19%	5.689%
39	6.957	1745	1747	1748	rBV	153	84	0.01%	0.001%
40	7.067	1779	1781	1784	rVB	352	238	0.03%	0.003%
41	7.092	1785	1789	1795	rBV2	430	501	0.05%	0.007%
42	7.137	1801	1803	1807	rBV2	212	135	0.01%	0.002%
43	7.298	1851	1853	1855	rBV2	170	101	0.01%	0.001%
44	7.417	1884	1890	1895	rVB2	344	301	0.03%	0.004%
45	7.562	1922	1935	1949	rBV	132496	230252	24.50%	3.018%
46	7.790	2003	2006	2007	rBV	150	64	0.01%	0.001%
47	7.893	2025	2038	2071	rBV	470204	817221	86.97%	10.711%
48	8.131	2109	2112	2114	rBV2	144	106	0.01%	0.001%
49	8.176	2114	2126	2147	rVV	92788	156366	16.64%	2.049%
50	8.276	2155	2157	2161	rBV	159	124	0.01%	0.002%
51	8.375	2184	2188	2192	rVB2	348	220	0.02%	0.003%
52	8.423	2200	2203	2204	rBV2	232	115	0.01%	0.002%
53	8.552	2229	2243	2250	rBV3	3921	6163	0.66%	0.081%
54	8.626	2255	2266	2297	rBV	231333	427792	45.52%	5.607%
55	8.780	2312	2314	2319	rBV2	273	193	0.02%	0.003%
56	8.886	2344	2347	2350	rBV	100	76	0.01%	0.001%
57	8.906	2350	2353	2354	rBV	279	140	0.01%	0.002%
58	9.057	2398	2400	2403	rBV2	215	126	0.01%	0.002%
59	9.089	2407	2410	2416	rVV	372	263	0.03%	0.003%
60	9.150	2427	2429	2430	rBV	256	92	0.01%	0.001%
61	9.263	2461	2464	2468	rBV	257	201	0.02%	0.003%
62	9.414	2497	2511	2534	rBV	433101	723126	76.95%	9.478%
63	9.700	2595	2600	2609	rVB3	457	658	0.07%	0.009%
64	9.735	2609	2611	2613	rBV	227	152	0.02%	0.002%
65	9.935	2671	2673	2677	rBV	207	114	0.01%	0.001%
66	9.957	2677	2680	2682	rVV2	213	120	0.01%	0.002%
67	10.243	2767	2769	2772	rBV	280	177	0.02%	0.002%
68	10.411	2819	2821	2825	rBV	200	170	0.02%	0.002%
69	10.681	2903	2905	2908	rVB	250	113	0.01%	0.001%
70	10.751	2914	2927	2949	rBV	316024	502094	53.43%	6.581%
71	10.861	2959	2961	2964	rBV	294	197	0.02%	0.003%
72	10.957	2988	2991	2996	rBV2	297	222	0.02%	0.003%
73	10.980	2996	2998	2999	rBV2	282	120	0.01%	0.002%
74	11.018	3008	3010	3016	rVB	187	99	0.01%	0.001%
75	11.092	3029	3033	3038	rBV	355	272	0.03%	0.004%
76	11.137	3044	3047	3049	rBV	182	121	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
 Data File : VU053519.D
 Acq On : 03 Apr 2023 14:52
 Operator : JC/MD
 Sample : 02158-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TB(20230328)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M

Title : VOC Analysis

77	11.314	3098	3102	3108	rBV4	1362	1818	0.19%	0.024%
78	11.462	3147	3148	3152	rVB	272	103	0.01%	0.001%
79	11.745	3233	3236	3241	rVB	540	407	0.04%	0.005%
80	11.806	3243	3255	3275	rBV	484343	768468	81.78%	10.072%
81	12.121	3352	3353	3354	rBV	241	61	0.01%	0.001%
82	12.189	3361	3374	3391	rBV	483691	787200	83.77%	10.318%
83	12.401	3436	3440	3443	rBV2	333	310	0.03%	0.004%
84	12.552	3484	3487	3491	rBV	300	259	0.03%	0.003%
85	12.767	3551	3554	3557	rBV2	301	227	0.02%	0.003%
86	12.947	3608	3610	3614	rVB	515	225	0.02%	0.003%
87	12.996	3622	3625	3629	rBV2	411	390	0.04%	0.005%
88	13.999	3934	3937	3941	rBV2	439	278	0.03%	0.004%
89	15.629	4441	4444	4446	rBV2	1044	663	0.07%	0.009%




Sum of corrected areas: 7629567

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053519.D
Acq On : 03 Apr 2023 14:52
Operator : JC/MD
Sample : 02158-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TB(20230328)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

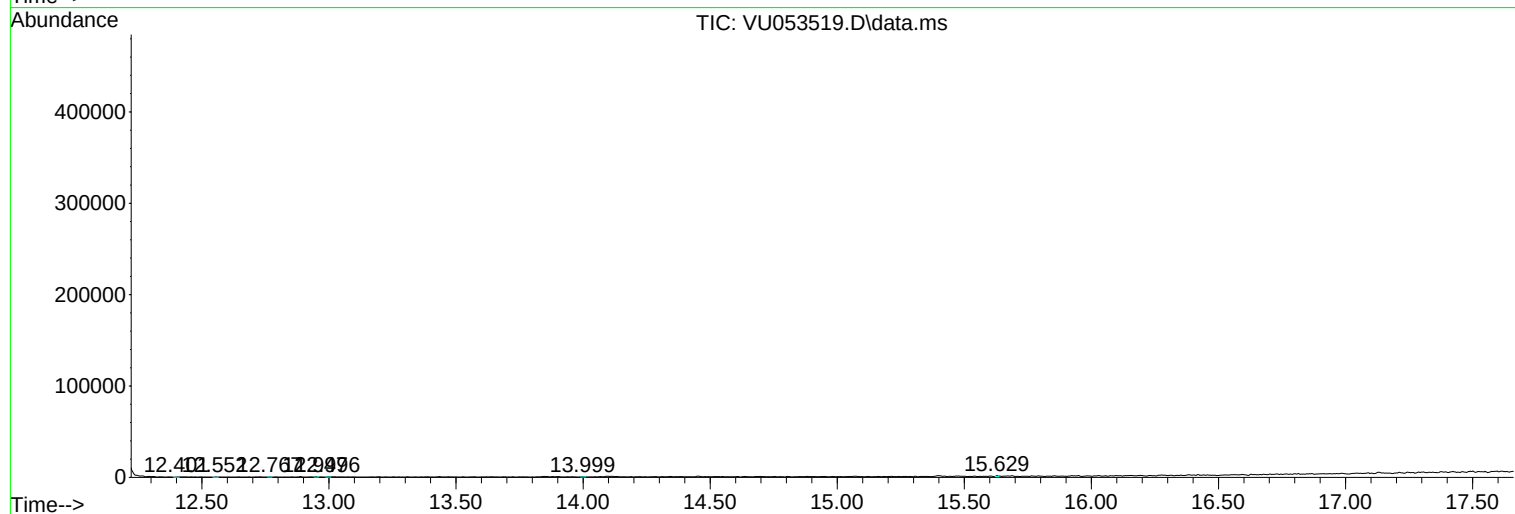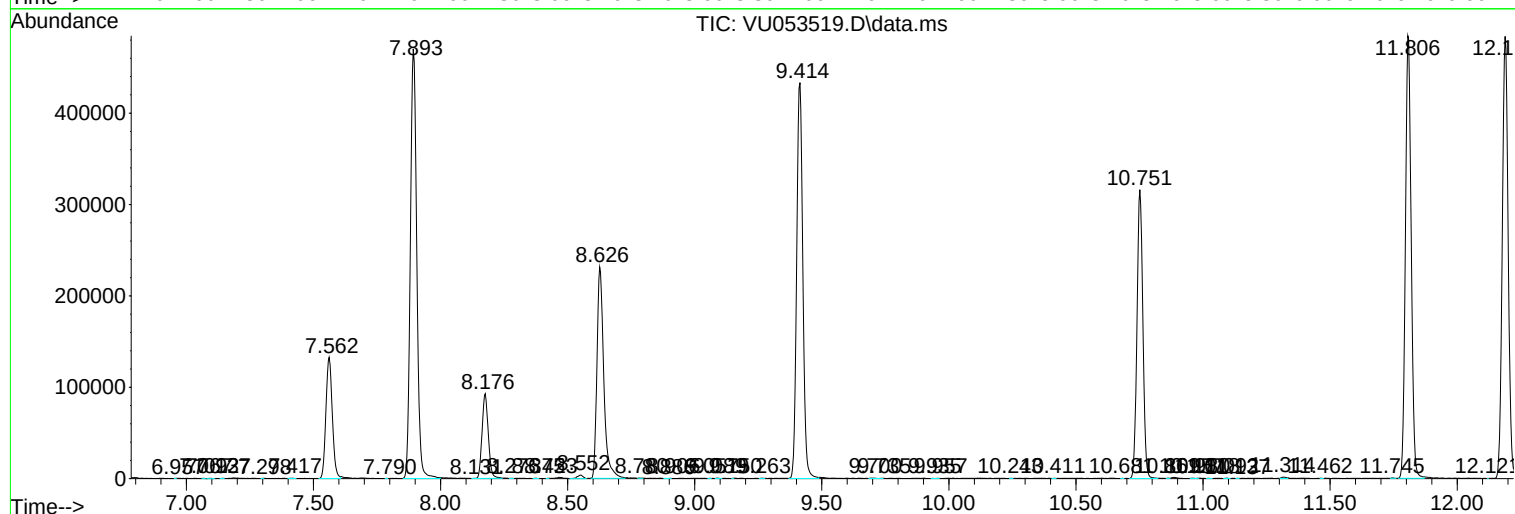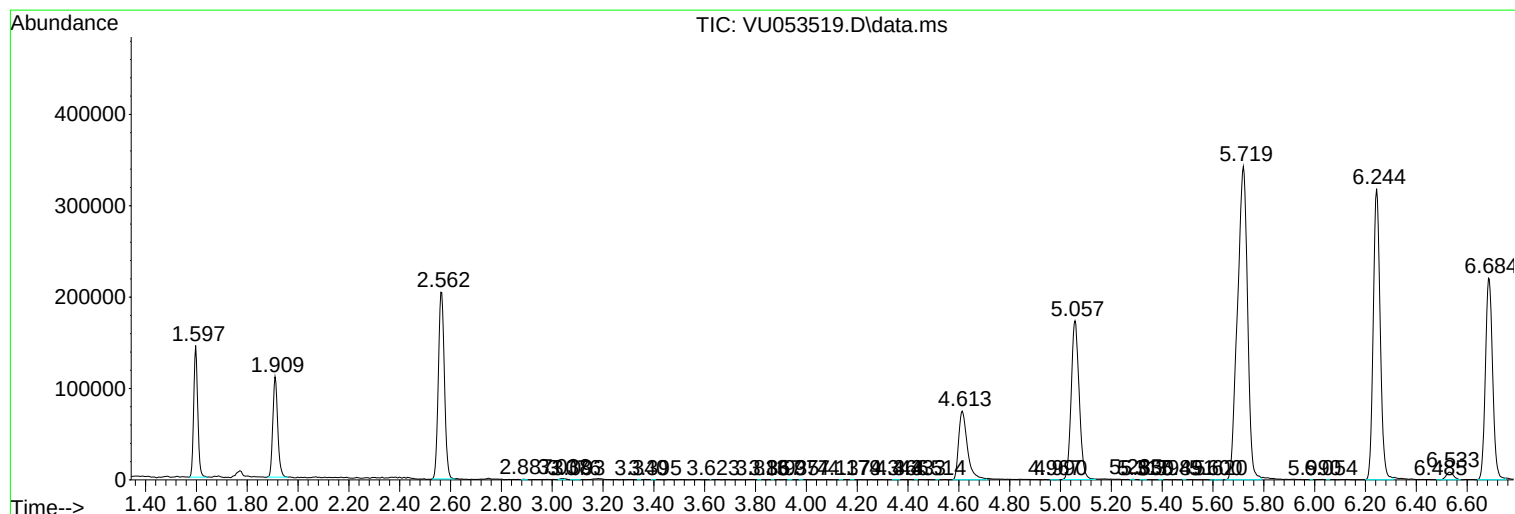

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053519.D
Acq On : 03 Apr 2023 14:52
Operator : JC/MD
Sample : 02158-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TB(20230328)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053519.D
Acq On : 03 Apr 2023 14:52
Operator : JC/MD
Sample : 02158-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TB(20230328)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------