

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
 Data File : VU053521.D
 Acq On : 03 Apr 2023 15:39
 Operator : JC/MD
 Sample : 02158-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TB(20230329)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M

Title : VOC Analysis

Signal : TIC: VU053521.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	90	rBV	141195	150556	15.69%	1.987%
2	1.909	169	177	191	rVB	106899	145002	15.11%	1.914%
3	2.510	361	364	368	rBV2	620	378	0.04%	0.005%
4	2.565	368	381	398	rBV	197415	325436	33.91%	4.295%
5	2.944	496	499	501	rBV	293	218	0.02%	0.003%
6	3.047	521	531	539	rVB5	1731	2876	0.30%	0.038%
7	3.086	539	543	545	rBV2	224	154	0.02%	0.002%
8	3.173	561	570	584	rVB4	1347	3230	0.34%	0.043%
9	3.227	584	587	590	rBV	269	161	0.02%	0.002%
10	3.407	640	643	646	rBV	309	278	0.03%	0.004%
11	3.616	705	708	712	rVB2	291	195	0.02%	0.003%
12	3.642	712	716	720	rVV2	347	318	0.03%	0.004%
13	3.678	724	727	729	rVV	266	157	0.02%	0.002%
14	3.787	758	761	764	rBV	225	170	0.02%	0.002%
15	3.816	769	770	775	rVB2	317	202	0.02%	0.003%
16	3.838	775	777	782	rBV2	160	159	0.02%	0.002%
17	3.932	802	806	810	rBV	444	294	0.03%	0.004%
18	3.973	816	819	824	rBV	196	237	0.02%	0.003%
19	4.038	836	839	842	rBV2	275	197	0.02%	0.003%
20	4.208	890	892	898	rVB	309	172	0.02%	0.002%
21	4.407	951	954	957	rBV2	236	169	0.02%	0.002%
22	4.446	963	966	971	rBV2	267	248	0.03%	0.003%
23	4.613	1005	1018	1051	rBV	75585	185115	19.29%	2.443%
24	4.848	1088	1091	1094	rBV	298	257	0.03%	0.003%
25	4.903	1105	1108	1110	rBV2	379	257	0.03%	0.003%
26	5.057	1139	1156	1178	rBV2	176103	392363	40.89%	5.178%
27	5.295	1227	1230	1232	rBV	271	157	0.02%	0.002%
28	5.356	1244	1249	1250	rBV	237	170	0.02%	0.002%
29	5.404	1259	1264	1268	rBV2	293	234	0.02%	0.003%
30	5.430	1268	1272	1276	rBV	173	148	0.02%	0.002%
31	5.510	1295	1297	1302	rVB2	248	167	0.02%	0.002%
32	5.719	1341	1362	1385	rBV2	351781	959596	100.00%	12.665%
33	5.967	1436	1439	1442	rVB	327	201	0.02%	0.003%
34	5.986	1442	1445	1448	rVB2	342	226	0.02%	0.003%
35	6.047	1458	1464	1467	rBV2	599	452	0.05%	0.006%
36	6.157	1494	1498	1499	rBV	216	154	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
 Data File : VU053521.D
 Acq On : 03 Apr 2023 15:39
 Operator : JC/MD
 Sample : 02158-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TB(20230329)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	6.243	1511	1525	1550	rBV	315829	603776	62.92%	7.969%
38	6.456	1586	1591	1593	rBV	347	339	0.04%	0.004%
39	6.472	1593	1596	1603	rVB3	331	330	0.03%	0.004%
40	6.530	1603	1614	1624	rBV7	5396	10743	1.12%	0.142%
41	6.629	1642	1645	1649	rBV4	443	435	0.05%	0.006%
42	6.684	1649	1662	1681	rBV	215047	422109	43.99%	5.571%
43	6.825	1703	1706	1707	rBV	267	158	0.02%	0.002%
44	6.896	1722	1728	1731	rBV	337	350	0.04%	0.005%
45	7.179	1807	1816	1819	rBV3	560	704	0.07%	0.009%
46	7.394	1878	1883	1887	rBV2	351	340	0.04%	0.004%
47	7.475	1904	1908	1909	rBV	243	167	0.02%	0.002%
48	7.562	1922	1935	1953	rBV	126335	225963	23.55%	2.982%
49	7.684	1969	1973	1974	rBV	447	284	0.03%	0.004%
50	7.893	2025	2038	2069	rBV	454388	799564	83.32%	10.553%
51	8.105	2102	2104	2108	rBV2	283	160	0.02%	0.002%
52	8.173	2114	2125	2141	rBV	88858	151047	15.74%	1.994%
53	8.317	2167	2170	2176	rVB	369	265	0.03%	0.003%
54	8.346	2176	2179	2183	rBV2	226	226	0.02%	0.003%
55	8.465	2210	2216	2220	rVV2	922	996	0.10%	0.013%
56	8.539	2236	2239	2240	rBV	743	414	0.04%	0.005%
57	8.626	2253	2266	2299	rBV	228655	419643	43.73%	5.538%
58	8.857	2331	2338	2340	rBV	262	238	0.02%	0.003%
59	9.041	2390	2395	2399	rVB	299	280	0.03%	0.004%
60	9.066	2400	2403	2405	rBV2	276	183	0.02%	0.002%
61	9.218	2446	2450	2453	rVB	288	172	0.02%	0.002%
62	9.256	2459	2462	2465	rBV	247	194	0.02%	0.003%
63	9.275	2465	2468	2472	rVB	342	245	0.03%	0.003%
64	9.298	2472	2475	2478	rBV2	245	214	0.02%	0.003%
65	9.414	2498	2511	2530	rBV	432418	721245	75.16%	9.519%
66	9.690	2594	2597	2603	rVB3	358	327	0.03%	0.004%
67	9.722	2604	2607	2613	rBV	219	175	0.02%	0.002%
68	9.751	2613	2616	2619	rBV2	224	151	0.02%	0.002%
69	9.803	2629	2632	2637	rVB	310	265	0.03%	0.003%
70	9.954	2674	2679	2684	rVB2	293	369	0.04%	0.005%
71	10.063	2710	2713	2717	rBV2	209	149	0.02%	0.002%
72	10.295	2780	2785	2794	rVB2	325	543	0.06%	0.007%
73	10.365	2804	2807	2810	rBV	263	215	0.02%	0.003%
74	10.562	2865	2868	2869	rBV	282	150	0.02%	0.002%
75	10.613	2880	2884	2886	rVB	212	161	0.02%	0.002%
76	10.635	2886	2891	2893	rBV2	378	317	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
 Data File : VU053521.D
 Acq On : 03 Apr 2023 15:39
 Operator : JC/MD
 Sample : 02158-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TB(20230329)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

77	10.751	2912	2927	2947	rBV	309942	493829	51.46%	6.518%
78	10.825	2949	2950	2956	rVB2	471	247	0.03%	0.003%
79	10.886	2963	2969	2976	rVB3	790	1210	0.13%	0.016%
80	10.922	2976	2980	2983	rVV	181	183	0.02%	0.002%
81	10.951	2987	2989	2993	rVB	330	184	0.02%	0.002%
82	10.973	2993	2996	2998	rBV2	233	161	0.02%	0.002%
83	10.989	2998	3001	3008	rVB2	280	298	0.03%	0.004%
84	11.127	3042	3044	3046	rBV2	282	150	0.02%	0.002%
85	11.156	3051	3053	3060	rBV2	143	151	0.02%	0.002%
86	11.324	3098	3105	3107	rBV4	1642	1769	0.18%	0.023%
87	11.471	3148	3151	3156	rVB2	404	323	0.03%	0.004%
88	11.594	3186	3189	3191	rVV2	249	154	0.02%	0.002%
89	11.680	3213	3216	3219	rBV	252	212	0.02%	0.003%
90	11.748	3234	3237	3242	rVB2	500	436	0.05%	0.006%
91	11.809	3243	3256	3277	rBV	487822	770685	80.31%	10.171%
92	12.188	3361	3374	3396	rBV	475967	770217	80.26%	10.165%
93	12.285	3402	3404	3408	rBV2	637	326	0.03%	0.004%
94	12.577	3492	3495	3497	rBV	265	161	0.02%	0.002%
95	13.221	3693	3695	3700	rVB2	416	297	0.03%	0.004%
96	13.246	3701	3703	3707	rBV2	197	164	0.02%	0.002%
97	13.391	3745	3748	3751	rVB3	469	311	0.03%	0.004%
98	13.539	3790	3794	3797	rBV2	304	312	0.03%	0.004%
99	13.851	3887	3891	3892	rBV2	616	402	0.04%	0.005%
100	14.446	4071	4076	4078	rBV4	942	846	0.09%	0.011%


Sum of corrected areas: 7576938

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053521.D
Acq On : 03 Apr 2023 15:39
Operator : JC/MD
Sample : 02158-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TB(20230329)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

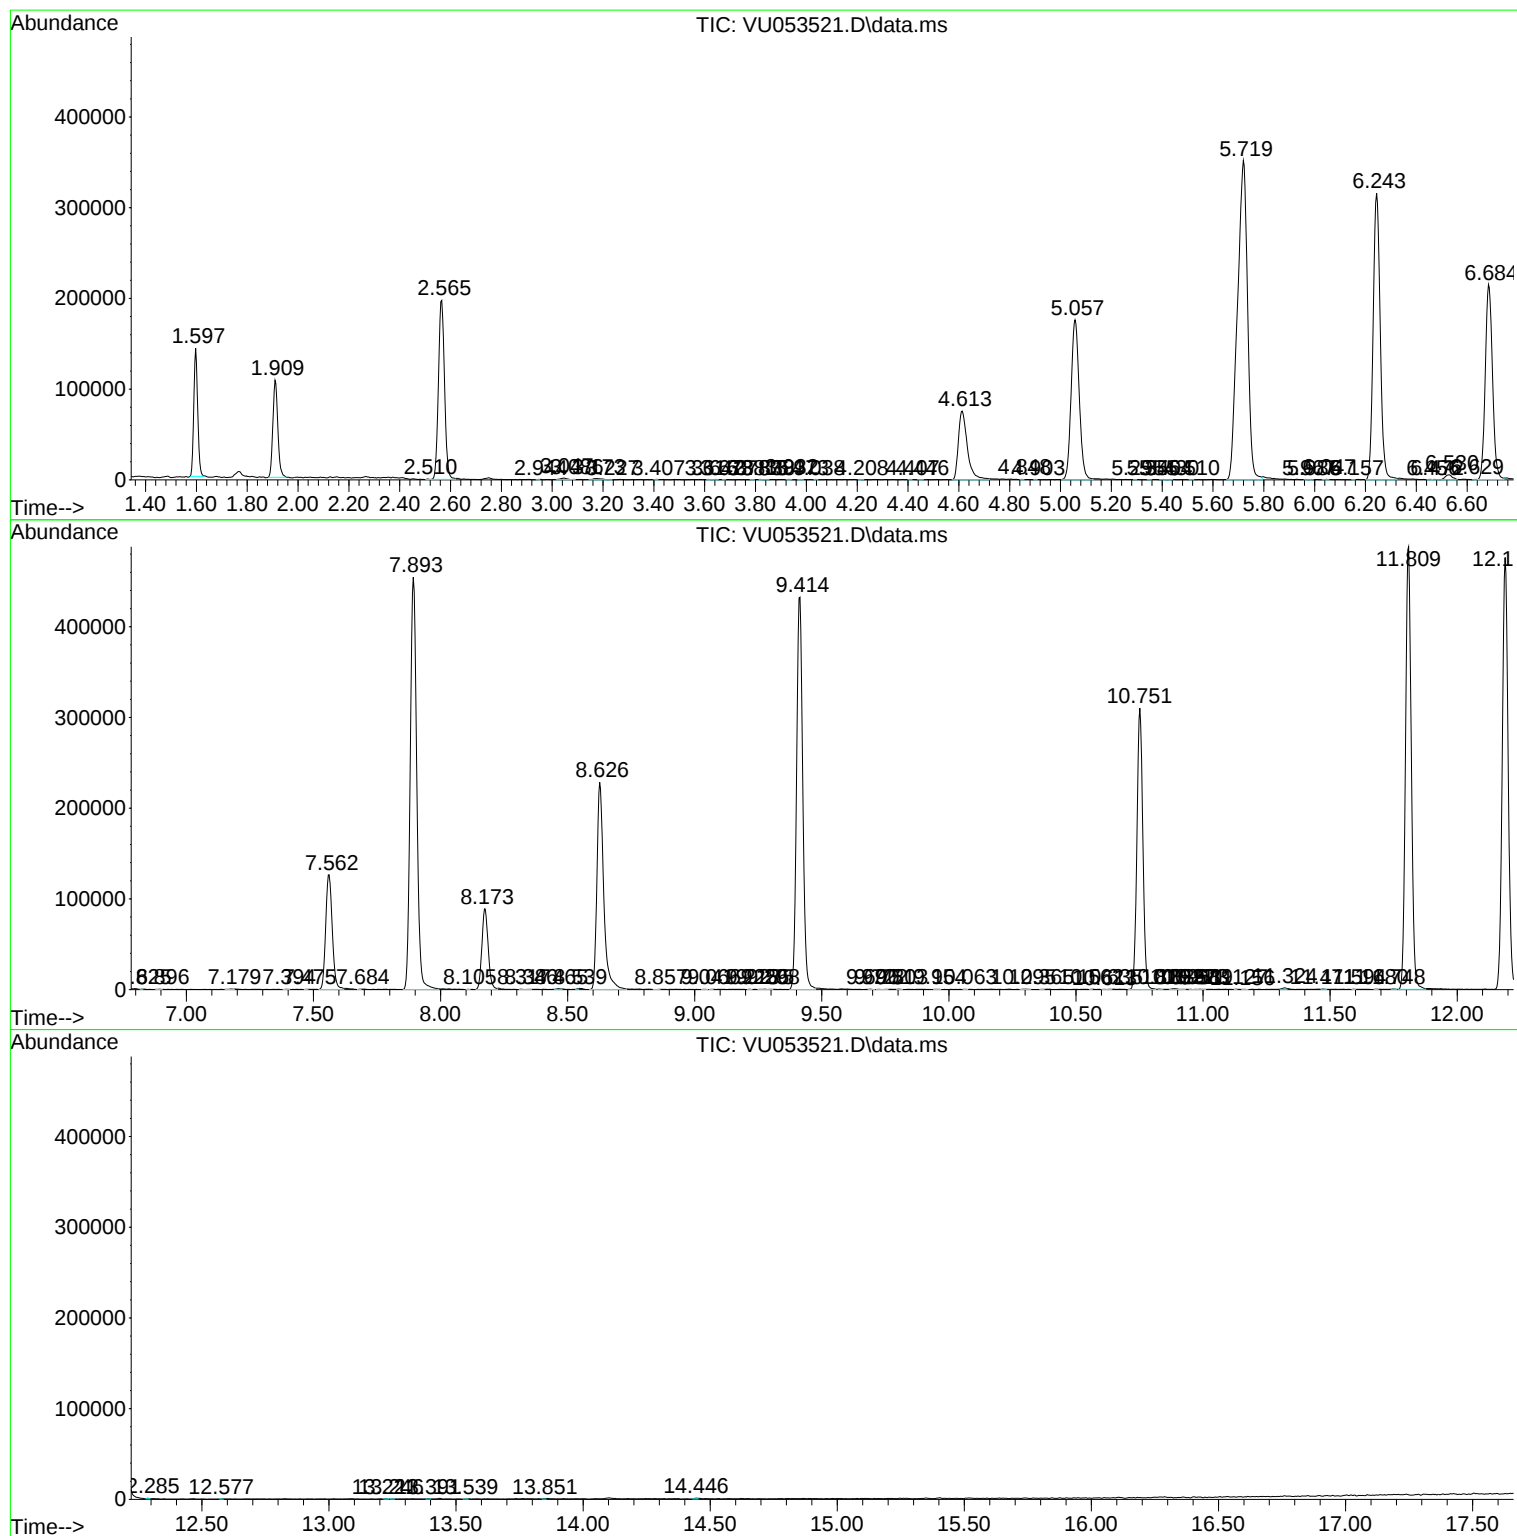

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053521.D
Acq On : 03 Apr 2023 15:39
Operator : JC/MD
Sample : 02158-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TB(20230329)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053521.D
Acq On : 03 Apr 2023 15:39
Operator : JC/MD
Sample : 02158-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TB(20230329)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------