

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
 Data File : VU053522.D
 Acq On : 03 Apr 2023 16:02
 Operator : JC/MD
 Sample : 02158-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 FB(20230328)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M

Title : VOC Analysis

Signal : TIC: VU053522.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rVB	144556	160295	16.32%	2.074%
2	1.909	169	177	192	rVB	109109	149196	15.19%	1.931%
3	2.565	368	381	398	rBV	212914	340058	34.63%	4.401%
4	2.681	415	417	420	rBV2	362	182	0.02%	0.002%
5	3.038	522	528	531	rBV2	1674	2005	0.20%	0.026%
6	3.401	637	641	644	rVB	287	197	0.02%	0.003%
7	3.414	644	645	649	rBV	246	96	0.01%	0.001%
8	3.584	695	698	700	rBV	228	116	0.01%	0.002%
9	3.816	767	770	772	rBV	232	163	0.02%	0.002%
10	3.870	783	787	791	rBV	454	454	0.05%	0.006%
11	3.890	791	793	795	rVV	142	59	0.01%	0.001%
12	3.931	804	806	809	rVB	243	143	0.01%	0.002%
13	3.951	809	812	815	rBV2	277	207	0.02%	0.003%
14	4.028	834	836	838	rBV	186	98	0.01%	0.001%
15	4.079	850	852	857	rBV	185	106	0.01%	0.001%
16	4.221	893	896	899	rBV	157	88	0.01%	0.001%
17	4.462	968	971	975	rBV	211	131	0.01%	0.002%
18	4.571	1003	1005	1006	rBV	205	113	0.01%	0.001%
19	4.613	1006	1018	1046	rVV	76146	187484	19.09%	2.426%
20	4.909	1107	1110	1113	rBV2	319	238	0.02%	0.003%
21	5.057	1140	1156	1177	rBV	182732	395484	40.28%	5.118%
22	5.282	1223	1226	1229	rVB3	584	387	0.04%	0.005%
23	5.398	1259	1262	1264	rBV	212	109	0.01%	0.001%
24	5.430	1269	1272	1275	rVB	219	105	0.01%	0.001%
25	5.488	1288	1290	1291	rVB	144	34	0.00%	0.000%
26	5.501	1291	1294	1295	rBV	168	84	0.01%	0.001%
27	5.555	1307	1311	1314	rBV	273	195	0.02%	0.003%
28	5.594	1321	1323	1326	rVB	161	108	0.01%	0.001%
29	5.636	1334	1336	1338	rVB	161	83	0.01%	0.001%
30	5.719	1340	1362	1385	rBV3	354688	981956	100.00%	12.708%
31	5.902	1417	1419	1420	rBV	396	176	0.02%	0.002%
32	6.018	1452	1455	1456	rVB	247	86	0.01%	0.001%
33	6.099	1476	1480	1483	rBV2	341	312	0.03%	0.004%
34	6.115	1483	1485	1489	rVB2	229	138	0.01%	0.002%
35	6.140	1491	1493	1499	rBV	205	166	0.02%	0.002%
36	6.243	1512	1525	1547	rBV	310696	588960	59.98%	7.622%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
 Data File : VU053522.D
 Acq On : 03 Apr 2023 16:02
 Operator : JC/MD
 Sample : 02158-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 FB(20230328)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	6.472	1594	1596	1599	rBV	147	48	0.00%	0.001%
38	6.523	1602	1612	1625	rBV8	5114	10854	1.11%	0.140%
39	6.603	1635	1637	1644	rVB	184	147	0.01%	0.002%
40	6.684	1648	1662	1687	rBV	222158	437511	44.56%	5.662%
41	6.896	1715	1728	1730	rBV2	368	734	0.07%	0.009%
42	6.986	1753	1756	1758	rBV	448	280	0.03%	0.004%
43	7.108	1791	1794	1799	rVB	424	374	0.04%	0.005%
44	7.131	1799	1801	1802	rBV	252	107	0.01%	0.001%
45	7.166	1810	1812	1815	rBV	163	56	0.01%	0.001%
46	7.182	1815	1817	1821	rBV2	516	358	0.04%	0.005%
47	7.234	1830	1833	1835	rBV	235	178	0.02%	0.002%
48	7.243	1835	1836	1839	rVV	162	58	0.01%	0.001%
49	7.259	1839	1841	1842	rBV	147	46	0.00%	0.001%
50	7.285	1847	1849	1852	rVV2	253	189	0.02%	0.002%
51	7.301	1852	1854	1857	rVV	337	138	0.01%	0.002%
52	7.320	1857	1860	1863	rVV2	266	164	0.02%	0.002%
53	7.340	1864	1866	1869	rVV	227	107	0.01%	0.001%
54	7.478	1905	1909	1911	rBV2	236	160	0.02%	0.002%
55	7.562	1923	1935	1960	rBV	131543	233802	23.81%	3.026%
56	7.735	1986	1989	1993	rBV2	355	234	0.02%	0.003%
57	7.783	2000	2004	2006	rBV	308	223	0.02%	0.003%
58	7.893	2025	2038	2062	rBV	474845	828890	84.41%	10.727%
59	8.176	2114	2126	2139	rBV	91470	153776	15.66%	1.990%
60	8.291	2159	2162	2163	rBV	153	88	0.01%	0.001%
61	8.372	2183	2187	2191	rBV2	280	278	0.03%	0.004%
62	8.471	2207	2218	2227	rBV3	1570	2653	0.27%	0.034%
63	8.552	2236	2243	2248	rBV4	1344	1449	0.15%	0.019%
64	8.626	2254	2266	2301	rBV	243530	446468	45.47%	5.778%
65	8.790	2316	2317	2320	rBV2	262	106	0.01%	0.001%
66	8.902	2349	2352	2356	rVB2	353	253	0.03%	0.003%
67	8.973	2370	2374	2377	rVB2	281	195	0.02%	0.003%
68	8.996	2377	2381	2385	rBV	375	341	0.03%	0.004%
69	9.111	2416	2417	2418	rBV	131	34	0.00%	0.000%
70	9.134	2422	2424	2426	rVV	207	84	0.01%	0.001%
71	9.311	2476	2479	2481	rBV	249	163	0.02%	0.002%
72	9.414	2498	2511	2538	rBV	422045	718271	73.15%	9.296%
73	9.626	2574	2577	2578	rBV	211	108	0.01%	0.001%
74	9.690	2595	2597	2601	rBV2	344	251	0.03%	0.003%
75	9.751	2612	2616	2620	rBV2	286	301	0.03%	0.004%
76	9.918	2665	2668	2671	rBV2	298	215	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
 Data File : VU053522.D
 Acq On : 03 Apr 2023 16:02
 Operator : JC/MD
 Sample : 02158-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 FB(20230328)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

77	10.079	2716	2718	2722	rBV	219	179	0.02%	0.002%
78	10.275	2777	2779	2784	rVB	255	188	0.02%	0.002%
79	10.401	2815	2818	2823	rBV2	237	216	0.02%	0.003%
80	10.600	2876	2880	2883	rBV	258	207	0.02%	0.003%
81	10.639	2888	2892	2894	rBV	410	350	0.04%	0.005%
82	10.751	2914	2927	2942	rBV	321016	510846	52.02%	6.611%
83	10.835	2951	2953	2957	rBV2	368	191	0.02%	0.002%
84	10.928	2980	2982	2988	rVB	376	228	0.02%	0.003%
85	11.076	3024	3028	3031	rBV	293	247	0.03%	0.003%
86	11.320	3098	3104	3110	rBV2	1456	1933	0.20%	0.025%
87	11.385	3120	3124	3126	rBV2	304	271	0.03%	0.004%
88	11.809	3243	3256	3277	rBV	470805	766655	78.07%	9.922%
89	12.118	3349	3352	3356	rBV2	363	228	0.02%	0.003%
90	12.188	3361	3374	3394	rBV	492641	794809	80.94%	10.286%
91	13.243	3701	3702	3705	rVB	366	148	0.02%	0.002%
92	13.548	3795	3797	3801	rVB	595	326	0.03%	0.004%
93	14.015	3939	3942	3947	rBV2	595	547	0.06%	0.007%




Sum of corrected areas: 7727073

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053522.D
Acq On : 03 Apr 2023 16:02
Operator : JC/MD
Sample : 02158-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
FB(20230328)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

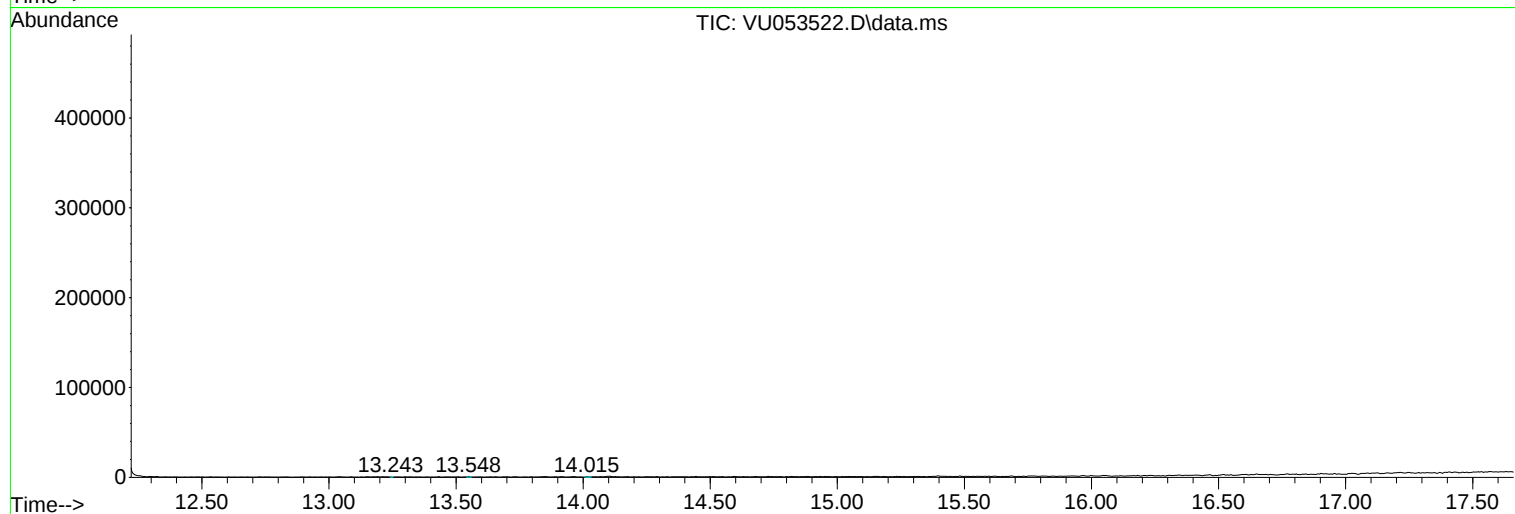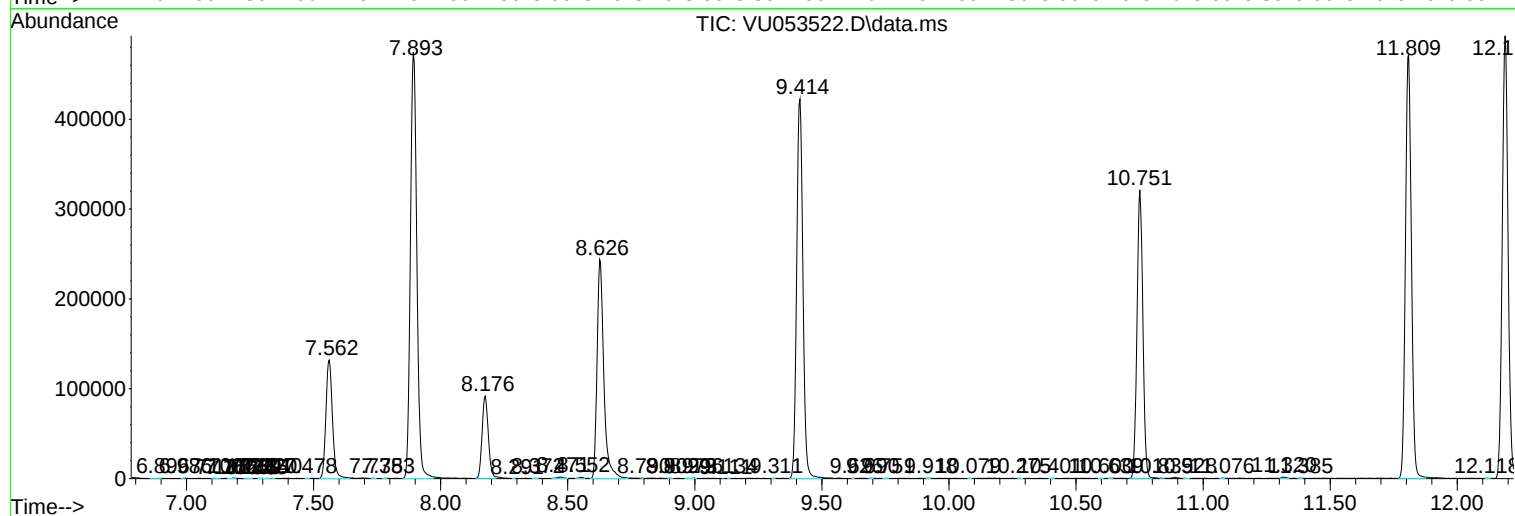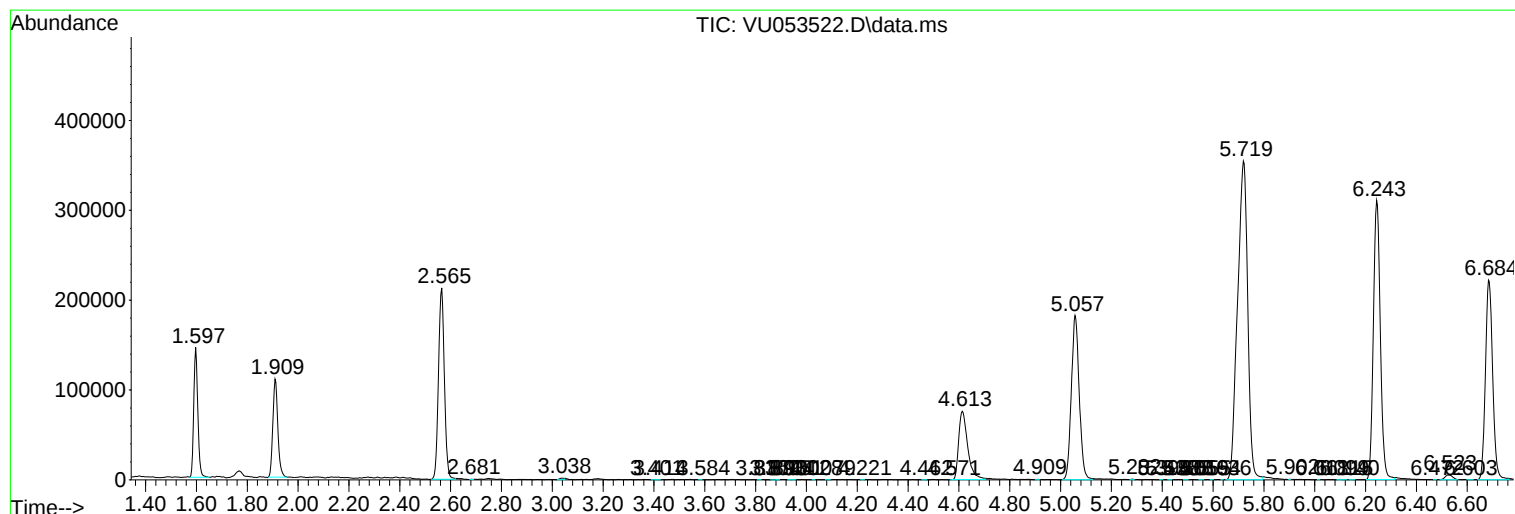

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053522.D
Acq On : 03 Apr 2023 16:02
Operator : JC/MD
Sample : 02158-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
FB(20230328)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053522.D
Acq On : 03 Apr 2023 16:02
Operator : JC/MD
Sample : 02158-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
FB(20230328)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------