

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
 Data File : VU053524.D
 Acq On : 03 Apr 2023 16:50
 Operator : JC/MD
 Sample : 02158-20
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 FB(20230330)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053524.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rVB	140531	156467	16.31%	2.103%
2	1.909	169	177	194	rVB	108464	147953	15.42%	1.989%
3	2.565	368	381	396	rBV	205113	331678	34.58%	4.458%
4	3.041	521	529	539	rBV3	1666	2911	0.30%	0.039%
5	3.176	562	571	573	rBV3	926	1274	0.13%	0.017%
6	3.385	628	636	640	rBV2	323	563	0.06%	0.008%
7	3.475	661	664	668	rVB2	270	209	0.02%	0.003%
8	3.552	680	688	691	rBV	249	320	0.03%	0.004%
9	3.825	769	773	776	rVV	221	139	0.01%	0.002%
10	3.941	806	809	811	rBV2	222	159	0.02%	0.002%
11	4.015	829	832	837	rVB	223	166	0.02%	0.002%
12	4.070	845	849	853	rVB2	189	161	0.02%	0.002%
13	4.279	912	914	917	rVB	370	208	0.02%	0.003%
14	4.407	952	954	957	rBV2	215	136	0.01%	0.002%
15	4.613	1006	1018	1041	rBV	79663	188386	19.64%	2.532%
16	4.944	1114	1121	1125	rBV2	470	520	0.05%	0.007%
17	4.967	1125	1128	1132	rVV2	377	306	0.03%	0.004%
18	5.057	1140	1156	1176	rBV	180371	395537	41.23%	5.316%
19	5.269	1220	1222	1225	rVV2	335	183	0.02%	0.002%
20	5.292	1225	1229	1231	rBV	297	208	0.02%	0.003%
21	5.324	1236	1239	1241	rBV2	266	200	0.02%	0.003%
22	5.385	1254	1258	1262	rBV	245	212	0.02%	0.003%
23	5.430	1270	1272	1275	rBV	233	174	0.02%	0.002%
24	5.581	1313	1319	1323	rBV2	269	238	0.02%	0.003%
25	5.626	1330	1333	1338	rVB	278	181	0.02%	0.002%
26	5.719	1340	1362	1384	rBV2	355826	959274	100.00%	12.893%
27	5.886	1411	1414	1420	rVB3	600	480	0.05%	0.006%
28	5.960	1434	1437	1439	rBV	198	140	0.01%	0.002%
29	6.112	1481	1484	1487	rVB2	500	333	0.03%	0.004%
30	6.134	1487	1491	1500	rBV	146	195	0.02%	0.003%
31	6.182	1503	1506	1509	rBV	197	168	0.02%	0.002%
32	6.243	1511	1525	1542	rBV	285211	540829	56.38%	7.269%
33	6.472	1594	1596	1599	rVB2	224	135	0.01%	0.002%
34	6.523	1602	1612	1624	rVB6	5347	10233	1.07%	0.138%
35	6.571	1624	1627	1629	rBV	357	166	0.02%	0.002%
36	6.587	1629	1632	1635	rBV3	385	310	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
 Data File : VU053524.D
 Acq On : 03 Apr 2023 16:50
 Operator : JC/MD
 Sample : 02158-20
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 FB(20230330)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	6.687	1648	1663	1685	rBV	219522	431029	44.93%	5.793%
38	6.957	1745	1747	1749	rVV	337	143	0.01%	0.002%
39	7.047	1772	1775	1779	rBV2	246	147	0.02%	0.002%
40	7.124	1795	1799	1802	rBV	234	234	0.02%	0.003%
41	7.185	1811	1818	1827	rBV2	551	905	0.09%	0.012%
42	7.259	1837	1841	1844	rBV	275	201	0.02%	0.003%
43	7.346	1865	1868	1872	rBV2	275	226	0.02%	0.003%
44	7.375	1875	1877	1881	rVB2	209	133	0.01%	0.002%
45	7.494	1911	1914	1918	rBV2	281	216	0.02%	0.003%
46	7.562	1919	1935	1958	rBV	130303	229392	23.91%	3.083%
47	7.700	1976	1978	1984	rVB2	366	334	0.03%	0.004%
48	7.822	2010	2016	2021	rBV2	226	238	0.02%	0.003%
49	7.893	2023	2038	2071	rBV	462125	805892	84.01%	10.832%
50	8.099	2100	2102	2105	rBV2	350	229	0.02%	0.003%
51	8.176	2113	2126	2143	rBV	87641	152188	15.86%	2.045%
52	8.292	2158	2162	2165	rBV	398	216	0.02%	0.003%
53	8.340	2174	2177	2180	rBV	194	152	0.02%	0.002%
54	8.472	2207	2218	2227	rBV4	1006	1850	0.19%	0.025%
55	8.517	2230	2232	2237	rVB2	408	319	0.03%	0.004%
56	8.546	2237	2241	2244	rBV2	873	782	0.08%	0.011%
57	8.626	2255	2266	2305	rBV	236992	432778	45.12%	5.817%
58	8.838	2330	2332	2336	rVV	174	143	0.01%	0.002%
59	8.928	2357	2360	2363	rBV	155	135	0.01%	0.002%
60	8.960	2367	2370	2376	rVB2	256	238	0.02%	0.003%
61	8.992	2376	2380	2386	rVB2	220	247	0.03%	0.003%
62	9.021	2386	2389	2391	rBV	244	176	0.02%	0.002%
63	9.256	2459	2462	2465	rBV	208	161	0.02%	0.002%
64	9.324	2480	2483	2484	rBV	257	166	0.02%	0.002%
65	9.414	2498	2511	2534	rBV	388683	652683	68.04%	8.772%
66	9.571	2556	2560	2564	rBV3	297	232	0.02%	0.003%
67	9.632	2570	2579	2581	rBV2	262	308	0.03%	0.004%
68	9.697	2595	2599	2601	rBV3	312	244	0.03%	0.003%
69	9.854	2643	2648	2650	rBV	258	191	0.02%	0.003%
70	9.970	2679	2684	2686	rBV2	218	207	0.02%	0.003%
71	10.005	2691	2695	2701	rBV2	293	400	0.04%	0.005%
72	10.054	2707	2710	2712	rBV	259	140	0.01%	0.002%
73	10.105	2722	2726	2729	rBV	278	219	0.02%	0.003%
74	10.333	2794	2797	2801	rVB2	246	186	0.02%	0.002%
75	10.391	2812	2815	2818	rBV2	239	177	0.02%	0.002%
76	10.488	2843	2845	2849	rVB	232	152	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
 Data File : VU053524.D
 Acq On : 03 Apr 2023 16:50
 Operator : JC/MD
 Sample : 02158-20
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 FB(20230330)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

77	10.545	2859	2863	2868	rBV2	300	341	0.04%	0.005%
78	10.600	2878	2880	2883	rVB	337	162	0.02%	0.002%
79	10.751	2913	2927	2946	rBV	314180	503664	52.50%	6.769%
80	10.886	2963	2969	2974	rBV3	1010	1098	0.11%	0.015%
81	10.996	3000	3003	3006	rBV	289	195	0.02%	0.003%
82	11.102	3034	3036	3041	rVB2	211	151	0.02%	0.002%
83	11.320	3100	3104	3113	rVB4	892	1037	0.11%	0.014%
84	11.623	3194	3198	3201	rBV	252	228	0.02%	0.003%
85	11.806	3243	3255	3280	rBV	430875	693942	72.34%	9.327%
86	12.188	3361	3374	3392	rBV	483363	780805	81.40%	10.494%
87	12.420	3444	3446	3451	rBV2	230	167	0.02%	0.002%
88	12.674	3522	3525	3528	rBV	307	171	0.02%	0.002%
89	12.693	3529	3531	3535	rVB2	298	166	0.02%	0.002%
90	12.716	3535	3538	3542	rBV	244	198	0.02%	0.003%
91	12.970	3614	3617	3621	rVB2	378	271	0.03%	0.004%
92	13.012	3626	3630	3635	rBV2	264	307	0.03%	0.004%
93	13.082	3648	3652	3655	rBV	474	360	0.04%	0.005%
94	13.163	3672	3677	3681	rBV2	325	417	0.04%	0.006%
95	13.214	3691	3693	3695	rBV	301	142	0.01%	0.002%
96	13.465	3769	3771	3776	rBV2	316	311	0.03%	0.004%
97	13.613	3815	3817	3820	rVB2	403	199	0.02%	0.003%
98	13.738	3853	3856	3858	rBV	340	185	0.02%	0.002%
99	13.851	3887	3891	3898	rBV4	605	767	0.08%	0.010%
100	14.301	4029	4031	4034	rBV	391	173	0.02%	0.002%




Sum of corrected areas: 7440218

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053524.D
Acq On : 03 Apr 2023 16:50
Operator : JC/MD
Sample : 02158-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
FB(20230330)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

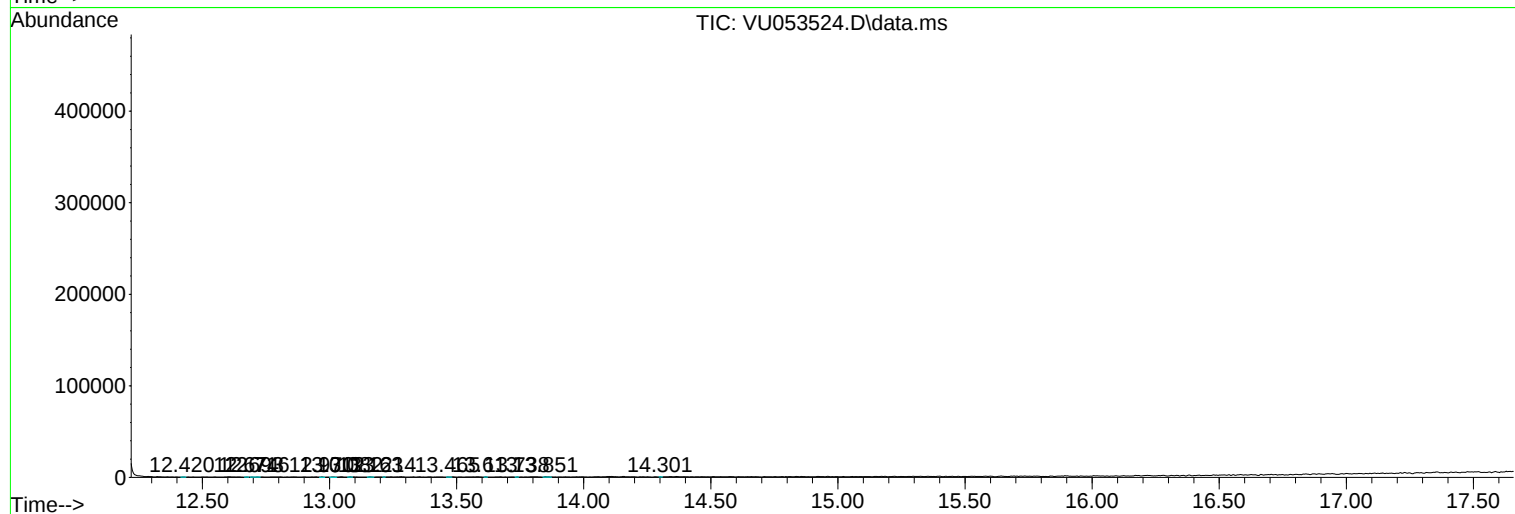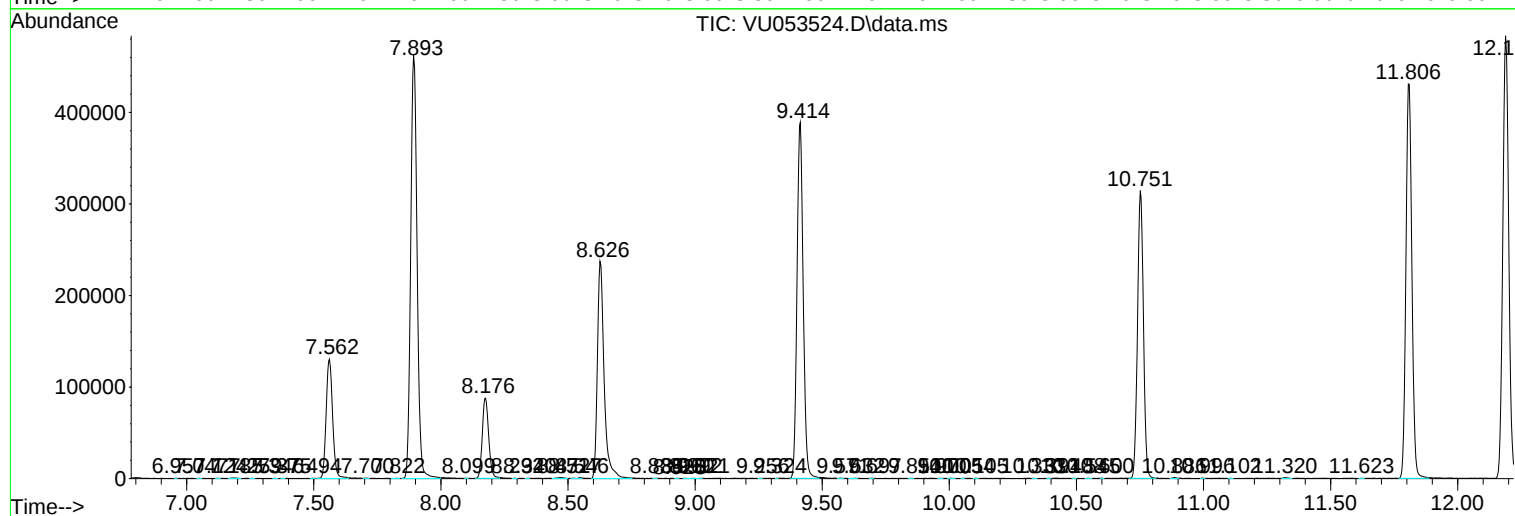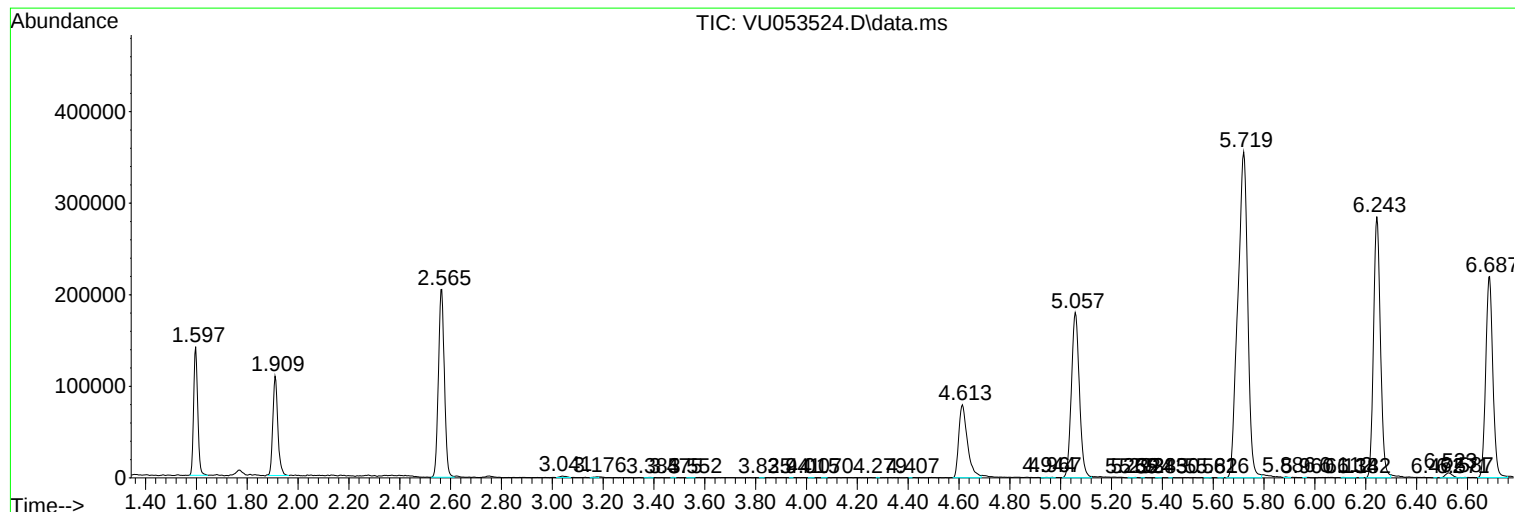

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053524.D
Acq On : 03 Apr 2023 16:50
Operator : JC/MD
Sample : 02158-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
FB(20230330)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053524.D
Acq On : 03 Apr 2023 16:50
Operator : JC/MD
Sample : 02158-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
FB(20230330)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------