

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
 Data File : VU053526.D
 Acq On : 03 Apr 2023 17:38
 Operator : JC/MD
 Sample : 02158-22
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EB(20230331)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053526.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rVB	131163	147116	16.00%	2.015%
2	1.909	169	177	195	rVB	100669	141311	15.37%	1.935%
3	2.562	369	380	394	rBV	186390	308260	33.52%	4.221%
4	3.041	522	529	537	rBV3	1365	2528	0.27%	0.035%
5	3.343	620	623	629	rBV2	336	444	0.05%	0.006%
6	3.440	651	653	657	rVB2	270	123	0.01%	0.002%
7	3.629	710	712	717	rBV	218	139	0.02%	0.002%
8	3.906	797	798	800	rBV	148	57	0.01%	0.001%
9	3.999	824	827	828	rBV	188	87	0.01%	0.001%
10	4.047	838	842	845	rVB	257	158	0.02%	0.002%
11	4.247	901	904	907	rBV	155	119	0.01%	0.002%
12	4.388	945	948	950	rBV	243	158	0.02%	0.002%
13	4.427	958	960	963	rBV	178	109	0.01%	0.001%
14	4.613	1006	1018	1050	rBV	77289	187913	20.44%	2.573%
15	4.960	1124	1126	1127	rBV	176	70	0.01%	0.001%
16	5.057	1140	1156	1174	rBV	170529	376242	40.92%	5.152%
17	5.382	1254	1257	1259	rVB	170	72	0.01%	0.001%
18	5.391	1259	1260	1263	rVB	145	35	0.00%	0.000%
19	5.407	1263	1265	1267	rBV	176	88	0.01%	0.001%
20	5.423	1267	1270	1272	rVV	218	100	0.01%	0.001%
21	5.472	1280	1285	1290	rBV2	278	299	0.03%	0.004%
22	5.504	1291	1295	1297	rBV	220	175	0.02%	0.002%
23	5.529	1301	1303	1305	rBV	171	88	0.01%	0.001%
24	5.626	1332	1333	1336	rBV	124	44	0.00%	0.001%
25	5.719	1341	1362	1385	rBV2	337258	919517	100.00%	12.592%
26	5.886	1412	1414	1415	rBV2	493	162	0.02%	0.002%
27	5.944	1430	1432	1437	rBV3	209	142	0.02%	0.002%
28	5.999	1446	1449	1451	rBV	205	113	0.01%	0.002%
29	6.031	1455	1459	1460	rBV2	353	247	0.03%	0.003%
30	6.131	1489	1490	1493	rBV	142	41	0.00%	0.001%
31	6.153	1494	1497	1502	rVB	315	245	0.03%	0.003%
32	6.243	1512	1525	1545	rBV	299097	573150	62.33%	7.849%
33	6.484	1597	1600	1601	rBV	167	74	0.01%	0.001%
34	6.529	1605	1614	1624	rVB6	4289	8356	0.91%	0.114%
35	6.684	1649	1662	1682	rBV	207177	404668	44.01%	5.541%
36	6.980	1752	1754	1755	rBV	178	81	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
 Data File : VU053526.D
 Acq On : 03 Apr 2023 17:38
 Operator : JC/MD
 Sample : 02158-22
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EB(20230331)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.021	1763	1767	1772	rBV2	335	267	0.03%	0.004%
38	7.082	1783	1786	1790	rBV	192	226	0.02%	0.003%
39	7.137	1798	1803	1807	rBV	360	383	0.04%	0.005%
40	7.160	1807	1810	1812	rBV2	274	192	0.02%	0.003%
41	7.246	1835	1837	1838	rBV2	168	77	0.01%	0.001%
42	7.269	1842	1844	1847	rBV	153	79	0.01%	0.001%
43	7.562	1922	1935	1960	rBV	123587	216862	23.58%	2.970%
44	7.726	1984	1986	1989	rBV	217	80	0.01%	0.001%
45	7.796	2005	2008	2009	rBV2	355	189	0.02%	0.003%
46	7.893	2025	2038	2064	rBV	437039	768538	83.58%	10.524%
47	8.176	2113	2126	2140	rBV	86799	144702	15.74%	1.982%
48	8.279	2155	2158	2161	rBV2	265	176	0.02%	0.002%
49	8.385	2189	2191	2197	rBV	136	94	0.01%	0.001%
50	8.410	2197	2199	2201	rBV	127	55	0.01%	0.001%
51	8.446	2208	2210	2213	rBV2	362	303	0.03%	0.004%
52	8.549	2239	2242	2243	rBV2	435	202	0.02%	0.003%
53	8.626	2255	2266	2301	rBV	235012	429399	46.70%	5.880%
54	8.835	2329	2331	2334	rBV2	199	115	0.01%	0.002%
55	8.870	2339	2342	2344	rVB	421	217	0.02%	0.003%
56	8.886	2344	2347	2349	rBV	186	97	0.01%	0.001%
57	8.899	2349	2351	2353	rBV	152	83	0.01%	0.001%
58	8.967	2369	2372	2377	rBV2	204	145	0.02%	0.002%
59	9.153	2426	2430	2431	rBV	145	97	0.01%	0.001%
60	9.414	2498	2511	2538	rBV	422475	689382	74.97%	9.440%
61	9.594	2565	2567	2568	rBV	122	30	0.00%	0.000%
62	9.619	2572	2575	2577	rBV	177	88	0.01%	0.001%
63	9.632	2577	2579	2581	rBV2	276	134	0.01%	0.002%
64	9.690	2594	2597	2600	rBV2	368	228	0.02%	0.003%
65	9.725	2605	2608	2610	rBV2	241	158	0.02%	0.002%
66	10.008	2693	2696	2698	rBV2	232	151	0.02%	0.002%
67	10.047	2706	2708	2711	rVB	284	133	0.01%	0.002%
68	10.124	2730	2732	2733	rBV	219	70	0.01%	0.001%
69	10.278	2777	2780	2782	rBV2	182	108	0.01%	0.001%
70	10.481	2841	2843	2846	rBV	223	91	0.01%	0.001%
71	10.677	2902	2904	2906	rBV	174	66	0.01%	0.001%
72	10.751	2914	2927	2949	rBV	302292	486898	52.95%	6.668%
73	10.889	2966	2970	2977	rVB2	576	688	0.07%	0.009%
74	11.205	3066	3068	3069	rBV2	216	85	0.01%	0.001%
75	11.314	3100	3102	3104	rBV2	169	95	0.01%	0.001%
76	11.758	3236	3240	3243	rBV2	307	260	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053526.D
Acq On : 03 Apr 2023 17:38
Operator : JC/MD
Sample : 02158-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EB(20230331)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M

Title : VOC Analysis

77	11.809	3243	3256	3279	rBV	470788	742823	80.78%	10.172%
78	12.188	3361	3374	3400	rBV	455401	745092	81.03%	10.203%
79	12.751	3547	3549	3552	rBV	214	86	0.01%	0.001%
80	12.954	3607	3612	3613	rBV	368	285	0.03%	0.004%
81	13.127	3664	3666	3670	rVB	497	241	0.03%	0.003%
82	13.548	3795	3797	3799	rBV	381	206	0.02%	0.003%


Sum of corrected areas: 7302507

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053526.D
Acq On : 03 Apr 2023 17:38
Operator : JC/MD
Sample : 02158-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EB(20230331)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

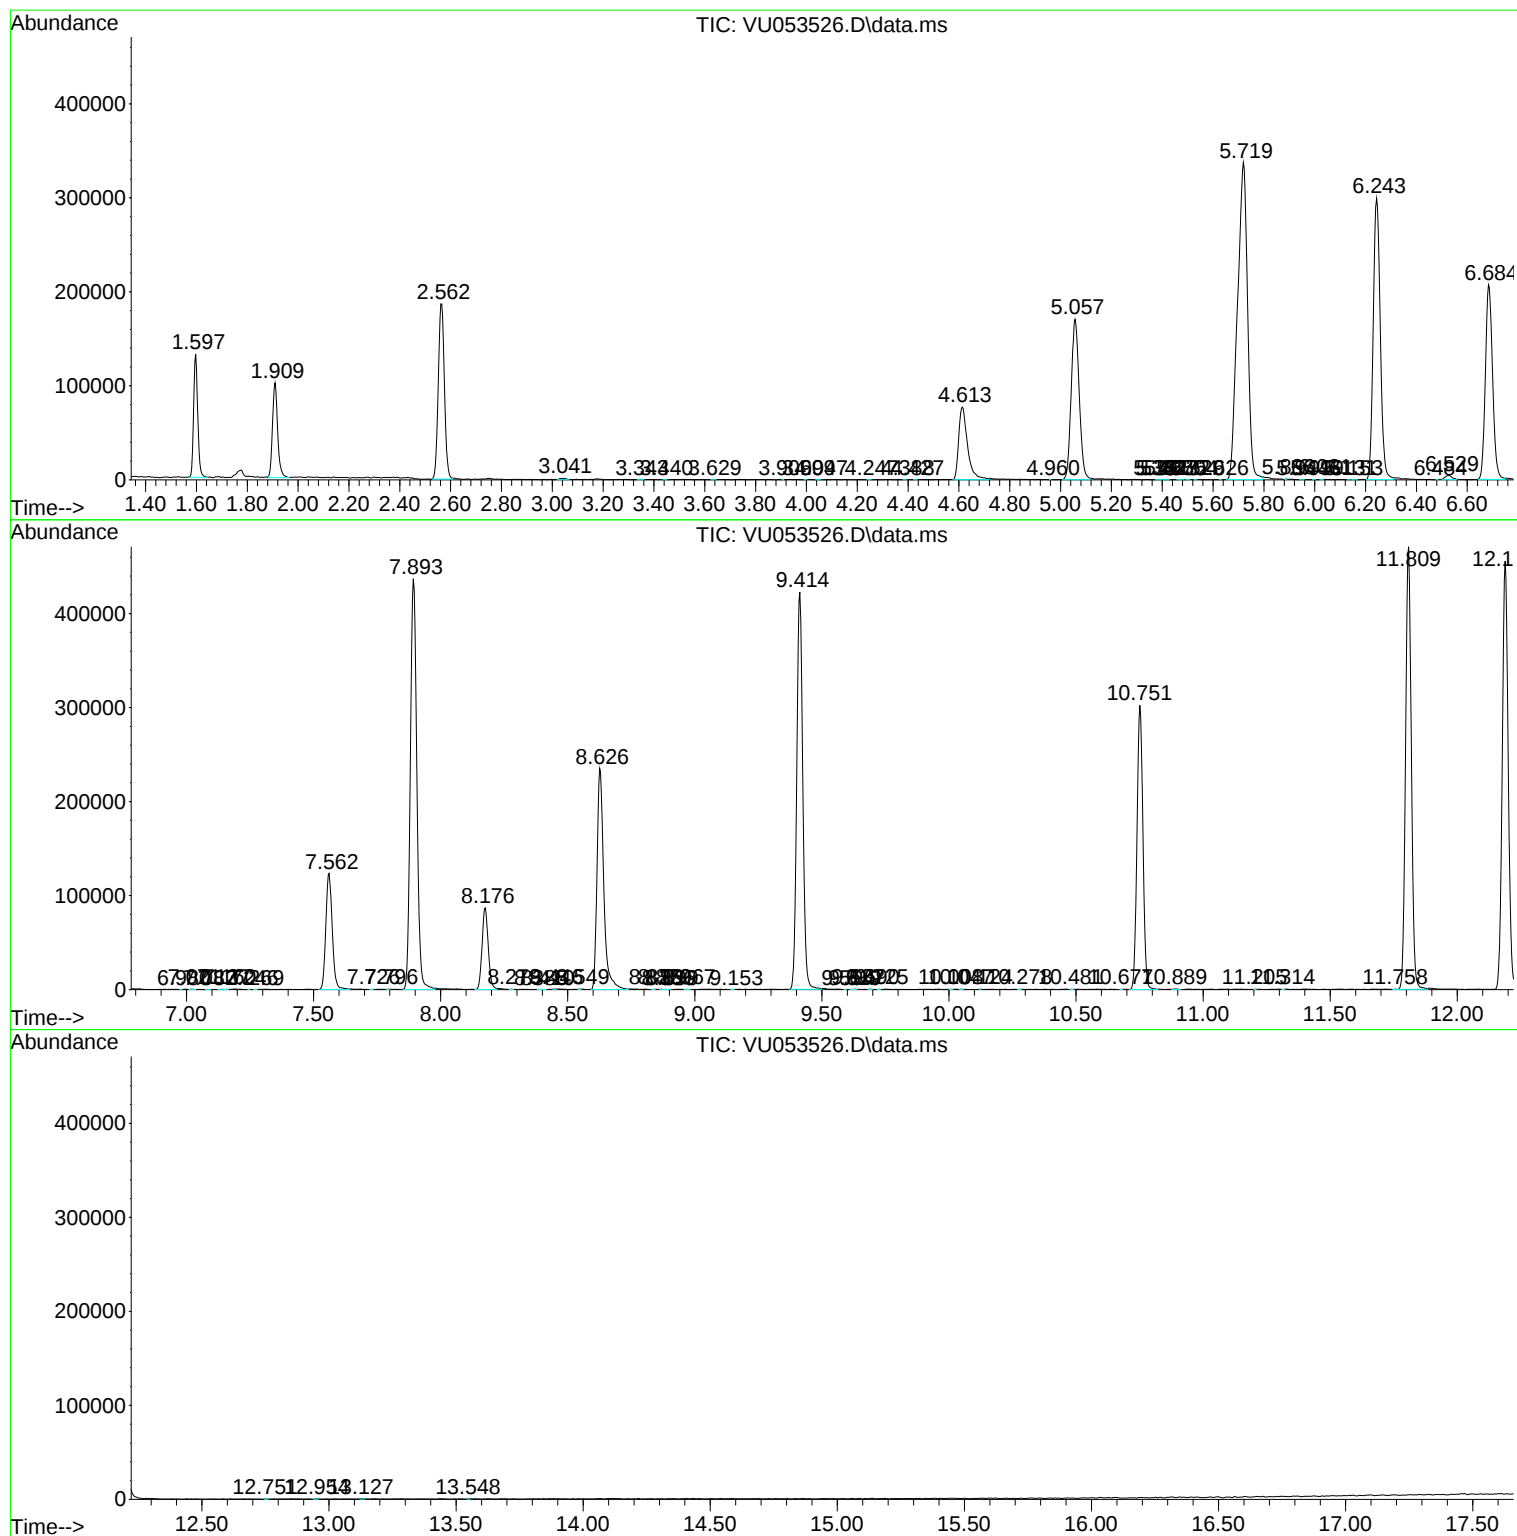

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053526.D
Acq On : 03 Apr 2023 17:38
Operator : JC/MD
Sample : 02158-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EB(20230331)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053526.D
Acq On : 03 Apr 2023 17:38
Operator : JC/MD
Sample : 02158-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EB(20230331)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------