

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
 Data File : VU053530.D
 Acq On : 03 Apr 2023 19:13
 Operator : JC/MD
 Sample : 02158-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-6(20230329)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053530.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rVB	153161	172281	2.62%	0.669%
2	1.909	170	177	193	rVB	115277	161182	2.45%	0.626%
3	2.565	369	381	397	rBV	216852	356256	5.42%	1.384%
4	2.819	457	460	462	rBV	523	303	0.00%	0.001%
5	2.974	505	508	510	rBV	338	235	0.00%	0.001%
6	3.533	679	682	685	rBV2	306	223	0.00%	0.001%
7	3.700	731	734	738	rVB	487	343	0.01%	0.001%
8	3.723	738	741	744	rBV2	242	190	0.00%	0.001%
9	3.893	789	794	797	rBV2	202	224	0.00%	0.001%
10	4.054	842	844	848	rBV2	372	256	0.00%	0.001%
11	4.134	865	869	874	rBV2	428	428	0.01%	0.002%
12	4.247	900	904	907	rVB2	407	277	0.00%	0.001%
13	4.273	907	912	913	rBV	234	207	0.00%	0.001%
14	4.369	935	942	945	rBV2	321	378	0.01%	0.001%
15	4.613	1005	1018	1022	rBV	82184	146816	2.24%	0.570%
16	4.909	1108	1110	1116	rVB5	547	517	0.01%	0.002%
17	5.057	1139	1156	1178	rBV	183427	406793	6.19%	1.580%
18	5.282	1223	1226	1229	rBV2	360	313	0.00%	0.001%
19	5.317	1233	1237	1239	rVB2	295	173	0.00%	0.001%
20	5.334	1239	1242	1245	rBV2	295	214	0.00%	0.001%
21	5.379	1254	1256	1260	rBV	338	274	0.00%	0.001%
22	5.449	1275	1278	1282	rBV	309	291	0.00%	0.001%
23	5.485	1286	1289	1291	rBV2	249	162	0.00%	0.001%
24	5.559	1310	1312	1318	rVB2	433	319	0.00%	0.001%
25	5.588	1318	1321	1325	rBV2	350	279	0.00%	0.001%
26	5.620	1328	1331	1334	rBV2	360	216	0.00%	0.001%
27	5.719	1341	1362	1397	rBV2	361760	1028370	15.66%	3.995%
28	5.964	1431	1438	1441	rBV4	478	481	0.01%	0.002%
29	6.128	1486	1489	1490	rBV	358	197	0.00%	0.001%
30	6.243	1511	1525	1549	rBV	312441	593856	9.04%	2.307%
31	6.449	1582	1589	1590	rBV2	317	388	0.01%	0.002%
32	6.539	1602	1617	1632	rBV2	63812	123883	1.89%	0.481%
33	6.684	1647	1662	1680	rBV2	222113	434328	6.61%	1.687%
34	6.890	1721	1726	1729	rBV2	373	253	0.00%	0.001%
35	6.967	1747	1750	1753	rBV	231	157	0.00%	0.001%
36	7.057	1773	1778	1780	rBV3	456	372	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
 Data File : VU053530.D
 Acq On : 03 Apr 2023 19:13
 Operator : JC/MD
 Sample : 02158-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-6(20230329)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.179	1811	1816	1822	rBV2	679	750	0.01%	0.003%
38	7.388	1876	1881	1888	rVB	203	251	0.00%	0.001%
39	7.430	1891	1894	1896	rBV	253	164	0.00%	0.001%
40	7.562	1919	1935	1962	rBV	134067	238127	3.63%	0.925%
41	7.687	1970	1974	1975	rBV2	427	278	0.00%	0.001%
42	7.796	2006	2008	2011	rVB	349	179	0.00%	0.001%
43	7.819	2011	2015	2018	rBV	258	177	0.00%	0.001%
44	7.893	2025	2038	2050	rVV	476295	815623	12.42%	3.168%
45	7.967	2051	2061	2088	rVB	487200	860859	13.11%	3.344%
46	8.176	2114	2126	2148	rVV	91139	158219	2.41%	0.615%
47	8.253	2148	2150	2152	rVB2	426	166	0.00%	0.001%
48	8.346	2176	2179	2182	rVV3	326	199	0.00%	0.001%
49	8.378	2185	2189	2193	rBV2	557	311	0.00%	0.001%
50	8.549	2229	2242	2256	rBV	429651	723402	11.01%	2.810%
51	8.626	2257	2266	2295	rVB	253798	462624	7.04%	1.797%
52	8.796	2315	2319	2322	rBV3	372	302	0.00%	0.001%
53	8.861	2332	2339	2341	rBV2	849	921	0.01%	0.004%
54	9.105	2410	2415	2417	rBV	203	196	0.00%	0.001%
55	9.198	2441	2444	2448	rVB	196	155	0.00%	0.001%
56	9.240	2455	2457	2459	rBV	312	163	0.00%	0.001%
57	9.285	2468	2471	2476	rVB	308	230	0.00%	0.001%
58	9.324	2479	2483	2484	rBV	276	203	0.00%	0.001%
59	9.443	2498	2520	2550	rVV2	2023023	4048236	61.64%	15.726%
60	9.568	2552	2559	2572	rVB	25494	41750	0.64%	0.162%
61	9.690	2586	2597	2612	rVB	87566	148553	2.26%	0.577%
62	9.883	2654	2657	2658	rBV	360	192	0.00%	0.001%
63	9.909	2661	2665	2667	rBV2	208	185	0.00%	0.001%
64	10.099	2712	2724	2736	rBV	26234	42537	0.65%	0.165%
65	10.247	2765	2770	2772	rVB2	444	336	0.01%	0.001%
66	10.292	2781	2784	2788	rVB2	225	164	0.00%	0.001%
67	10.484	2833	2844	2852	rBV2	3211	4483	0.07%	0.017%
68	10.661	2894	2899	2902	rBV2	558	428	0.01%	0.002%
69	10.751	2914	2927	2945	rBV	328508	516364	7.86%	2.006%
70	10.877	2963	2966	2967	rBV	678	356	0.01%	0.001%
71	10.996	2989	3003	3022	rBV	14927	33896	0.52%	0.132%
72	11.086	3025	3031	3043	rVB3	7792	11045	0.17%	0.043%
73	11.230	3068	3076	3083	rVV7	3449	5460	0.08%	0.021%
74	11.288	3086	3094	3108	rVB3	6476	9278	0.14%	0.036%
75	11.465	3139	3149	3164	rVB	22579	34357	0.52%	0.133%
76	11.520	3164	3166	3170	rBV2	322	168	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
 Data File : VU053530.D
 Acq On : 03 Apr 2023 19:13
 Operator : JC/MD
 Sample : 02158-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-6(20230329)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

77	11.552	3170	3176	3177	rBV2	530	437	0.01%	0.002%
78	11.613	3193	3195	3199	rVV2	265	162	0.00%	0.001%
79	11.742	3221	3235	3246	rBV	717727	1131703	17.23%	4.396%
80	11.832	3246	3263	3277	rVB2	2008649	3807585	57.98%	14.791%
81	12.089	3332	3343	3350	rBV10	7865	17166	0.26%	0.067%
82	12.192	3363	3375	3397	rVB2	563529	1233071	18.78%	4.790%
83	12.520	3476	3477	3483	rVB3	543	362	0.01%	0.001%
84	12.568	3483	3492	3500	rBV2	7526	10148	0.15%	0.039%
85	12.616	3503	3507	3511	rBV3	509	425	0.01%	0.002%
86	12.664	3519	3522	3523	rBV	592	302	0.00%	0.001%
87	12.877	3578	3588	3595	rBV7	2209	3528	0.05%	0.014%
88	12.970	3611	3617	3626	rVV4	4166	5599	0.09%	0.022%
89	13.021	3626	3633	3644	rVB2	7041	10867	0.17%	0.042%
90	13.185	3682	3684	3685	rBV	373	155	0.00%	0.001%
91	13.217	3687	3694	3703	rVB4	6877	10131	0.15%	0.039%
92	13.449	3758	3766	3777	rVB5	7836	12252	0.19%	0.048%
93	13.513	3783	3786	3788	rBV	424	320	0.00%	0.001%
94	13.594	3809	3811	3814	rBV	351	248	0.00%	0.001%
95	13.687	3835	3840	3847	rBV4	697	804	0.01%	0.003%
96	13.835	3872	3886	3912	rBV	4173033	6567612	100.00%	25.513%
97	14.082	3953	3963	3981	rVB	60100	97868	1.49%	0.380%
98	14.324	4026	4038	4057	rVB	765970	1234325	18.79%	4.795%
99	14.658	4139	4142	4144	rBV2	694	348	0.01%	0.001%
100	15.787	4488	4493	4503	rVB7	2772	4374	0.07%	0.017%




Sum of corrected areas: 25742514

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053530.D
Acq On : 03 Apr 2023 19:13
Operator : JC/MD
Sample : 02158-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-6(20230329)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

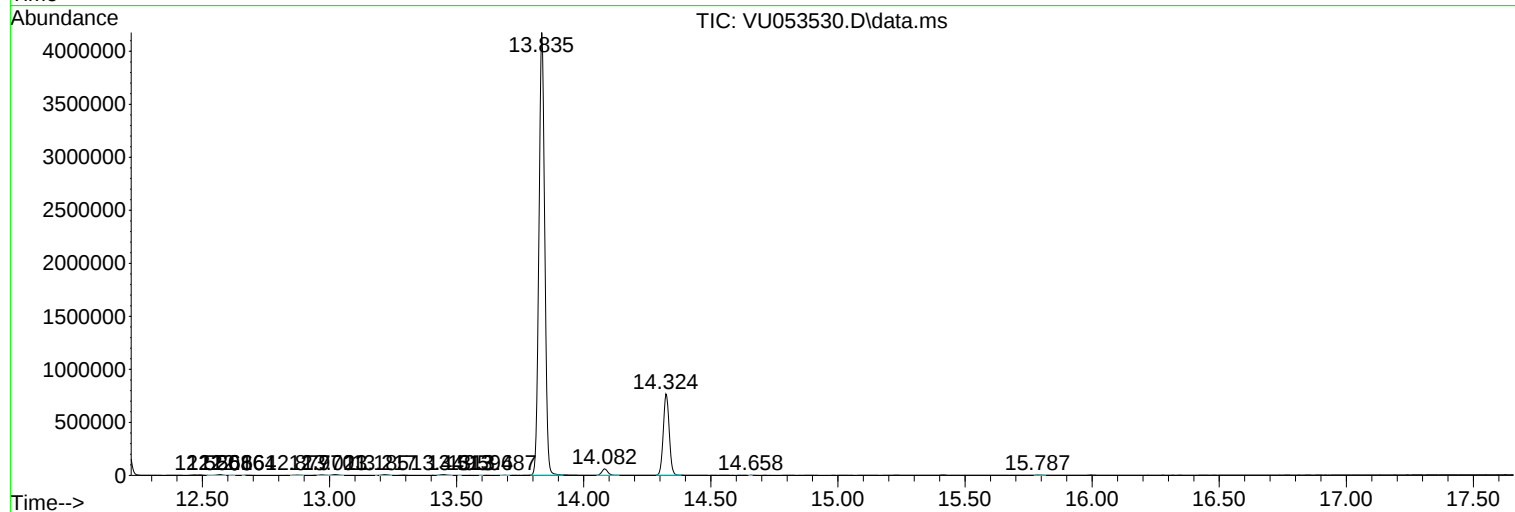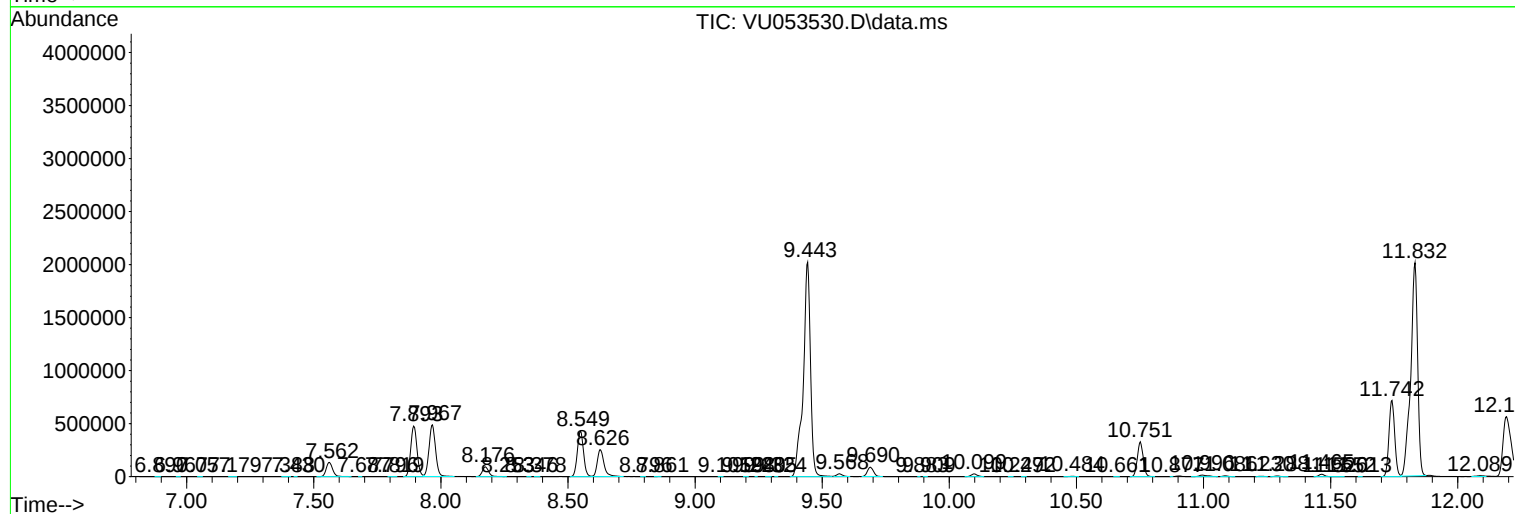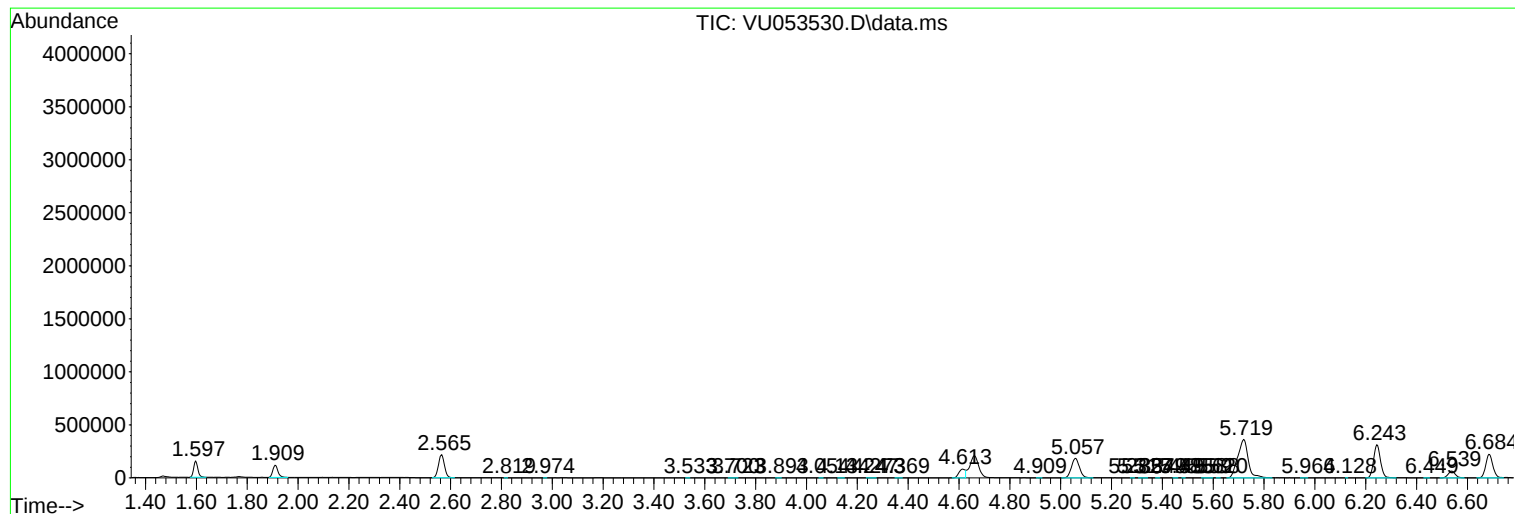

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053530.D
Acq On : 03 Apr 2023 19:13
Operator : JC/MD
Sample : 02158-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-6(20230329)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053530.D
Acq On : 03 Apr 2023 19:13
Operator : JC/MD
Sample : 02158-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-6(20230329)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------