

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
 Data File : VU053533.D
 Acq On : 03 Apr 2023 20:24
 Operator : JC/MD
 Sample : 02158-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-10(20230329)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053533.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	94	rBV	139859	154955	16.41%	1.867%
2	1.909	170	177	194	rVB	104113	143629	15.21%	1.731%
3	2.565	369	381	395	rBV	201230	325337	34.45%	3.921%
4	2.893	479	483	487	rBV4	429	435	0.05%	0.005%
5	3.083	539	542	547	rVB	333	222	0.02%	0.003%
6	3.115	547	552	554	rBV3	363	257	0.03%	0.003%
7	3.144	558	561	562	rBV	409	274	0.03%	0.003%
8	3.276	599	602	607	rVB	167	158	0.02%	0.002%
9	3.407	637	643	645	rBV2	267	221	0.02%	0.003%
10	3.546	683	686	689	rBV3	278	193	0.02%	0.002%
11	3.732	742	744	750	rVB	214	193	0.02%	0.002%
12	3.867	770	786	801	rBV2	15458	35243	3.73%	0.425%
13	3.996	814	826	837	rVV4	2719	6331	0.67%	0.076%
14	4.041	837	840	844	rVB2	251	193	0.02%	0.002%
15	4.173	878	881	884	rBV	277	179	0.02%	0.002%
16	4.272	908	912	915	rBV2	207	156	0.02%	0.002%
17	4.446	963	966	970	rBV2	245	202	0.02%	0.002%
18	4.533	989	993	997	rBV2	303	255	0.03%	0.003%
19	4.613	1004	1018	1050	rBV	78703	227851	24.13%	2.746%
20	4.983	1128	1133	1136	rBV2	285	214	0.02%	0.003%
21	5.057	1140	1156	1179	rBV	169843	387052	40.99%	4.664%
22	5.282	1223	1226	1228	rBV2	276	185	0.02%	0.002%
23	5.398	1260	1262	1266	rVB2	256	191	0.02%	0.002%
24	5.443	1271	1276	1278	rVB	332	272	0.03%	0.003%
25	5.719	1340	1362	1387	rBV2	345608	944354	100.00%	11.380%
26	5.951	1429	1434	1437	rBV2	304	286	0.03%	0.003%
27	6.002	1447	1450	1454	rVB2	245	199	0.02%	0.002%
28	6.031	1457	1459	1464	rBV	367	349	0.04%	0.004%
29	6.118	1481	1486	1489	rBV2	271	260	0.03%	0.003%
30	6.243	1510	1525	1545	rBV	310513	588436	62.31%	7.091%
31	6.539	1602	1617	1628	rVB5	8953	18099	1.92%	0.218%
32	6.684	1648	1662	1682	rBV	213726	418748	44.34%	5.046%
33	6.845	1708	1712	1713	rBV	303	161	0.02%	0.002%
34	6.909	1727	1732	1736	rBV2	150	183	0.02%	0.002%
35	6.957	1737	1747	1759	rBV3	6886	13181	1.40%	0.159%
36	7.050	1771	1776	1779	rVV2	241	272	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
 Data File : VU053533.D
 Acq On : 03 Apr 2023 20:24
 Operator : JC/MD
 Sample : 02158-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-10(20230329)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.137	1800	1803	1807	rBV	183	150	0.02%	0.002%
38	7.156	1807	1809	1812	rBV	240	176	0.02%	0.002%
39	7.298	1850	1853	1856	rBV2	258	217	0.02%	0.003%
40	7.414	1886	1889	1895	rVB2	191	173	0.02%	0.002%
41	7.562	1922	1935	1952	rBV	125922	221198	23.42%	2.666%
42	7.648	1959	1962	1966	rBV3	438	306	0.03%	0.004%
43	7.780	2000	2003	2007	rBV2	236	218	0.02%	0.003%
44	7.893	2023	2038	2053	rBV	449329	775040	82.07%	9.340%
45	8.121	2104	2109	2113	rBV2	270	262	0.03%	0.003%
46	8.176	2114	2126	2146	rBV	87041	149422	15.82%	1.801%
47	8.301	2163	2165	2169	rVB2	244	185	0.02%	0.002%
48	8.327	2169	2173	2176	rBV2	261	262	0.03%	0.003%
49	8.369	2183	2186	2191	rVB2	258	198	0.02%	0.002%
50	8.394	2191	2194	2198	rBV2	199	193	0.02%	0.002%
51	8.455	2210	2213	2215	rBV2	623	429	0.05%	0.005%
52	8.549	2231	2242	2255	rBV	43028	72381	7.66%	0.872%
53	8.626	2255	2266	2303	rVV	234554	429402	45.47%	5.175%
54	8.954	2366	2368	2374	rBV2	170	174	0.02%	0.002%
55	9.108	2412	2416	2418	rBV	266	210	0.02%	0.003%
56	9.311	2476	2479	2483	rBV2	257	217	0.02%	0.003%
57	9.414	2494	2511	2536	rBV	427210	724218	76.69%	8.728%
58	9.568	2554	2559	2567	rVB3	1714	2025	0.21%	0.024%
59	9.690	2588	2597	2610	rBV3	6772	10833	1.15%	0.131%
60	9.835	2639	2642	2645	rBV	261	171	0.02%	0.002%
61	9.995	2688	2692	2694	rBV2	272	205	0.02%	0.002%
62	10.102	2717	2725	2736	rVB7	2140	3042	0.32%	0.037%
63	10.266	2773	2776	2779	rVV	289	196	0.02%	0.002%
64	10.291	2781	2784	2787	rVB	265	163	0.02%	0.002%
65	10.404	2815	2819	2822	rBV2	340	244	0.03%	0.003%
66	10.507	2848	2851	2859	rVB	345	281	0.03%	0.003%
67	10.674	2899	2903	2905	rVV	272	191	0.02%	0.002%
68	10.751	2915	2927	2946	rBV	315524	504423	53.41%	6.079%
69	10.883	2963	2968	2973	rBV	603	775	0.08%	0.009%
70	10.999	2996	3004	3005	rBV2	685	561	0.06%	0.007%
71	11.089	3026	3032	3036	rBV2	650	749	0.08%	0.009%
72	11.465	3141	3149	3158	rBV2	1365	2149	0.23%	0.026%
73	11.529	3167	3169	3173	rVB	302	150	0.02%	0.002%
74	11.745	3227	3236	3244	rBV4	7221	10802	1.14%	0.130%
75	11.809	3244	3256	3278	rVV	484464	810006	85.77%	9.761%
76	12.085	3339	3342	3345	rBV2	377	323	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
 Data File : VU053533.D
 Acq On : 03 Apr 2023 20:24
 Operator : JC/MD
 Sample : 02158-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-10(20230329)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

77	12.188	3361	3374	3398	rVV	463078	766891	81.21%	9.242%
78	12.307	3409	3411	3413	rBV	343	197	0.02%	0.002%
79	12.436	3449	3451	3457	rVB	271	185	0.02%	0.002%
80	12.465	3457	3460	3461	rBV	321	209	0.02%	0.003%
81	12.571	3491	3493	3501	rVB2	831	824	0.09%	0.010%
82	12.616	3504	3507	3511	rVB2	428	311	0.03%	0.004%
83	12.655	3516	3519	3523	rBV	234	233	0.02%	0.003%
84	12.709	3532	3536	3538	rBV2	356	221	0.02%	0.003%
85	12.802	3563	3565	3569	rBV	322	207	0.02%	0.002%
86	12.825	3569	3572	3576	rVV	377	309	0.03%	0.004%
87	12.941	3604	3608	3614	rVB3	502	589	0.06%	0.007%
88	13.220	3690	3695	3698	rBV3	610	566	0.06%	0.007%
89	13.323	3722	3727	3731	rBV2	430	478	0.05%	0.006%
90	13.452	3763	3767	3772	rBV3	472	440	0.05%	0.005%
91	13.529	3788	3791	3794	rBV2	336	258	0.03%	0.003%
92	13.581	3803	3807	3815	rBV5	2772	2991	0.32%	0.036%
93	13.693	3840	3842	3845	rBV2	351	209	0.02%	0.003%
94	13.835	3875	3886	3908	rBV	272604	445868	47.21%	5.373%
95	14.040	3945	3950	3954	rBV5	1909	2304	0.24%	0.028%
96	14.188	3986	3996	4005	rBV5	4361	7241	0.77%	0.087%
97	14.327	4029	4039	4056	rVB3	44642	74897	7.93%	0.903%
98	14.741	4165	4168	4170	rBV2	646	394	0.04%	0.005%
99	15.269	4328	4332	4335	rBV3	573	484	0.05%	0.006%
100	15.462	4389	4392	4396	rVB4	925	684	0.07%	0.008%


Sum of corrected areas: 8298036

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053533.D
Acq On : 03 Apr 2023 20:24
Operator : JC/MD
Sample : 02158-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-10(20230329)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

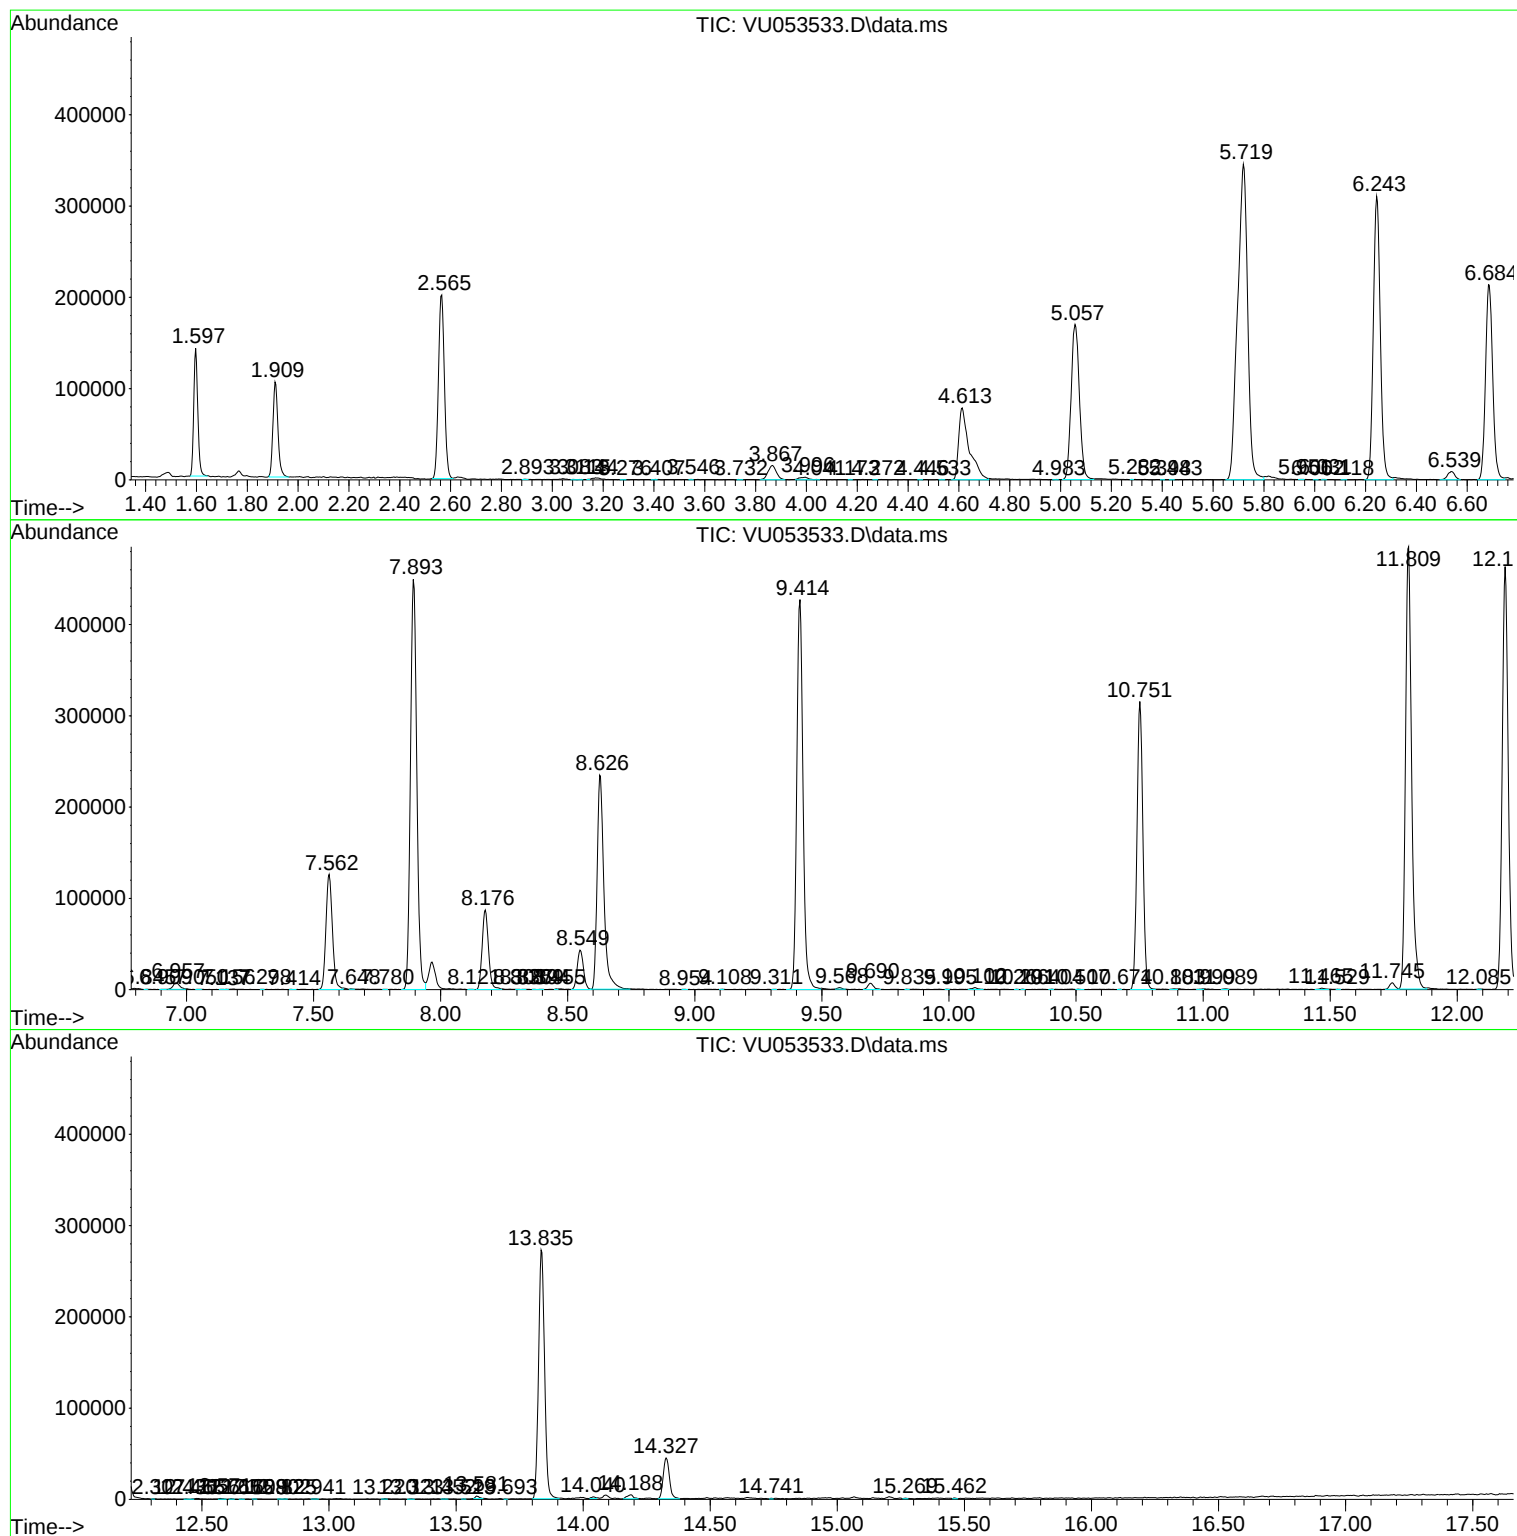

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053533.D
Acq On : 03 Apr 2023 20:24
Operator : JC/MD
Sample : 02158-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-10(20230329)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053533.D
Acq On : 03 Apr 2023 20:24
Operator : JC/MD
Sample : 02158-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-10(20230329)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------