

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
 Data File : VU053538.D
 Acq On : 03 Apr 2023 23:09
 Operator : JC/MD
 Sample : 02158-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-7S(20230329)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053538.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rVB	140569	158028	4.78%	1.430%
2	1.909	169	177	196	rVB	104470	144061	4.36%	1.303%
3	2.565	369	381	395	rBV	203006	329175	9.95%	2.978%
4	2.710	424	426	429	rBV2	301	164	0.00%	0.001%
5	2.842	464	467	470	rBV2	351	243	0.01%	0.002%
6	3.044	522	530	537	rVB3	1239	1865	0.06%	0.017%
7	3.169	565	569	573	rBV4	772	785	0.02%	0.007%
8	3.253	593	595	597	rBV2	205	136	0.00%	0.001%
9	3.353	614	626	642	rVB2	19787	39757	1.20%	0.360%
10	3.562	685	691	693	rBV2	270	245	0.01%	0.002%
11	3.864	771	785	804	rVB	24527	54470	1.65%	0.493%
12	3.977	815	820	821	rBV2	1036	659	0.02%	0.006%
13	4.038	837	839	843	rBV	192	136	0.00%	0.001%
14	4.060	843	846	848	rVV	209	155	0.00%	0.001%
15	4.115	859	863	868	rVB2	202	177	0.01%	0.002%
16	4.144	869	872	876	rVB2	296	220	0.01%	0.002%
17	4.224	891	897	901	rVB2	282	255	0.01%	0.002%
18	4.247	901	904	906	rBV	279	152	0.00%	0.001%
19	4.613	1006	1018	1023	rBV	80488	150432	4.55%	1.361%
20	4.841	1087	1089	1091	rBV3	397	192	0.01%	0.002%
21	5.057	1140	1156	1178	rBV	178360	381363	11.53%	3.450%
22	5.304	1231	1233	1236	rVB	292	142	0.00%	0.001%
23	5.375	1252	1255	1256	rBV	332	176	0.01%	0.002%
24	5.456	1276	1280	1284	rBV2	276	236	0.01%	0.002%
25	5.504	1292	1295	1298	rVB	300	192	0.01%	0.002%
26	5.530	1298	1303	1304	rVB2	267	212	0.01%	0.002%
27	5.610	1325	1328	1332	rVB	265	214	0.01%	0.002%
28	5.642	1332	1338	1339	rBV2	322	249	0.01%	0.002%
29	5.719	1341	1362	1390	rBV2	341132	957373	28.95%	8.662%
30	5.928	1423	1427	1432	rBV3	312	347	0.01%	0.003%
31	5.964	1436	1438	1443	rBV2	303	257	0.01%	0.002%
32	6.108	1480	1483	1486	rVV2	416	276	0.01%	0.002%
33	6.243	1508	1525	1543	rBV2	308344	575296	17.40%	5.205%
34	6.526	1604	1613	1615	rBV6	5322	6260	0.19%	0.057%
35	6.684	1649	1662	1679	rBV	209055	410076	12.40%	3.710%
36	6.960	1741	1748	1755	rBV3	1446	2194	0.07%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
 Data File : VU053538.D
 Acq On : 03 Apr 2023 23:09
 Operator : JC/MD
 Sample : 02158-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-7S(20230329)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.034	1768	1771	1774	rVB2	252	199	0.01%	0.002%
38	7.201	1822	1823	1826	rVB2	292	152	0.00%	0.001%
39	7.288	1847	1850	1855	rVB	218	163	0.00%	0.001%
40	7.330	1861	1863	1866	rVB	327	152	0.00%	0.001%
41	7.353	1866	1870	1874	rBV2	309	258	0.01%	0.002%
42	7.507	1915	1918	1922	rBV	314	252	0.01%	0.002%
43	7.562	1922	1935	1949	rBV	122365	213913	6.47%	1.935%
44	7.806	2005	2011	2012	rBV	316	281	0.01%	0.003%
45	7.893	2025	2038	2054	rBV	441538	771206	23.32%	6.977%
46	8.176	2115	2126	2142	rBV	84677	144486	4.37%	1.307%
47	8.398	2192	2195	2199	rVV2	197	175	0.01%	0.002%
48	8.459	2212	2214	2215	rBV	336	178	0.01%	0.002%
49	8.549	2232	2242	2252	rVB3	11719	19283	0.58%	0.174%
50	8.626	2252	2266	2296	rBV	236103	435776	13.18%	3.943%
51	8.925	2357	2359	2362	rVB	389	186	0.01%	0.002%
52	8.947	2363	2366	2373	rVB2	258	215	0.01%	0.002%
53	9.031	2388	2392	2394	rBV	167	148	0.00%	0.001%
54	9.047	2394	2397	2400	rVV2	353	244	0.01%	0.002%
55	9.160	2427	2432	2435	rVB2	246	207	0.01%	0.002%
56	9.201	2441	2445	2450	rBV2	233	191	0.01%	0.002%
57	9.230	2452	2454	2457	rVV	217	136	0.00%	0.001%
58	9.414	2497	2511	2544	rBV2	416120	951081	28.76%	8.605%
59	9.568	2553	2559	2570	rVB7	2021	3134	0.09%	0.028%
60	9.642	2578	2582	2583	rBV2	237	169	0.01%	0.002%
61	9.693	2587	2598	2606	rBV2	2964	4450	0.13%	0.040%
62	9.745	2611	2614	2619	rVB	307	221	0.01%	0.002%
63	10.098	2722	2724	2726	rBV2	832	406	0.01%	0.004%
64	10.481	2834	2843	2854	rBV4	1370	2251	0.07%	0.020%
65	10.539	2858	2861	2864	rBV2	220	198	0.01%	0.002%
66	10.706	2910	2913	2915	rBV	307	186	0.01%	0.002%
67	10.751	2915	2927	2943	rVV	307616	493569	14.93%	4.466%
68	10.857	2958	2960	2964	rVB	293	160	0.00%	0.001%
69	10.877	2964	2966	2970	rBV2	290	229	0.01%	0.002%
70	11.089	3028	3032	3041	rVB3	1037	1219	0.04%	0.011%
71	11.250	3077	3082	3083	rBV	248	198	0.01%	0.002%
72	11.372	3115	3120	3123	rVB	426	342	0.01%	0.003%
73	11.417	3123	3134	3144	rBV	45800	70125	2.12%	0.634%
74	11.578	3181	3184	3187	rBV	261	147	0.00%	0.001%
75	11.661	3208	3210	3219	rVB	346	286	0.01%	0.003%
76	11.741	3223	3235	3245	rBV	294935	462301	13.98%	4.183%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
 Data File : VU053538.D
 Acq On : 03 Apr 2023 23:09
 Operator : JC/MD
 Sample : 02158-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-7S(20230329)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

77	11.832	3245	3263	3289	rVB2	1651297	3306817	100.00%	29.918%
78	12.053	3329	3332	3334	rBV2	334	196	0.01%	0.002%
79	12.188	3361	3374	3399	rBV	484322	812920	24.58%	7.355%
80	12.413	3441	3444	3449	rVV2	203	160	0.00%	0.001%
81	12.577	3493	3495	3497	rBV	341	164	0.00%	0.001%
82	12.651	3515	3518	3523	rBV2	245	217	0.01%	0.002%
83	12.684	3525	3528	3532	rVB	332	203	0.01%	0.002%
84	12.828	3569	3573	3576	rBV2	367	408	0.01%	0.004%
85	12.986	3619	3622	3625	rBV2	381	265	0.01%	0.002%
86	13.021	3629	3633	3638	rVB2	382	302	0.01%	0.003%
87	13.127	3663	3666	3668	rBV	355	233	0.01%	0.002%
88	13.221	3690	3695	3703	rVB4	2304	3189	0.10%	0.029%
89	13.269	3708	3710	3712	rBV	330	222	0.01%	0.002%
90	13.375	3741	3743	3746	rBV	363	211	0.01%	0.002%
91	13.475	3772	3774	3777	rBV2	345	190	0.01%	0.002%
92	13.516	3784	3787	3789	rVB2	254	146	0.00%	0.001%
93	13.568	3800	3803	3805	rBV2	363	251	0.01%	0.002%
94	13.655	3827	3830	3835	rVB2	399	279	0.01%	0.003%
95	13.680	3835	3838	3839	rBV	395	224	0.01%	0.002%
96	13.761	3861	3863	3870	rVB2	433	345	0.01%	0.003%
97	13.838	3870	3887	3906	rBV	63600	104951	3.17%	0.950%
98	14.089	3958	3965	3976	rBV2	5753	8699	0.26%	0.079%
99	14.227	4006	4008	4012	rBV2	432	296	0.01%	0.003%
100	14.330	4031	4040	4048	rBV3	12304	17252	0.52%	0.156%




Sum of corrected areas: 11052783

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053538.D
Acq On : 03 Apr 2023 23:09
Operator : JC/MD
Sample : 02158-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-7S(20230329)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

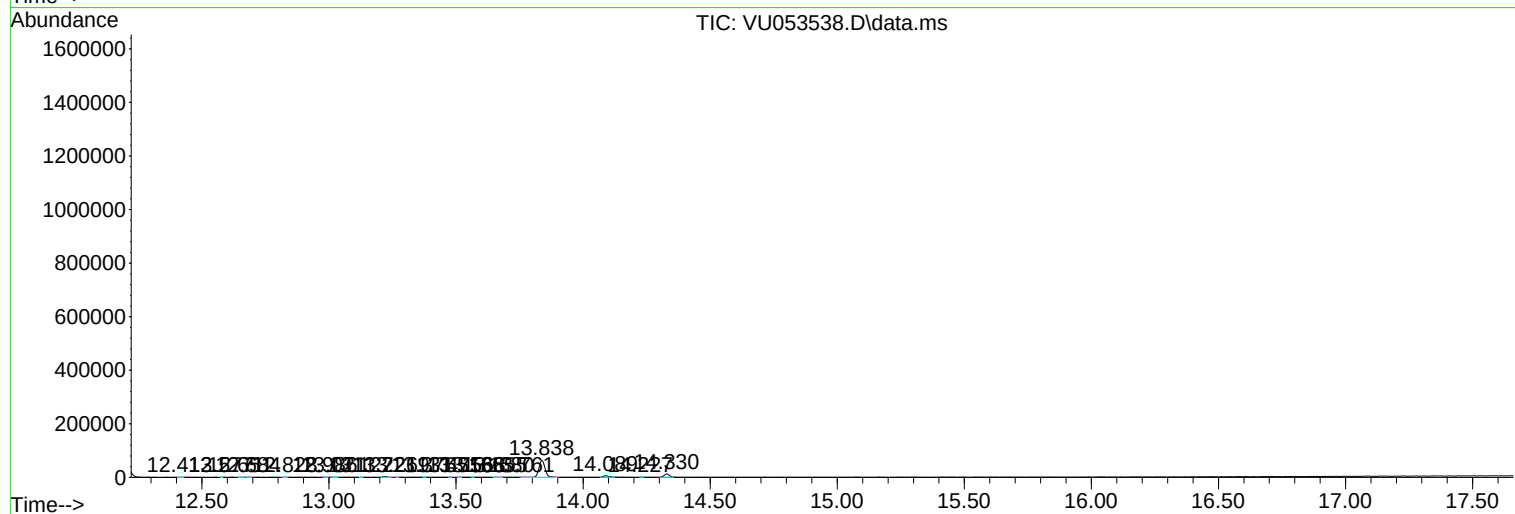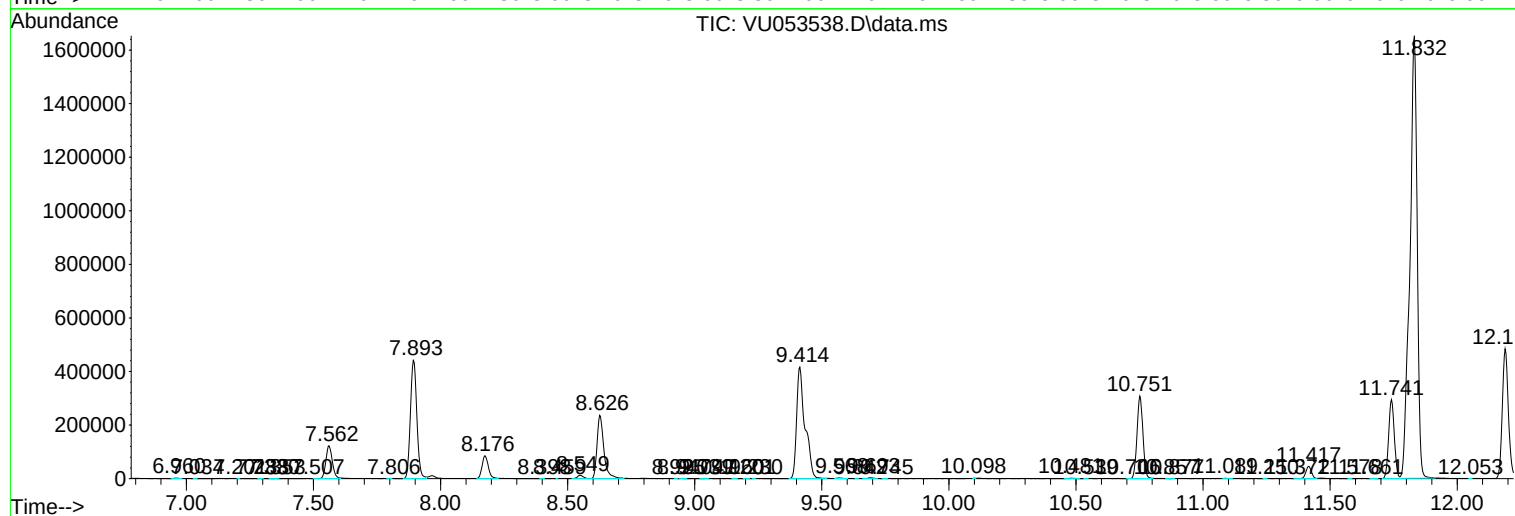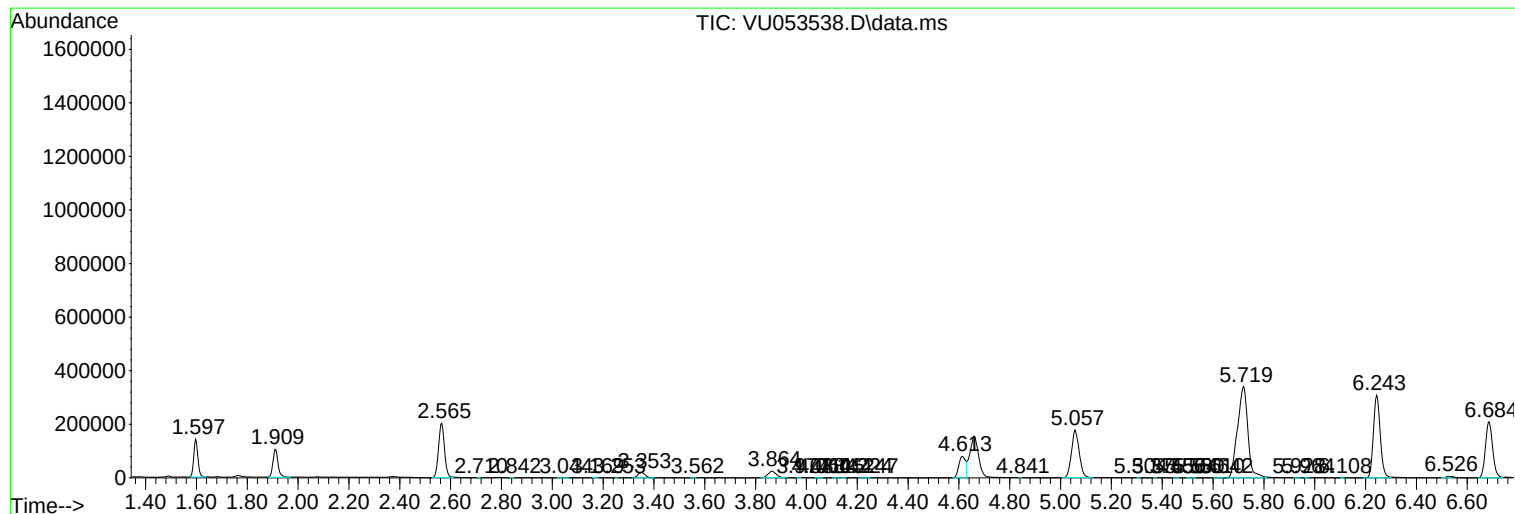

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053538.D
Acq On : 03 Apr 2023 23:09
Operator : JC/MD
Sample : 02158-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-7S(20230329)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053538.D
Acq On : 03 Apr 2023 23:09
Operator : JC/MD
Sample : 02158-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-7S(20230329)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------