

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
 Data File : VU053539.D
 Acq On : 03 Apr 2023 23:33
 Operator : JC/MD
 Sample : 02158-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-7D(20230329)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053539.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	94	rVB	143139	160648	3.06%	1.218%
2	1.909	169	177	195	rVB	106525	146853	2.80%	1.113%
3	2.562	369	380	394	rBV	201673	333630	6.36%	2.530%
4	2.723	427	430	432	rBV2	417	298	0.01%	0.002%
5	2.851	468	470	473	rVB	478	241	0.00%	0.002%
6	2.871	473	476	478	rBV2	373	245	0.00%	0.002%
7	2.967	503	506	509	rBV2	360	286	0.01%	0.002%
8	3.038	523	528	530	rBV2	981	992	0.02%	0.008%
9	3.350	614	625	641	rBV3	27366	53865	1.03%	0.408%
10	3.475	661	664	670	rBV2	408	390	0.01%	0.003%
11	3.861	766	784	804	rBV2	33295	82554	1.57%	0.626%
12	3.993	815	825	837	rVV6	2286	5265	0.10%	0.040%
13	4.054	841	844	847	rVB	204	136	0.00%	0.001%
14	4.109	858	861	862	rVB	150	59	0.00%	0.000%
15	4.211	890	893	895	rBV	177	86	0.00%	0.001%
16	4.305	919	922	923	rBV2	271	153	0.00%	0.001%
17	4.613	1006	1018	1022	rBV	80311	143345	2.73%	1.087%
18	5.057	1140	1156	1177	rBV	177611	387723	7.39%	2.940%
19	5.292	1226	1229	1231	rBV2	361	174	0.00%	0.001%
20	5.372	1253	1254	1260	rVB	566	325	0.01%	0.002%
21	5.719	1341	1362	1395	rBV2	345875	983419	18.74%	7.456%
22	5.925	1424	1426	1427	rBV2	325	117	0.00%	0.001%
23	5.973	1438	1441	1444	rVB2	305	185	0.00%	0.001%
24	6.012	1444	1453	1457	rBV	782	1119	0.02%	0.008%
25	6.063	1466	1469	1470	rBV	174	82	0.00%	0.001%
26	6.073	1470	1472	1476	rVB	372	232	0.00%	0.002%
27	6.096	1476	1479	1480	rBV	307	171	0.00%	0.001%
28	6.244	1511	1525	1542	rBV	297286	561964	10.71%	4.261%
29	6.481	1597	1599	1602	rVB	184	75	0.00%	0.001%
30	6.530	1603	1614	1627	rBV7	6760	14435	0.28%	0.109%
31	6.584	1627	1631	1636	rVB2	263	229	0.00%	0.002%
32	6.607	1636	1638	1641	rBV	293	162	0.00%	0.001%
33	6.684	1646	1662	1679	rBV	215211	418628	7.98%	3.174%
34	6.893	1722	1727	1730	rBV2	286	228	0.00%	0.002%
35	6.906	1730	1731	1733	rBV	151	45	0.00%	0.000%
36	6.961	1741	1748	1762	rBV3	2375	4545	0.09%	0.034%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
 Data File : VU053539.D
 Acq On : 03 Apr 2023 23:33
 Operator : JC/MD
 Sample : 02158-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-7D(20230329)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.063	1777	1780	1782	rBV2	236	170	0.00%	0.001%
38	7.125	1795	1799	1801	rBV	417	373	0.01%	0.003%
39	7.237	1831	1834	1836	rBV	203	104	0.00%	0.001%
40	7.359	1870	1872	1874	rBV	166	73	0.00%	0.001%
41	7.375	1874	1877	1880	rVB	201	106	0.00%	0.001%
42	7.456	1899	1902	1908	rVB	261	175	0.00%	0.001%
43	7.562	1922	1935	1955	rBV	124244	219512	4.18%	1.664%
44	7.678	1969	1971	1972	rBV2	363	144	0.00%	0.001%
45	7.694	1974	1976	1978	rBV	446	240	0.00%	0.002%
46	7.780	2000	2003	2005	rBV	328	154	0.00%	0.001%
47	7.809	2010	2012	2016	rVB	316	202	0.00%	0.002%
48	7.829	2016	2018	2019	rBV	176	78	0.00%	0.001%
49	7.893	2024	2038	2054	rBV	455023	784837	14.96%	5.951%
50	8.083	2095	2097	2099	rBV2	290	125	0.00%	0.001%
51	8.176	2114	2126	2147	rBV2	87305	148481	2.83%	1.126%
52	8.285	2157	2160	2161	rBV	231	120	0.00%	0.001%
53	8.411	2195	2199	2203	rVB2	218	169	0.00%	0.001%
54	8.436	2204	2207	2211	rVB	275	189	0.00%	0.001%
55	8.462	2211	2215	2218	rBV2	467	396	0.01%	0.003%
56	8.510	2229	2230	2233	rBV	152	54	0.00%	0.000%
57	8.552	2233	2243	2252	rVV3	9909	16714	0.32%	0.127%
58	8.626	2255	2266	2301	rBV	238253	434394	8.28%	3.294%
59	9.169	2432	2435	2437	rBV	178	96	0.00%	0.001%
60	9.247	2456	2459	2463	rVB	251	136	0.00%	0.001%
61	9.269	2463	2466	2467	rBV	184	88	0.00%	0.001%
62	9.333	2483	2486	2488	rBV2	280	202	0.00%	0.002%
63	9.414	2497	2511	2516	rBV	416602	706525	13.46%	5.357%
64	9.562	2554	2557	2560	rBV3	1089	990	0.02%	0.008%
65	9.629	2574	2578	2579	rBV	176	139	0.00%	0.001%
66	9.948	2676	2677	2678	rBV	147	33	0.00%	0.000%
67	9.983	2685	2688	2690	rBV	345	222	0.00%	0.002%
68	10.022	2697	2700	2703	rBV	235	189	0.00%	0.001%
69	10.073	2713	2716	2718	rBV2	250	160	0.00%	0.001%
70	10.214	2756	2760	2763	rBV	378	282	0.01%	0.002%
71	10.230	2763	2765	2769	rVB	247	138	0.00%	0.001%
72	10.401	2815	2818	2819	rBV	178	85	0.00%	0.001%
73	10.481	2834	2843	2849	rBV4	820	1193	0.02%	0.009%
74	10.642	2889	2893	2895	rBV	236	189	0.00%	0.001%
75	10.751	2915	2927	2945	rBV	317421	508646	9.69%	3.857%
76	11.028	3010	3013	3020	rBV2	231	282	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
 Data File : VU053539.D
 Acq On : 03 Apr 2023 23:33
 Operator : JC/MD
 Sample : 02158-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PMW-7D(20230329)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

77	11.266	3084	3087	3091	rVB	316	190	0.00%	0.001%
78	11.414	3124	3133	3144	rBV2	9851	14120	0.27%	0.107%
79	11.465	3144	3149	3157	rVB2	1324	1630	0.03%	0.012%
80	11.658	3206	3209	3214	rVB2	391	299	0.01%	0.002%
81	11.742	3222	3235	3245	rBV	512754	824452	15.71%	6.251%
82	11.832	3246	3263	3291	rVB2	2948613	5247561	100.00%	39.788%
83	12.189	3362	3374	3393	rBV	507931	862907	16.44%	6.543%
84	12.356	3424	3426	3429	rBV	276	159	0.00%	0.001%
85	12.613	3504	3506	3509	rBV	290	166	0.00%	0.001%
86	12.809	3565	3567	3569	rBV	319	133	0.00%	0.001%
87	12.938	3605	3607	3611	rBV	180	84	0.00%	0.001%
88	13.160	3674	3676	3682	rVB2	413	292	0.01%	0.002%
89	13.388	3744	3747	3748	rBV2	312	183	0.00%	0.001%
90	13.838	3877	3887	3905	rVB	58132	92315	1.76%	0.700%
91	14.330	4032	4040	4051	rVB2	9838	15118	0.29%	0.115%




Sum of corrected areas: 13188918

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053539.D
Acq On : 03 Apr 2023 23:33
Operator : JC/MD
Sample : 02158-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-7D(20230329)

Quant Title :

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

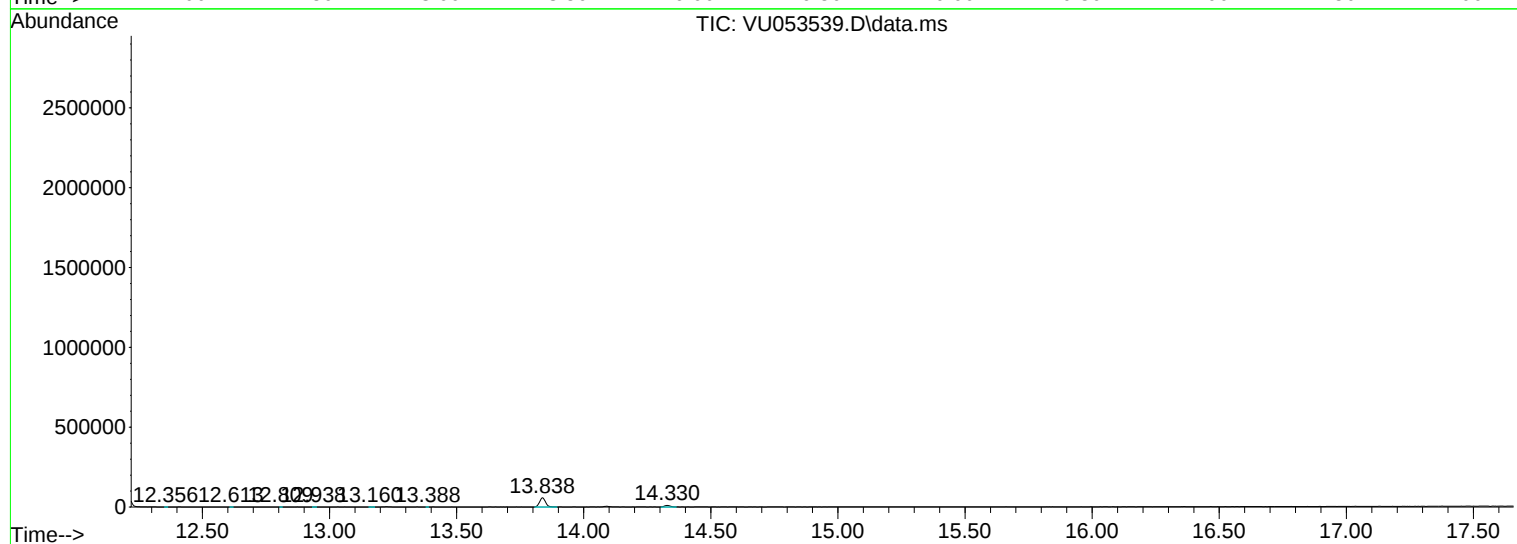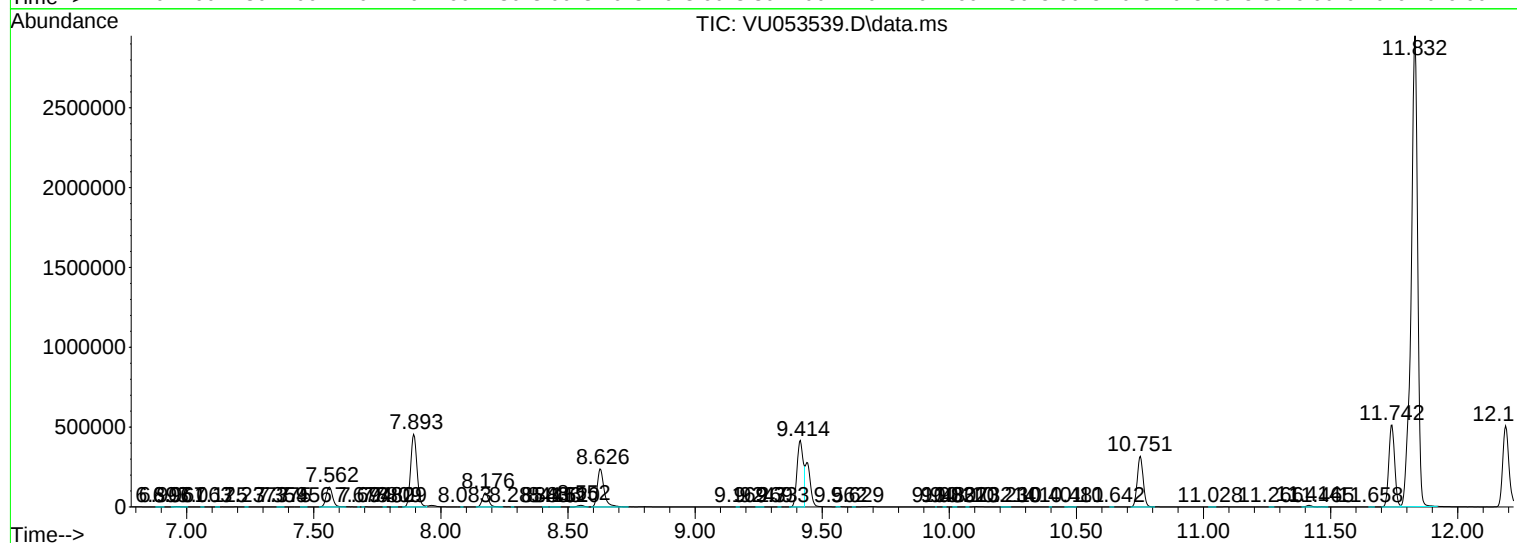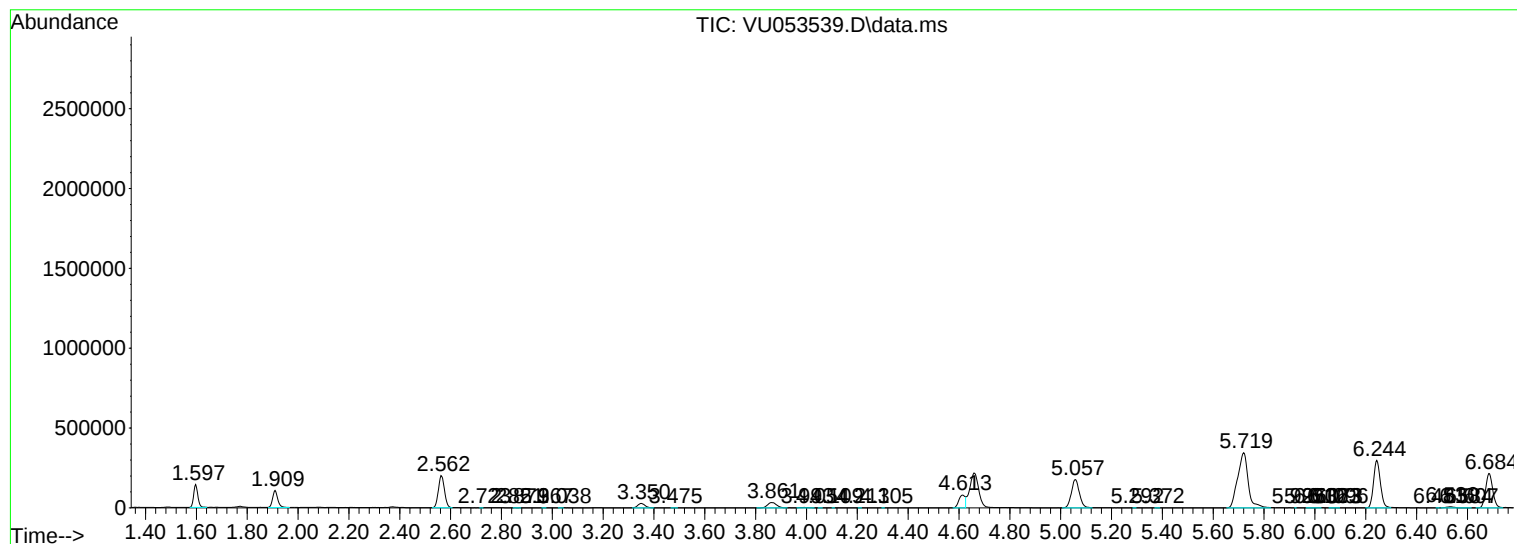

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053539.D
Acq On : 03 Apr 2023 23:33
Operator : JC/MD
Sample : 02158-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-7D(20230329)

Quant Title :

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053539.D
Acq On : 03 Apr 2023 23:33
Operator : JC/MD
Sample : 02158-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PMW-7D(20230329)

Quant Title :

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc