

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
 Data File : VU053544.D
 Acq On : 04 Apr 2023 01:32
 Operator : JC/MD
 Sample : 02158-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 MW-2(20230330)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053544.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	94	rVB	127206	141543	15.80%	1.956%
2	1.909	169	177	196	rVB	101453	138204	15.43%	1.909%
3	2.562	369	380	394	rBV	186756	303017	33.83%	4.186%
4	2.697	419	422	424	rBV	506	362	0.04%	0.005%
5	2.900	482	485	488	rBV	258	147	0.02%	0.002%
6	3.031	523	526	527	rBV2	551	332	0.04%	0.005%
7	3.318	613	615	616	rBV2	161	56	0.01%	0.001%
8	3.347	616	624	625	rBV2	1609	1561	0.17%	0.022%
9	3.440	651	653	658	rVB	201	89	0.01%	0.001%
10	3.630	709	712	715	rBV	298	203	0.02%	0.003%
11	3.665	721	723	725	rBV	191	95	0.01%	0.001%
12	3.707	733	736	738	rBV	232	173	0.02%	0.002%
13	3.861	778	784	797	rVB2	3552	6591	0.74%	0.091%
14	4.199	879	889	894	rBV	249	469	0.05%	0.006%
15	4.404	950	953	956	rVB2	293	175	0.02%	0.002%
16	4.424	956	959	961	rBV2	202	135	0.02%	0.002%
17	4.504	980	984	988	rBV2	265	189	0.02%	0.003%
18	4.613	1006	1018	1023	rBV	74789	142307	15.89%	1.966%
19	4.906	1107	1109	1114	rVB2	412	322	0.04%	0.004%
20	5.057	1140	1156	1176	rBV	168612	368563	41.14%	5.092%
21	5.231	1208	1210	1211	rBV	392	166	0.02%	0.002%
22	5.292	1226	1229	1232	rBV	287	209	0.02%	0.003%
23	5.334	1240	1242	1244	rBV	183	56	0.01%	0.001%
24	5.375	1253	1255	1257	rBV	247	119	0.01%	0.002%
25	5.533	1301	1304	1306	rBV	231	134	0.01%	0.002%
26	5.719	1341	1362	1380	rBV2	326450	895814	100.00%	12.377%
27	5.961	1435	1437	1441	rVB	311	203	0.02%	0.003%
28	6.109	1481	1483	1488	rVB2	260	162	0.02%	0.002%
29	6.244	1512	1525	1542	rBV	272358	513318	57.30%	7.092%
30	6.478	1595	1598	1600	rBV	168	80	0.01%	0.001%
31	6.530	1603	1614	1624	rBV9	4553	9408	1.05%	0.130%
32	6.687	1648	1663	1682	rBV	204464	402234	44.90%	5.557%
33	6.964	1747	1749	1750	rBV	319	144	0.02%	0.002%
34	7.182	1813	1817	1822	rBV3	520	565	0.06%	0.008%
35	7.305	1852	1855	1861	rVB2	306	253	0.03%	0.003%
36	7.356	1868	1871	1874	rVB	223	103	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
 Data File : VU053544.D
 Acq On : 04 Apr 2023 01:32
 Operator : JC/MD
 Sample : 02158-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 MW-2(20230330)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.430	1892	1894	1895	rBV	161	51	0.01%	0.001%
38	7.510	1916	1919	1922	rVB	226	130	0.01%	0.002%
39	7.562	1923	1935	1954	rBV	119014	204459	22.82%	2.825%
40	7.684	1970	1973	1975	rBV3	273	233	0.03%	0.003%
41	7.745	1989	1992	1994	rBV2	283	190	0.02%	0.003%
42	7.774	1999	2001	2005	rBV	296	273	0.03%	0.004%
43	7.893	2025	2038	2055	rBV	422946	741383	82.76%	10.243%
44	8.176	2113	2126	2146	rBV	81415	142375	15.89%	1.967%
45	8.314	2166	2169	2172	rVB2	241	140	0.02%	0.002%
46	8.449	2209	2211	2212	rBV	266	96	0.01%	0.001%
47	8.549	2234	2242	2253	rBV3	6179	10606	1.18%	0.147%
48	8.626	2254	2266	2296	rBV	219995	405144	45.23%	5.597%
49	9.038	2392	2394	2396	rBV	264	110	0.01%	0.002%
50	9.063	2400	2402	2403	rBV	228	53	0.01%	0.001%
51	9.301	2474	2476	2478	rBV	233	99	0.01%	0.001%
52	9.314	2478	2480	2481	rBV	149	48	0.01%	0.001%
53	9.414	2498	2511	2532	rBV	371121	628923	70.21%	8.689%
54	9.687	2589	2596	2597	rBV3	883	793	0.09%	0.011%
55	9.858	2647	2649	2651	rVB	168	62	0.01%	0.001%
56	10.012	2695	2697	2699	rBV2	206	134	0.01%	0.002%
57	10.195	2752	2754	2760	rVB	250	175	0.02%	0.002%
58	10.243	2766	2769	2771	rBV2	278	187	0.02%	0.003%
59	10.340	2796	2799	2802	rVB	200	116	0.01%	0.002%
60	10.449	2831	2833	2835	rBV	196	64	0.01%	0.001%
61	10.472	2838	2840	2841	rBV	318	136	0.02%	0.002%
62	10.751	2915	2927	2942	rBV	302648	482266	53.84%	6.663%
63	10.896	2964	2972	2975	rBV3	602	774	0.09%	0.011%
64	11.465	3143	3149	3157	rBV3	730	923	0.10%	0.013%
65	11.742	3225	3235	3244	rBV3	21543	33518	3.74%	0.463%
66	11.809	3244	3256	3277	rVV2	415339	762759	85.15%	10.538%
67	12.002	3314	3316	3320	rBV	238	153	0.02%	0.002%
68	12.189	3361	3374	3396	rBV	449294	730457	81.54%	10.092%
69	12.365	3426	3429	3433	rVB	180	129	0.01%	0.002%
70	12.388	3433	3436	3440	rBV2	414	359	0.04%	0.005%
71	12.870	3583	3586	3588	rBV2	390	271	0.03%	0.004%
72	13.044	3637	3640	3644	rBV2	508	350	0.04%	0.005%
73	13.144	3668	3671	3674	rBV	260	149	0.02%	0.002%
74	13.189	3681	3685	3687	rBV	303	228	0.03%	0.003%
75	13.552	3795	3798	3800	rBV	316	177	0.02%	0.002%
76	13.671	3832	3835	3837	rBV	363	183	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
 Data File : VU053544.D
 Acq On : 04 Apr 2023 01:32
 Operator : JC/MD
 Sample : 02158-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 MW-2(20230330)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M

Title : VOC Analysis

77	13.709	3845	3847	3851	rBV2	353	309	0.03%	0.004%
78	13.838	3875	3887	3902	rBV2	89356	147379	16.45%	2.036%
79	13.938	3916	3918	3922	rVB	349	198	0.02%	0.003%
80	13.960	3922	3925	3928	rBV2	417	297	0.03%	0.004%
81	13.980	3928	3931	3933	rBV	475	301	0.03%	0.004%
82	14.327	4033	4039	4052	rVB3	8571	13304	1.49%	0.184%


Sum of corrected areas: 7237965

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053544.D
Acq On : 04 Apr 2023 01:32
Operator : JC/MD
Sample : 02158-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MW-2(20230330)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

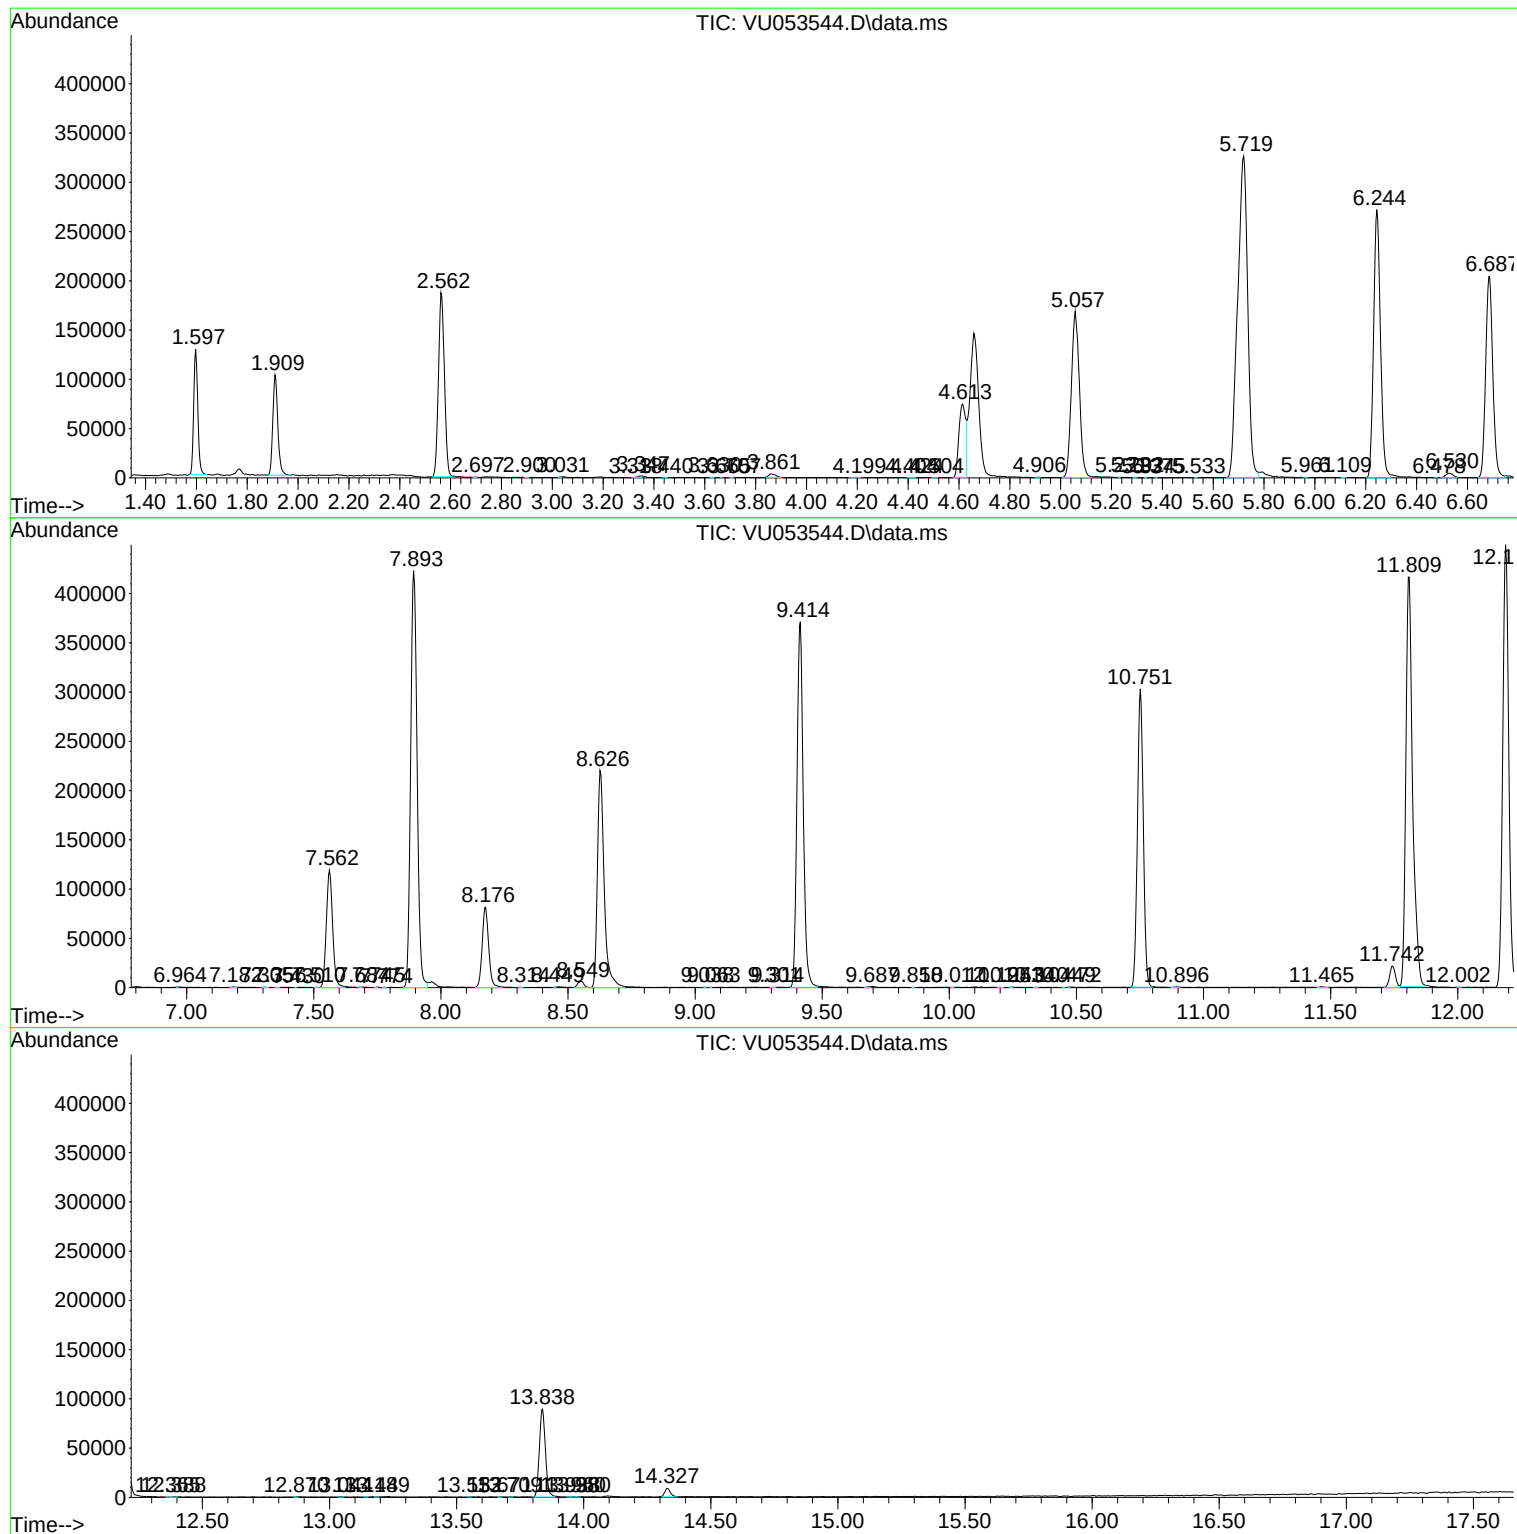

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053544.D
Acq On : 04 Apr 2023 01:32
Operator : JC/MD
Sample : 02158-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MW-2(20230330)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053544.D
Acq On : 04 Apr 2023 01:32
Operator : JC/MD
Sample : 02158-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MW-2(20230330)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------