


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040323\
Data File : VU053509.D
Acq On : 03 Apr 2023 10:26
Operator : JC/MD
Sample : BFB172
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB172

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Title : VOC Analysis
Last Update : Sat Apr 01 04:51:17 2023

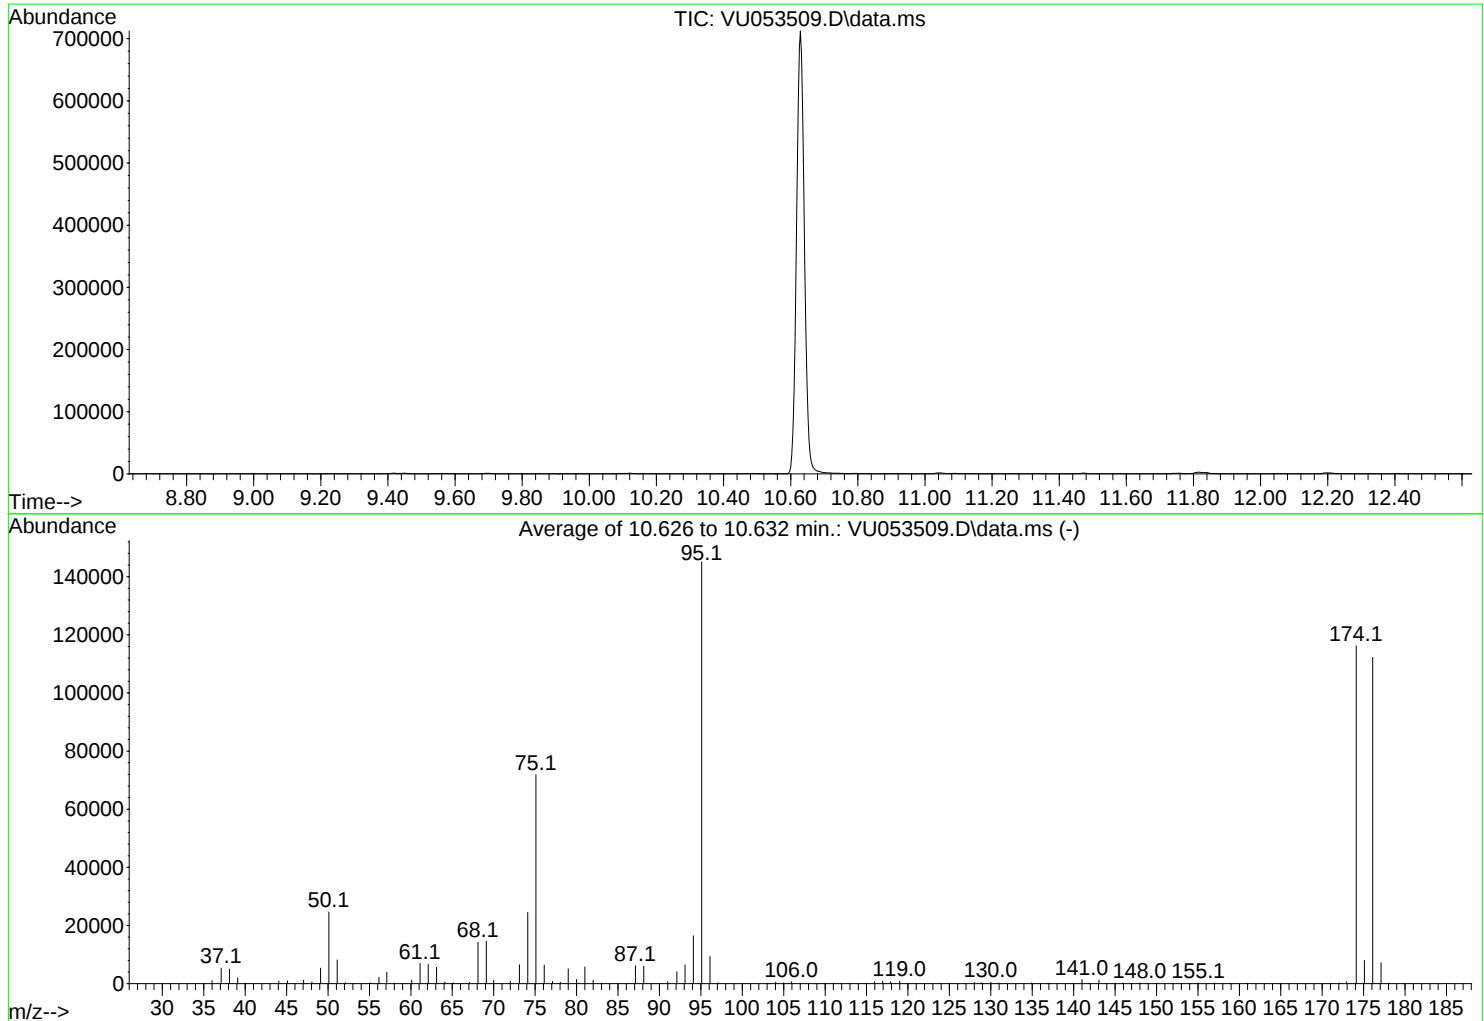

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2875

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.9	24595	PASS
75	95	30	80	49.5	71896	PASS
95	95	100	100	100.0	145109	PASS
96	95	5	9	6.4	9335	PASS
173	174	0.00	2	0.5	614	PASS
174	95	50	120	80.1	116181	PASS
175	174	5	9	6.9	8001	PASS
176	174	95	101	96.6	112245	PASS
177	176	5	9	6.4	7149	PASS

m/z	Abundance
44.00	170.0

Instrument :
MSVOA_U
ClientSampleId :
BFB172

m/z	Abundance
36.00	1179.0
37.10	5438.0
38.10	5325.0
39.10	2055.0
40.10	161.0
44.10	1204.0
45.10	1021.0
47.10	1203.0
48.10	613.0
49.10	5263.0
50.10	25120.0
51.10	8357.0
52.10	331.0
55.10	283.0
56.10	2134.0
57.10	3954.0
58.00	187.0
60.10	1298.0
61.10	7059.0
62.10	6818.0
63.10	5541.0
64.10	621.0
65.20	255.0
67.10	418.0
68.10	14179.0
69.10	14949.0
70.00	1134.0
72.00	843.0
73.10	6241.0
74.10	24928.0
75.10	71216.0
76.10	6496.0
77.10	897.0
78.00	539.0
79.00	5228.0
80.00	1488.0
81.00	5890.0
82.00	1188.0
83.00	158.0
87.10	6463.0
88.10	5974.0
91.00	644.0
92.10	4235.0
93.10	6382.0
94.10	16424.0
95.10	145344.0
96.10	9524.0
97.10	312.0
103.10	103.0
104.00	591.0
105.00	233.0
106.00	760.0
107.00	157.0
111.00	149.0
114.90	203.0
116.00	593.0
116.90	899.0
117.90	674.0
119.00	832.0
123.90	118.0
128.00	366.0
128.90	243.0
130.00	423.0
130.90	165.0
134.90	164.0
137.10	291.0
139.90	111.0
141.00	1412.0
141.90	176.0
143.00	1222.0
143.90	132.0
145.00	160.0
146.00	197.0
148.00	269.0
148.80	101.0
150.10	158.0
154.90	356.0
156.90	212.0
158.80	160.0
160.90	142.0
172.40	364.0
172.90	593.0
174.10	113432.0
175.10	7979.0
176.10	108824.0
177.10	7224.0
178.00	149.0

Instrument :
MSVOA_U
ClientSampleId :
BFB172

m/z	Abundance
36.00	1109.0
37.10	5555.0
38.10	5128.0
39.10	2091.0
40.10	189.0
44.10	1164.0
45.10	1038.0
47.10	1221.0
48.00	624.0
49.10	5431.0
50.10	25456.0
51.10	8415.0
52.10	326.0
55.10	266.0
56.20	2194.0
57.10	4064.0
58.00	240.0
60.10	1253.0
61.10	7206.0
62.10	6777.0
63.10	5918.0
64.10	561.0
65.20	269.0
67.10	480.0
68.10	14624.0
69.10	15034.0
70.00	1227.0
72.00	832.0
73.10	6817.0
74.10	25448.0
75.10	74080.0
76.10	6616.0
77.10	764.0
78.00	500.0
79.00	5255.0
80.00	1482.0
81.00	5897.0
82.00	1210.0
83.00	182.0
87.10	6339.0
88.10	6162.0
91.00	683.0
92.10	4137.0
93.10	6703.0
94.10	17000.0
95.10	149760.0
96.10	9608.0
97.10	280.0
103.10	124.0
104.10	574.0
105.00	325.0
105.90	718.0
106.90	130.0
109.90	108.0
111.20	160.0
111.90	105.0
113.00	101.0
114.90	176.0
116.00	652.0
116.90	944.0
117.90	705.0
119.00	985.0
123.90	101.0
128.10	410.0
128.80	304.0
130.00	523.0
131.00	234.0
134.90	225.0
137.00	236.0
141.00	1391.0
141.90	196.0
143.00	1267.0
143.90	107.0
145.00	154.0
145.90	244.0
147.10	112.0
148.00	270.0
148.90	111.0
150.00	176.0
155.10	348.0
156.20	129.0
156.90	205.0
158.90	168.0
160.90	189.0
172.10	293.0
173.00	624.0
174.10	119664.0
175.10	8138.0
176.10	115568.0
177.10	7414.0
178.10	177.0

Instrument :
MSVOA_U
ClientSampleId :
BFB172

m/z	Abundance
36.00	923.0
37.10	5099.0
38.10	4515.0
39.10	1858.0
40.10	185.0
44.10	1008.0
45.10	963.0
47.00	1242.0
48.00	624.0
49.10	5383.0
50.10	23208.0
51.10	7627.0
52.10	291.0
55.20	255.0
56.20	2093.0
57.10	3852.0
58.00	218.0
60.10	1133.0
61.10	6701.0
62.10	6189.0
63.10	5480.0
64.10	488.0
65.10	276.0
67.00	425.0
68.10	13923.0
69.10	13813.0
70.00	1201.0
72.00	700.0
73.10	6491.0
74.10	23056.0
75.10	70392.0
76.10	5949.0
77.10	630.0
78.10	434.0
79.00	4918.0
80.00	1376.0
81.00	5329.0
82.00	1148.0
83.00	186.0
86.20	103.0
87.10	5752.0
88.10	5939.0
91.00	641.0
92.10	3855.0
93.10	6405.0
94.10	15931.0
95.10	140224.0
96.10	8873.0
97.10	241.0
103.10	107.0
104.00	553.0
105.00	364.0
106.00	562.0
106.90	115.0
109.90	119.0
111.10	154.0
111.90	115.0
113.00	178.0
115.00	149.0
115.90	684.0
117.00	867.0
117.90	611.0
119.00	999.0
128.10	460.0
128.80	335.0
130.00	575.0
131.00	266.0
134.90	264.0
136.80	189.0
141.00	1451.0
141.80	175.0
143.10	1303.0
145.00	125.0
145.90	276.0
147.10	129.0
148.00	269.0
149.00	120.0
150.00	146.0
155.10	326.0
156.20	101.0
157.00	203.0
158.90	163.0
160.90	204.0
171.10	113.0
172.00	348.0
173.00	624.0
174.10	115448.0
175.10	7887.0
176.10	112344.0
177.10	6809.0
178.10	201.0

Instrument :
MSVOA_U
ClientSampleId :
BFB172