




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040324\
 Data File : VU058365.D
 Acq On : 03 Apr 2024 15:44
 Operator : MD/SY
 Sample : P1929-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AL2

Manual IntegrationsAPPROVED

Quant Time: Apr 04 01:24:59 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032124WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 04 01:17:39 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/05/2024
 Supervised By :Semsettin Yesilyurt 04/05/2024

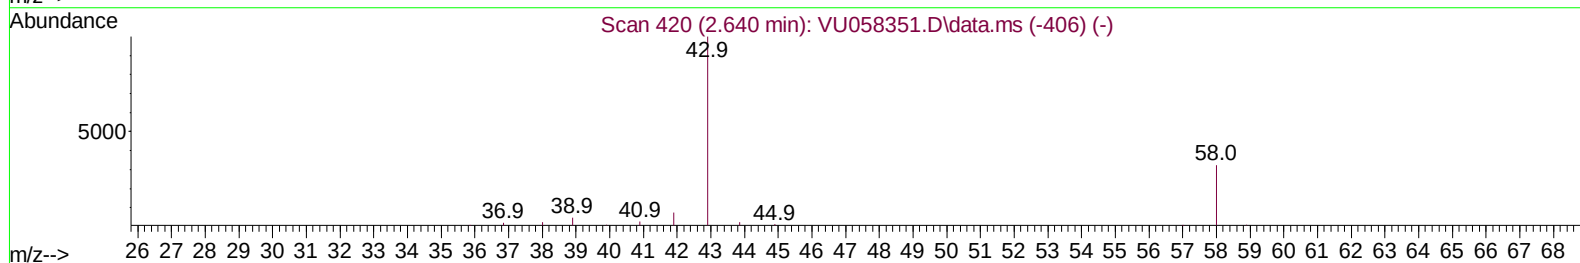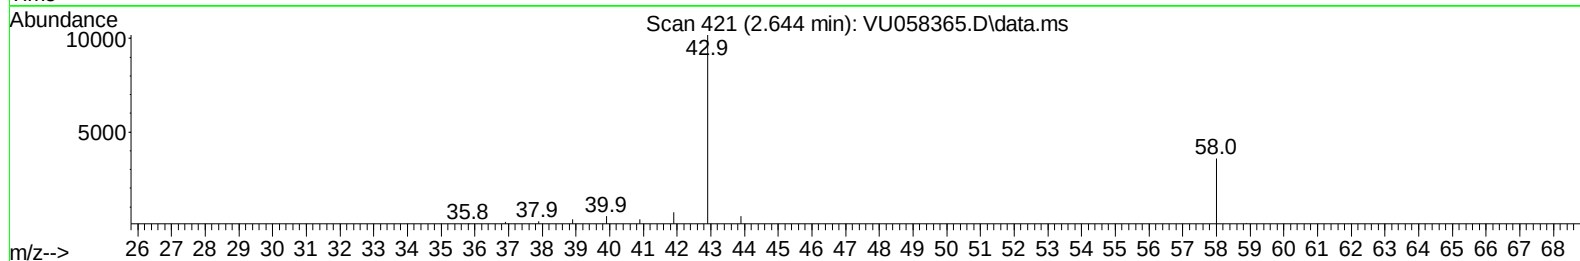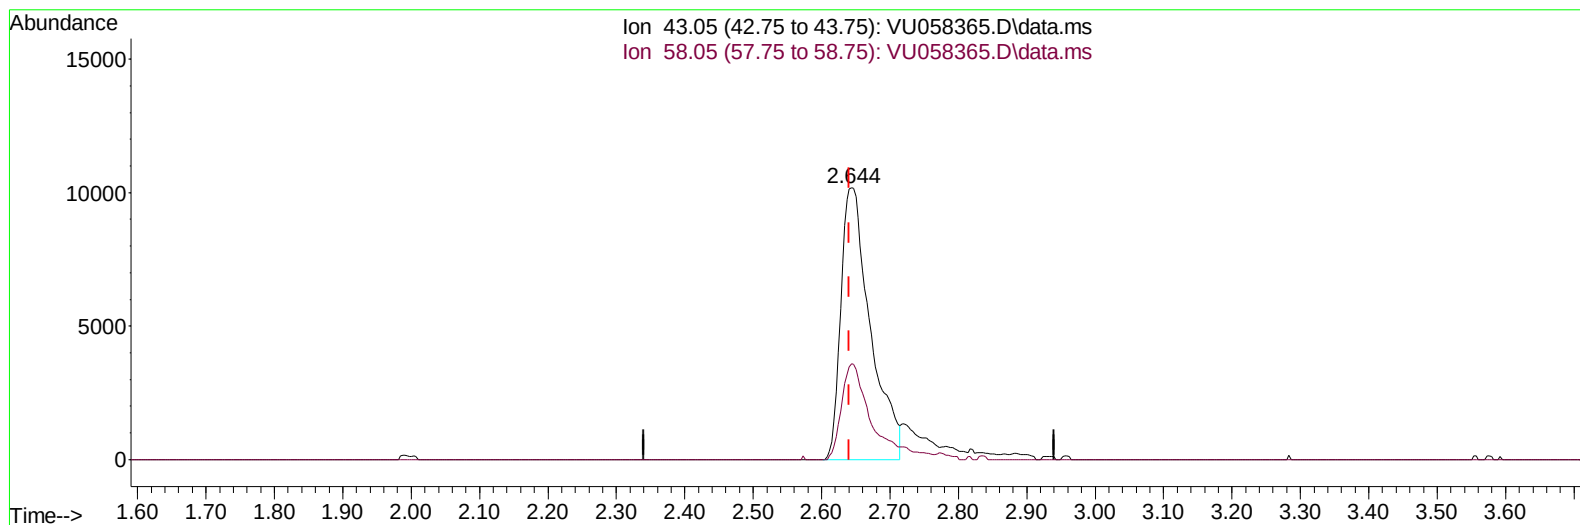

TIC: VU058365.D\data.ms

(13) Acetone (T)

2.644min (+ 0.003) 41.34 ug/L

response 30541

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.30	33.19
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040324\
Data File : VU058365.D
Acq On : 03 Apr 2024 15:44
Operator : MD/SY
Sample : P1929-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AL2

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 04/05/2024
Supervised By :Semsettin Yesilyurt 04/05/2024

Quant Time: Apr 04 01:24:59 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032124WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 04 01:17:39 2024
Response via : Initial Calibration

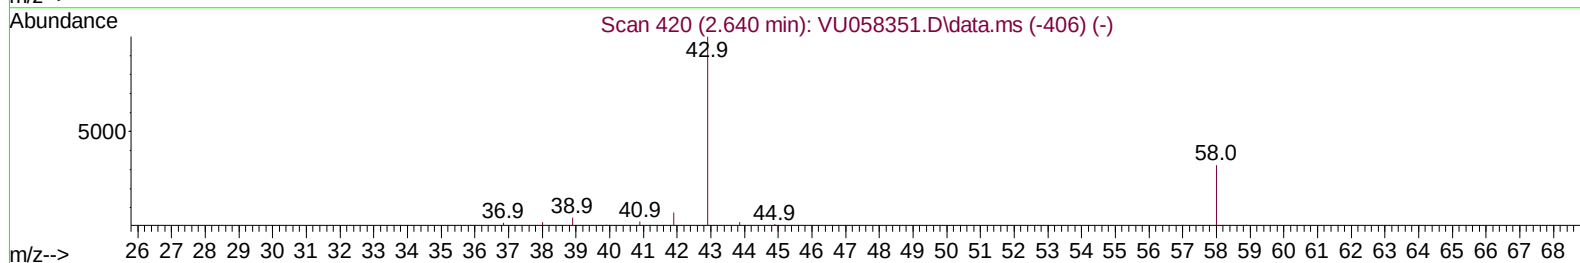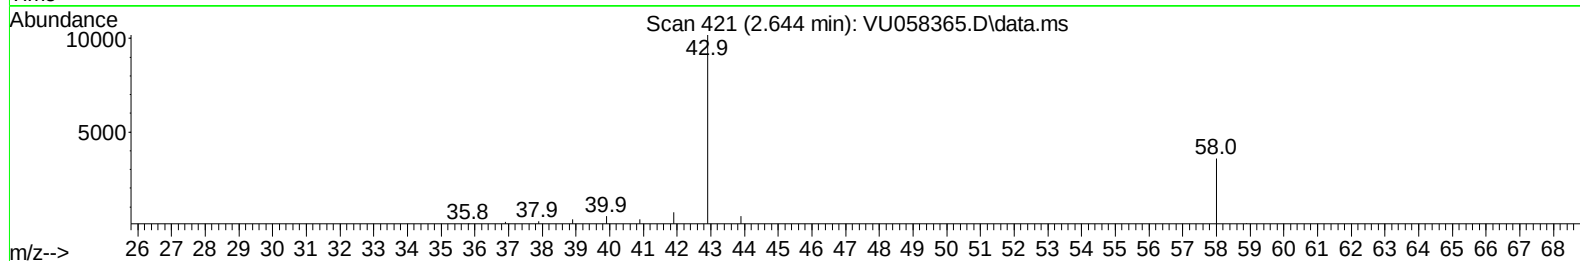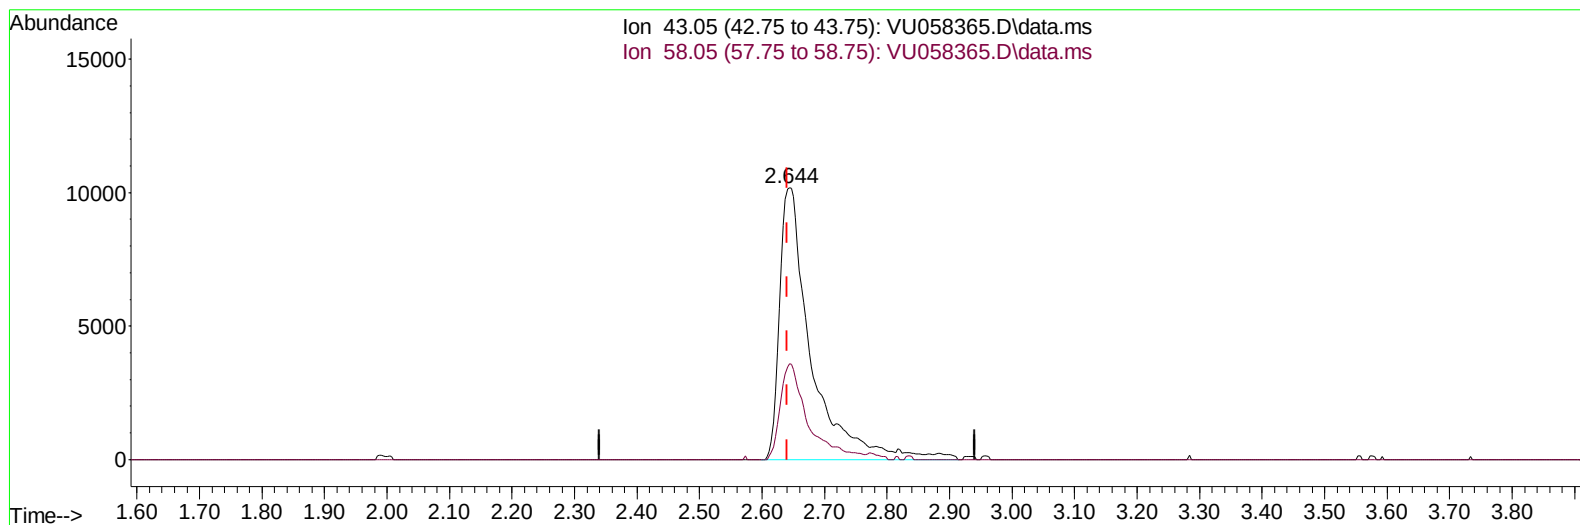

TIC: VU058365.D\data.ms

(13) Acetone (T)

2.644min (+ 0.003) 48.52 ug/L m

response 35844

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.30	28.28
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040324\
 Data File : VU058365.D
 Acq On : 03 Apr 2024 15:44
 Operator : MD/SY
 Sample : P1929-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AL2

Manual IntegrationsAPPROVED

Quant Time: Apr 04 01:24:59 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032124WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 04 01:17:39 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 04/05/2024
 Supervised By :Semsettin Yesilyurt 04/05/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		76036	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		72323	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		31842	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.595	65		20034	3.118	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	62.400%	
7) Chloroethane-d5	1.907	69		21394	4.079	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.600%	
11) 1,1-Dichloroethene-d2	2.560	65		9015	3.379	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.600%	
20) 2-Butanone-d5	4.624	46		62850	55.057	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	110.120%	
24) Chloroform-d	5.052	84		50695	4.413	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.200%	
26) 1,2-Dichloroethane-d4	5.695	65		25957	4.833	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.600%	
32) Benzene-d6	5.718	84		100318	4.271	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.400%	
36) 1,2-Dichloropropane-d6	6.682	67		32422	4.683	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.600%	
41) Toluene-d8	7.891	98		80752	3.880	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.600%	
43) trans-1,3-Dichloroprop...	8.174	79		8920	4.021	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.400%	
46) 2-Hexanone-d5	8.627	63		44225	49.228	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.460%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84		22583	5.007	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.200%	
66) 1,2-Dichlorobenzene-d4	12.187	152		28515	4.809	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.200%	
Target Compounds							
13) Acetone	2.644	43		35844m	48.517	ug/L	
21) 2-Butanone	4.708	43		49684	44.265	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040324\
Data File : VU058365.D
Acq On : 03 Apr 2024 15:44
Operator : MD/SY
Sample : P1929-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AL2

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 04/05/2024
Supervised By :Semsettin Yesilyurt 04/05/2024

Quant Time: Apr 04 01:24:59 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032124WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 04 01:17:39 2024
Response via : Initial Calibration

