


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU040324\
Data File : VU058350.D
Acq On : 03 Apr 2024 08:39
Operator : MD/SY
Sample : BFB135
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB135

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032124WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Apr 04 20:02:32 2024

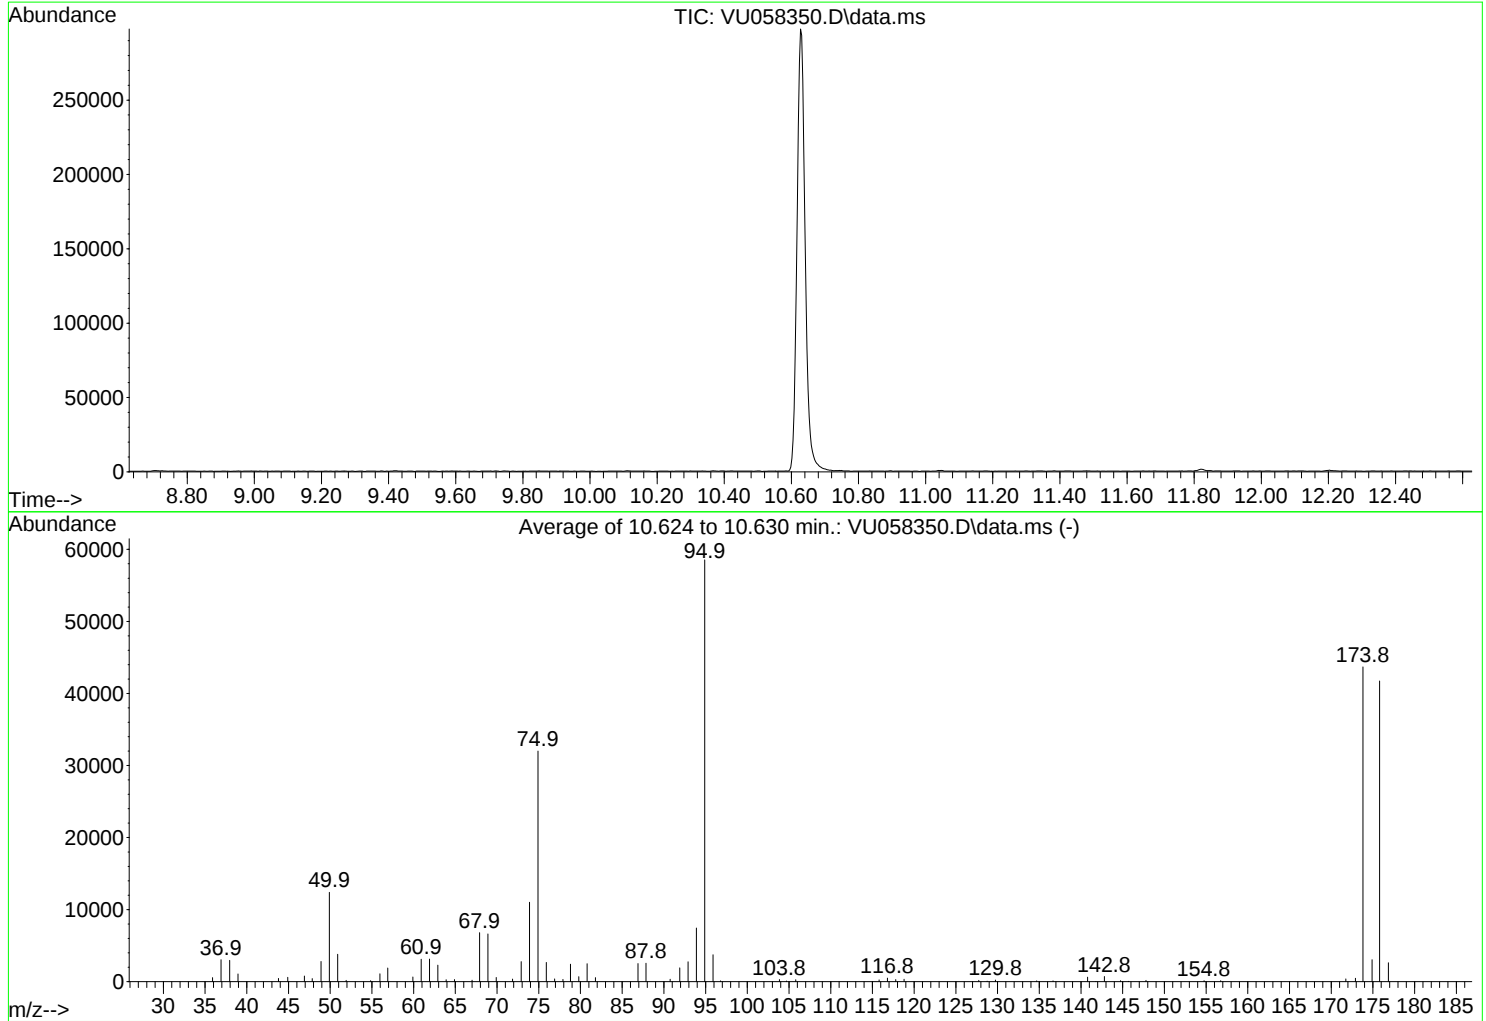

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.2	12403	PASS
75	95	30	80	54.7	32005	PASS
95	95	100	100	100.0	58547	PASS
96	95	5	9	6.4	3743	PASS
173	174	0.00	2	1.1	469	PASS
174	95	50	120	74.6	43683	PASS
175	174	5	9	7.0	3040	PASS
176	174	95	101	95.5	41720	PASS
177	176	5	9	6.3	2613	PASS

Scan 2890 (10.582 min): VU058350.D\data.ms
BFB135

m/z	Abundance
39.90	444.0
43.90	166.0

Instrument :
MSVOA_U
ClientSampleId :
BFB135

m/z	Abundance
35.90	558.0
36.90	2964.0
37.90	2888.0
39.00	1089.0
39.90	416.0
43.80	572.0
44.90	622.0
46.90	736.0
47.90	399.0
48.90	2737.0
49.90	12026.0
50.90	3691.0
51.90	178.0
54.80	123.0
56.00	1059.0
56.90	1809.0
59.90	661.0
60.90	3031.0
61.90	3055.0
62.90	2286.0
63.90	259.0
64.90	284.0
67.10	179.0
67.90	6470.0
68.90	6315.0
69.90	565.0
71.80	372.0
72.90	2600.0
73.90	10663.0
74.90	30904.0
75.90	2514.0
76.90	348.0
77.90	286.0
78.80	2287.0
79.80	650.0
80.80	2408.0
81.80	521.0
86.90	2391.0
87.90	2392.0
90.80	302.0
91.90	1852.0
92.90	2707.0
93.90	7267.0
94.90	56304.0
95.90	3649.0
96.80	106.0
103.80	288.0
105.80	258.0
115.80	203.0
116.80	503.0
117.80	259.0
118.80	320.0
127.80	163.0
129.70	218.0
134.70	109.0
136.70	116.0
140.80	607.0
141.80	104.0
142.80	716.0
144.80	142.0
147.80	167.0
154.80	148.0
156.70	143.0
171.70	343.0
172.90	441.0
173.80	40368.0
174.90	2900.0
175.80	38744.0
176.90	2504.0

Instrument :
MSVOA_U
ClientSampleId :
BFB135

m/z	Abundance
35.90	567.0
36.90	3147.0
38.00	3073.0
39.00	1099.0
39.90	436.0
43.80	627.0
44.90	611.0
46.90	825.0
47.90	426.0
48.90	2852.0
49.90	12820.0
50.90	3898.0
51.90	190.0
54.90	135.0
55.90	1118.0
56.90	1981.0
59.90	665.0
60.90	3213.0
61.90	3203.0
62.90	2345.0
63.90	266.0
64.90	304.0
67.00	187.0
67.90	7042.0
68.90	6825.0
69.90	591.0
71.80	353.0
72.90	2846.0
73.90	11435.0
74.90	32944.0
75.90	2720.0
76.90	396.0
77.90	341.0
78.80	2471.0
79.80	706.0
80.80	2573.0
81.80	566.0
86.90	2540.0
87.80	2654.0
90.70	354.0
91.90	1960.0
92.90	2828.0
93.90	7697.0
94.90	60432.0
95.90	3857.0
96.80	121.0
103.90	310.0
104.70	118.0
105.80	286.0
115.80	240.0
116.80	512.0
117.80	295.0
118.80	357.0
127.80	195.0
128.80	102.0
129.70	222.0
134.70	127.0
136.70	123.0
140.80	627.0
142.80	741.0
144.80	143.0
147.80	185.0
154.70	144.0
156.80	122.0
171.80	371.0
172.90	486.0
173.80	45048.0
174.90	3136.0
175.80	42984.0
176.90	2676.0

Instrument :
MSVOA_U
ClientSampleId :
BFB135

m/z	Abundance
35.90	547.0
36.90	3045.0
38.00	2882.0
38.90	1042.0
39.90	454.0
43.80	603.0
44.90	584.0
46.90	790.0
47.80	415.0
48.90	2776.0
49.90	12362.0
50.90	3833.0
51.90	178.0
54.90	141.0
55.90	1085.0
56.90	1901.0
59.90	632.0
60.90	3075.0
61.90	3141.0
62.90	2267.0
63.90	257.0
64.90	291.0
66.90	207.0
67.90	6882.0
68.90	6688.0
69.90	566.0
71.90	318.0
72.90	2861.0
73.90	10939.0
74.90	32168.0
75.90	2789.0
76.90	385.0
77.90	331.0
78.80	2477.0
79.80	699.0
80.80	2480.0
81.80	579.0
86.90	2595.0
87.80	2601.0
90.70	338.0
91.90	1893.0
92.90	2720.0
93.90	7336.0
94.90	58904.0
95.90	3723.0
96.80	102.0
103.90	284.0
104.70	133.0
105.80	280.0
115.80	264.0
116.80	482.0
117.80	295.0
118.80	353.0
127.70	194.0
128.70	118.0
129.80	226.0
134.70	129.0
136.60	116.0
140.80	632.0
142.80	712.0
144.70	120.0
145.70	110.0
147.80	194.0
154.70	138.0
156.80	113.0
171.80	396.0
172.90	479.0
173.80	45632.0
174.90	3085.0
175.80	43432.0
176.80	2660.0

Instrument :
MSVOA_U
ClientSampleId :
BFB135