
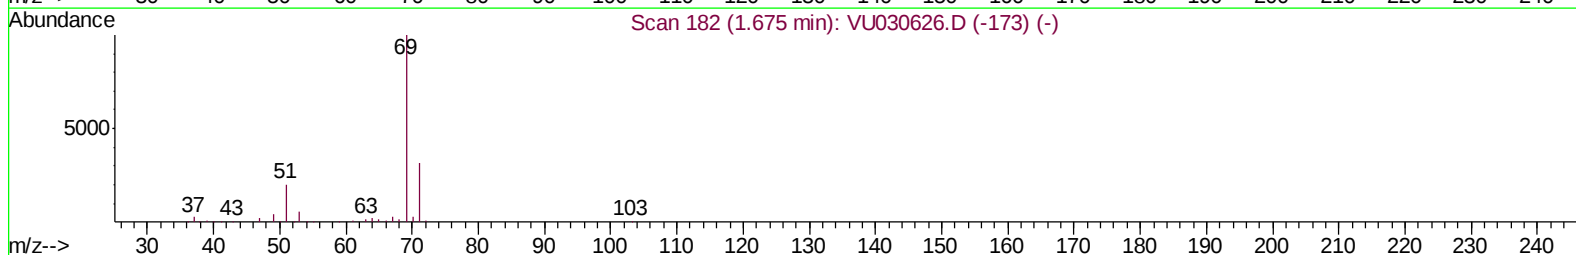
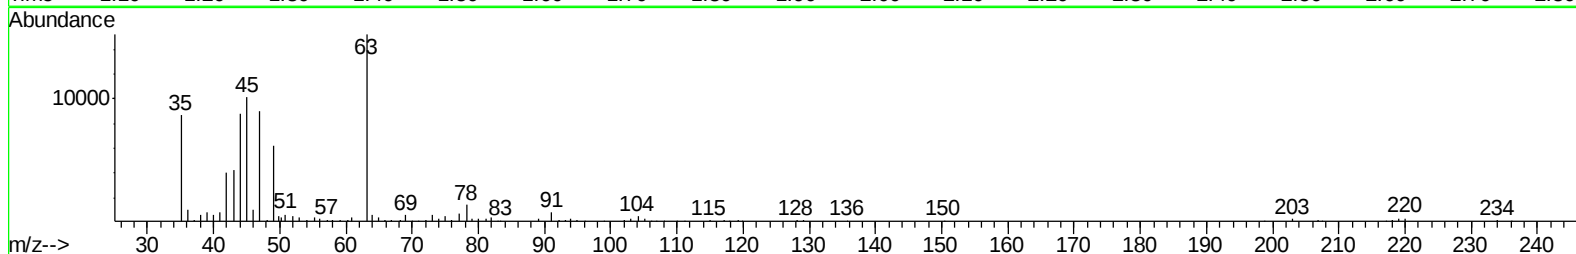


Data File : VU030628.D  
Acq On : 03 Apr 2019 15:38  
Operator : JC/SP  
Sample : K2119-14  
Misc : 5.43g/5mL/100uL/5.0mL/MSVOA\_U/MEOH  
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Apr 04 06:55:32 2019  
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\SOMULM032319WMA.M  
Quant Title : VOC Analysis  
QLast Update : Thu Apr 04 06:52:42 2019  
Response via : Initial Calibration

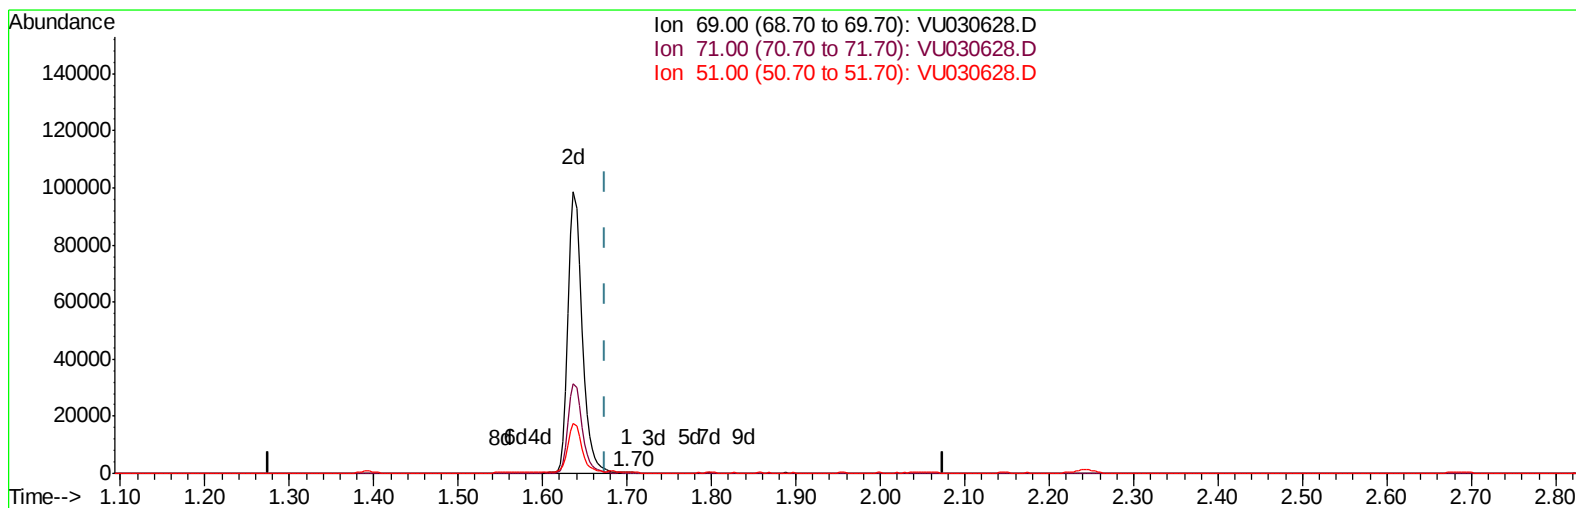

TIC: VU030628.D

(7) Chloroethane-d5 (S)

1.701min (+0.026) 0.17ug/L

response 477

| Ion   | Exp%  | Act%   |
|-------|-------|--------|
| 69.00 | 100   | 100    |
| 71.00 | 31.70 | 27.88  |
| 51.00 | 28.60 | 82.39# |
| 0.00  | 0.00  | 0.00   |