
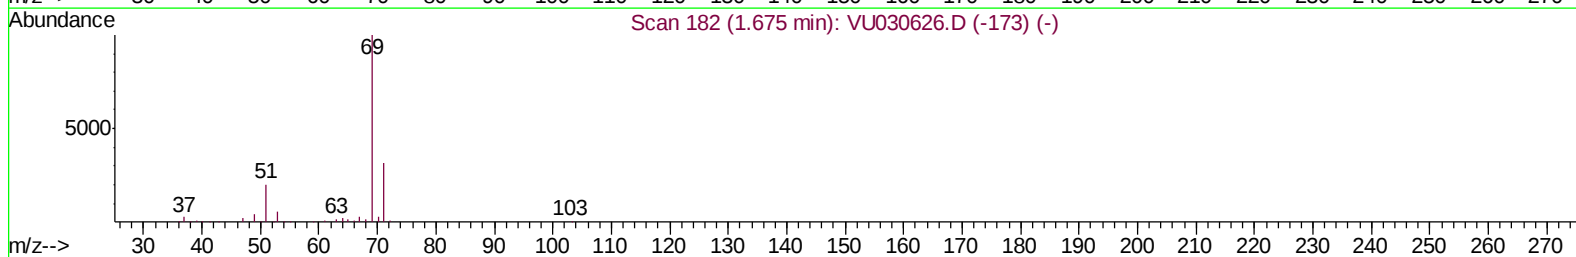
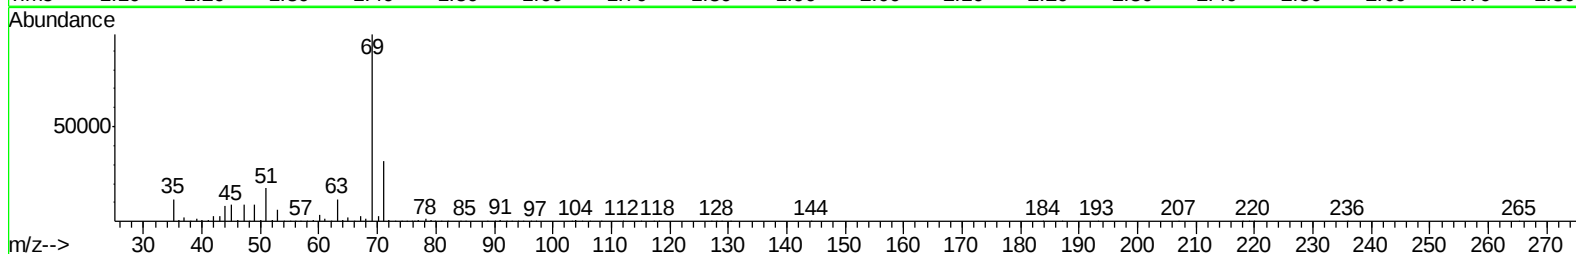


Data File : VU030628.D
Acq On : 03 Apr 2019 15:38
Operator : JC/SP
Sample : K2119-14
Misc : 5.43g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Apr 04 06:55:32 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 04 06:52:42 2019
Response via : Initial Calibration

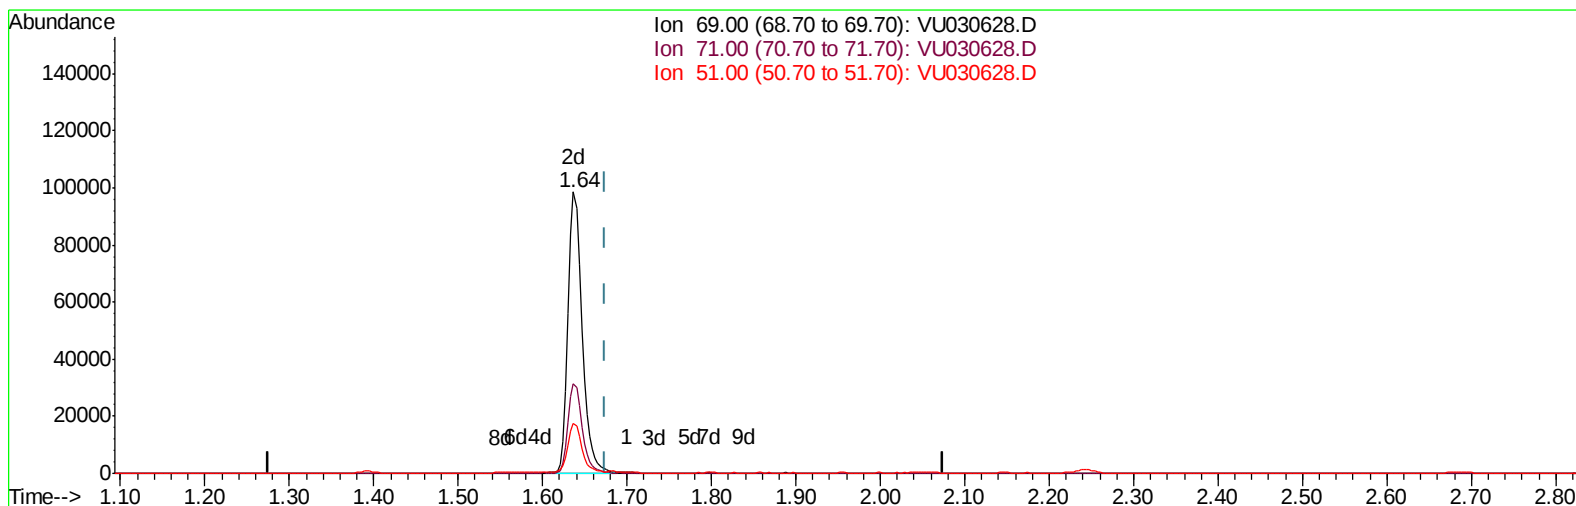

TIC: VU030628.D

(7) Chloroethane-d5 (S)

1.637min (-0.039) 41.24ug/L m

response 114077

Ion	Exp%	Act%
69.00	100	100
71.00	31.70	0.12#
51.00	28.60	0.34#
0.00	0.00	0.00