
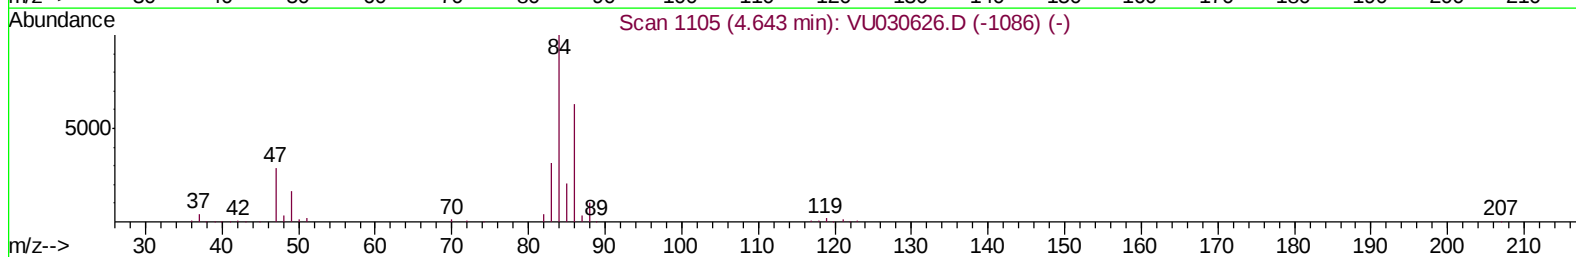
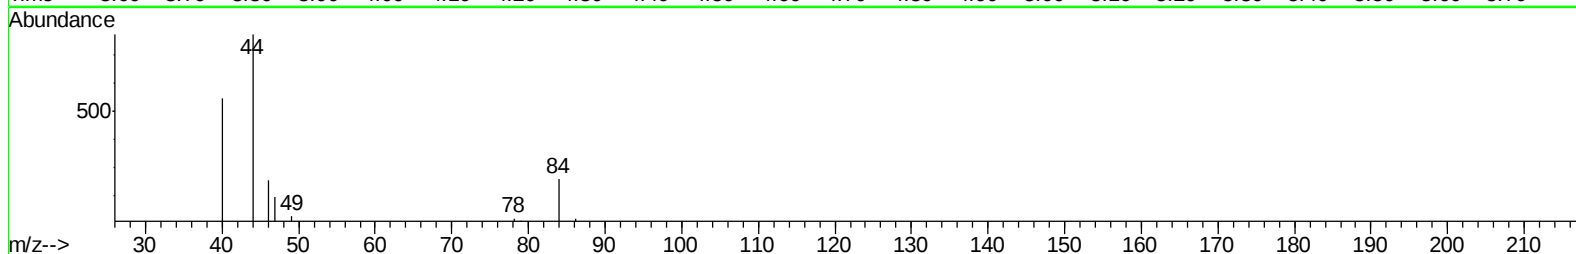


Data File : VU030629.D  
Acq On : 03 Apr 2019 16:01  
Operator : JC/SP  
Sample : K2119-15  
Misc : 5.01g/5mL/100uL/5.0mL/MSVOA\_U/MEOH  
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Apr 04 06:55:43 2019  
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\SOMULM032319WMA.M  
Quant Title : VOC Analysis  
QLast Update : Thu Apr 04 06:52:42 2019  
Response via : Initial Calibration

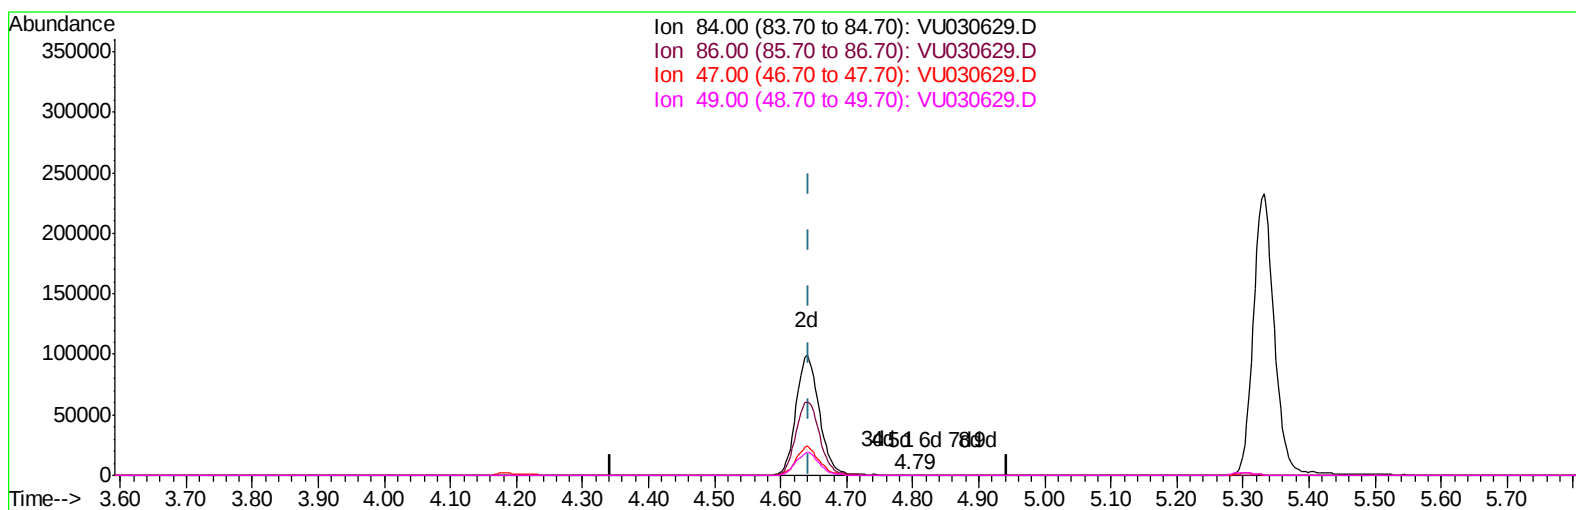

TIC: VU030629.D

(24) Chloroform-d (S)

4.794min (+0.151) 0.02ug/L

response 210

| Ion   | Exp%  | Act%  |
|-------|-------|-------|
| 84.00 | 100   | 100   |
| 86.00 | 62.50 | 50.48 |
| 47.00 | 46.00 | 44.29 |
| 49.00 | 27.30 | 21.43 |